

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030220\
Data File : FF006471.D
Signal(s) : FID2B.ch
Acq On : 02 Mar 2020 15:07
Operator : DD\AJ
Sample : PB127206BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 03 00:51:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.590	1466226	12.035 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.772	414672	2.968 ug/ml
16) N-HEXATRIACONTANE	20.024	172196	1.779 ug/ml
18) N-TETRACONTANE	21.601	267790	3.794 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030220\
Data File : FF006471.D
Signal(s) : FID2B.ch
Acq On : 02 Mar 2020 15:07
Operator : DD\AJ
Sample : PB127206BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 03 00:51:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

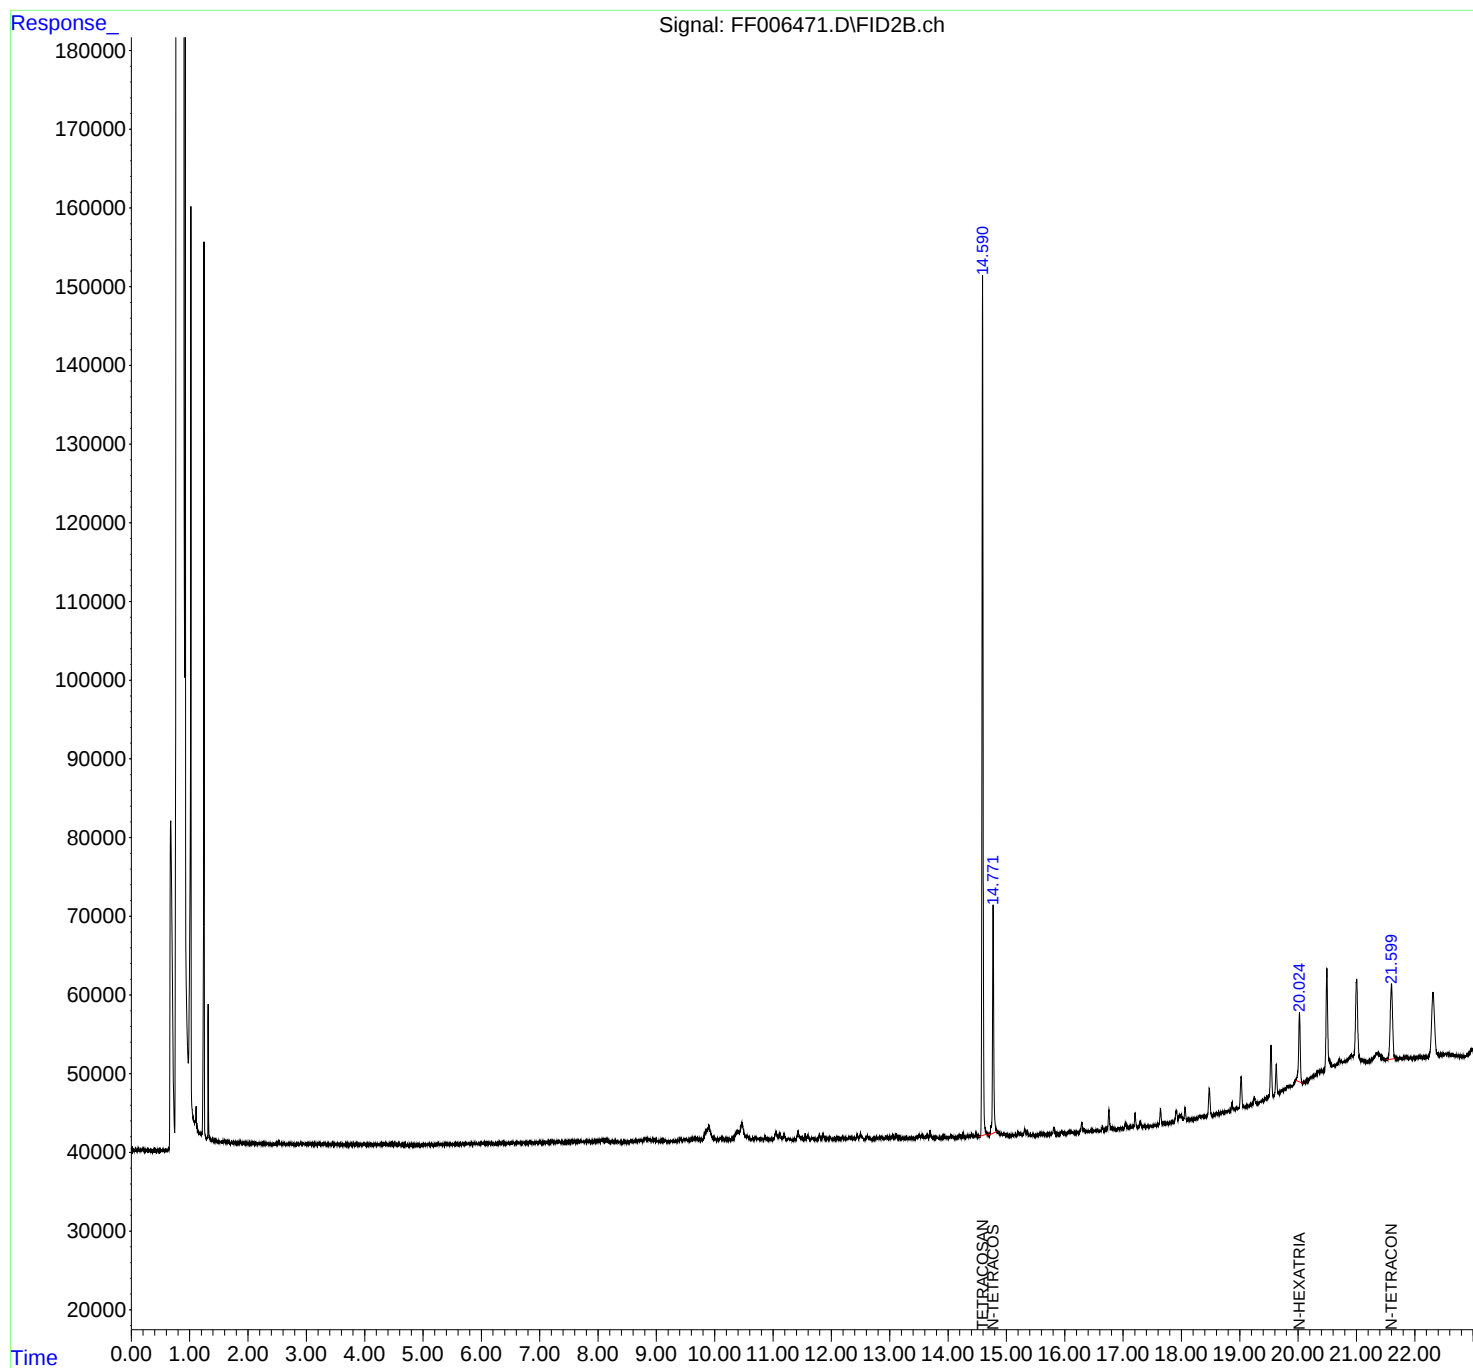


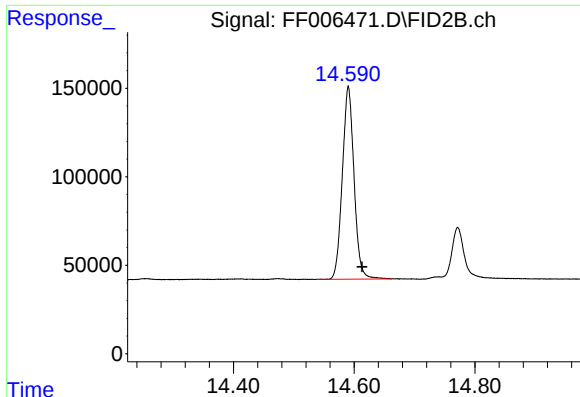

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.590 min
Delta R.T.: -0.023 min
Response: 1466226
Conc: 12.04 ug/ml

Instrument :
FID_F
ClientSampleId :

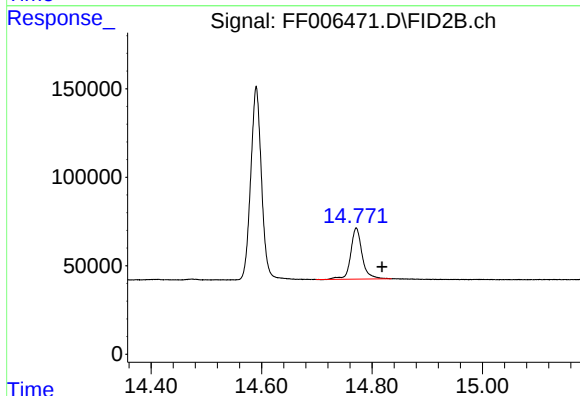


#10 N-TETRACOSANE

R.T.: 14.772 min
Delta R.T.: -0.047 min
Response: 414672
Conc: 2.97 ug/ml

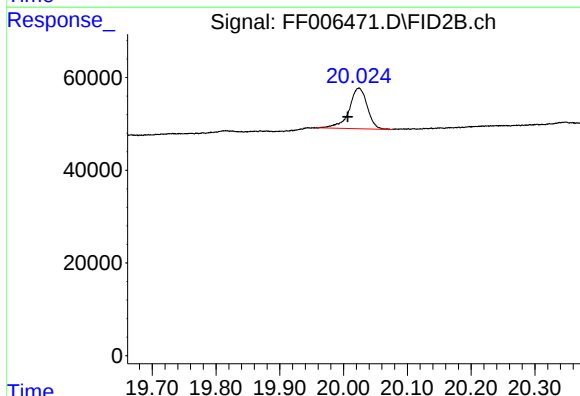

#16 N-HEXATRIACONTANE

R.T.: 20.024 min
Delta R.T.: 0.018 min
Response: 172196
Conc: 1.78 ug/ml

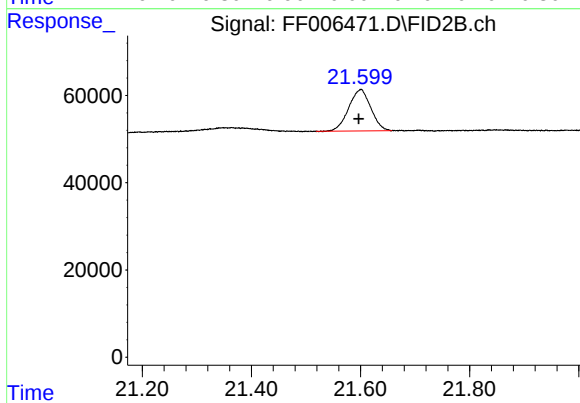

#18 N-TETRACONTANE

R.T.: 21.601 min
Delta R.T.: 0.004 min
Response: 267790
Conc: 3.79 ug/ml