

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF030220\  
 Data File : FF006473.D  
 Signal(s) : FID2B.ch  
 Acq On : 02 Mar 2020 16:08  
 Operator : DD\AJ  
 Sample : L1743-04  
 Misc :  
 ALS Vial : 57 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Mar 03 00:51:45 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF021020.M  
 Quant Title :  
 QLast Update : Tue Feb 11 10:27:03 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.593 | 1674290  | 13.743 ug/ml |
| Target Compounds              |        |          |              |
| 4) N-TETRADECANE              | 8.227  | 256094   | 1.862 ug/ml  |
| 7) N-EICOSANE                 | 12.514 | 167492   | 1.188 ug/ml  |
| 10) N-TETRACOSANE             | 14.817 | 38752    | 0.277 ug/ml  |
| 12) N-OCTACOSANE              | 16.757 | 100186   | 0.726 ug/ml  |
| 13) N-TRIACONTANE             | 17.639 | 162521   | 1.175 ug/ml  |
| 14) N-DOTRIACONTANE           | 18.468 | 127352   | 0.968 ug/ml  |
| 18) N-TETRACONTANE            | 21.574 | 171622   | 2.431 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF030220\  
Data File : FF006473.D  
Signal(s) : FID2B.ch  
Acq On : 02 Mar 2020 16:08  
Operator : DD\AJ  
Sample : L1743-04  
Misc :  
ALS Vial : 57 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Mar 03 00:51:45 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF021020.M  
Quant Title :  
QLast Update : Tue Feb 11 10:27:03 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

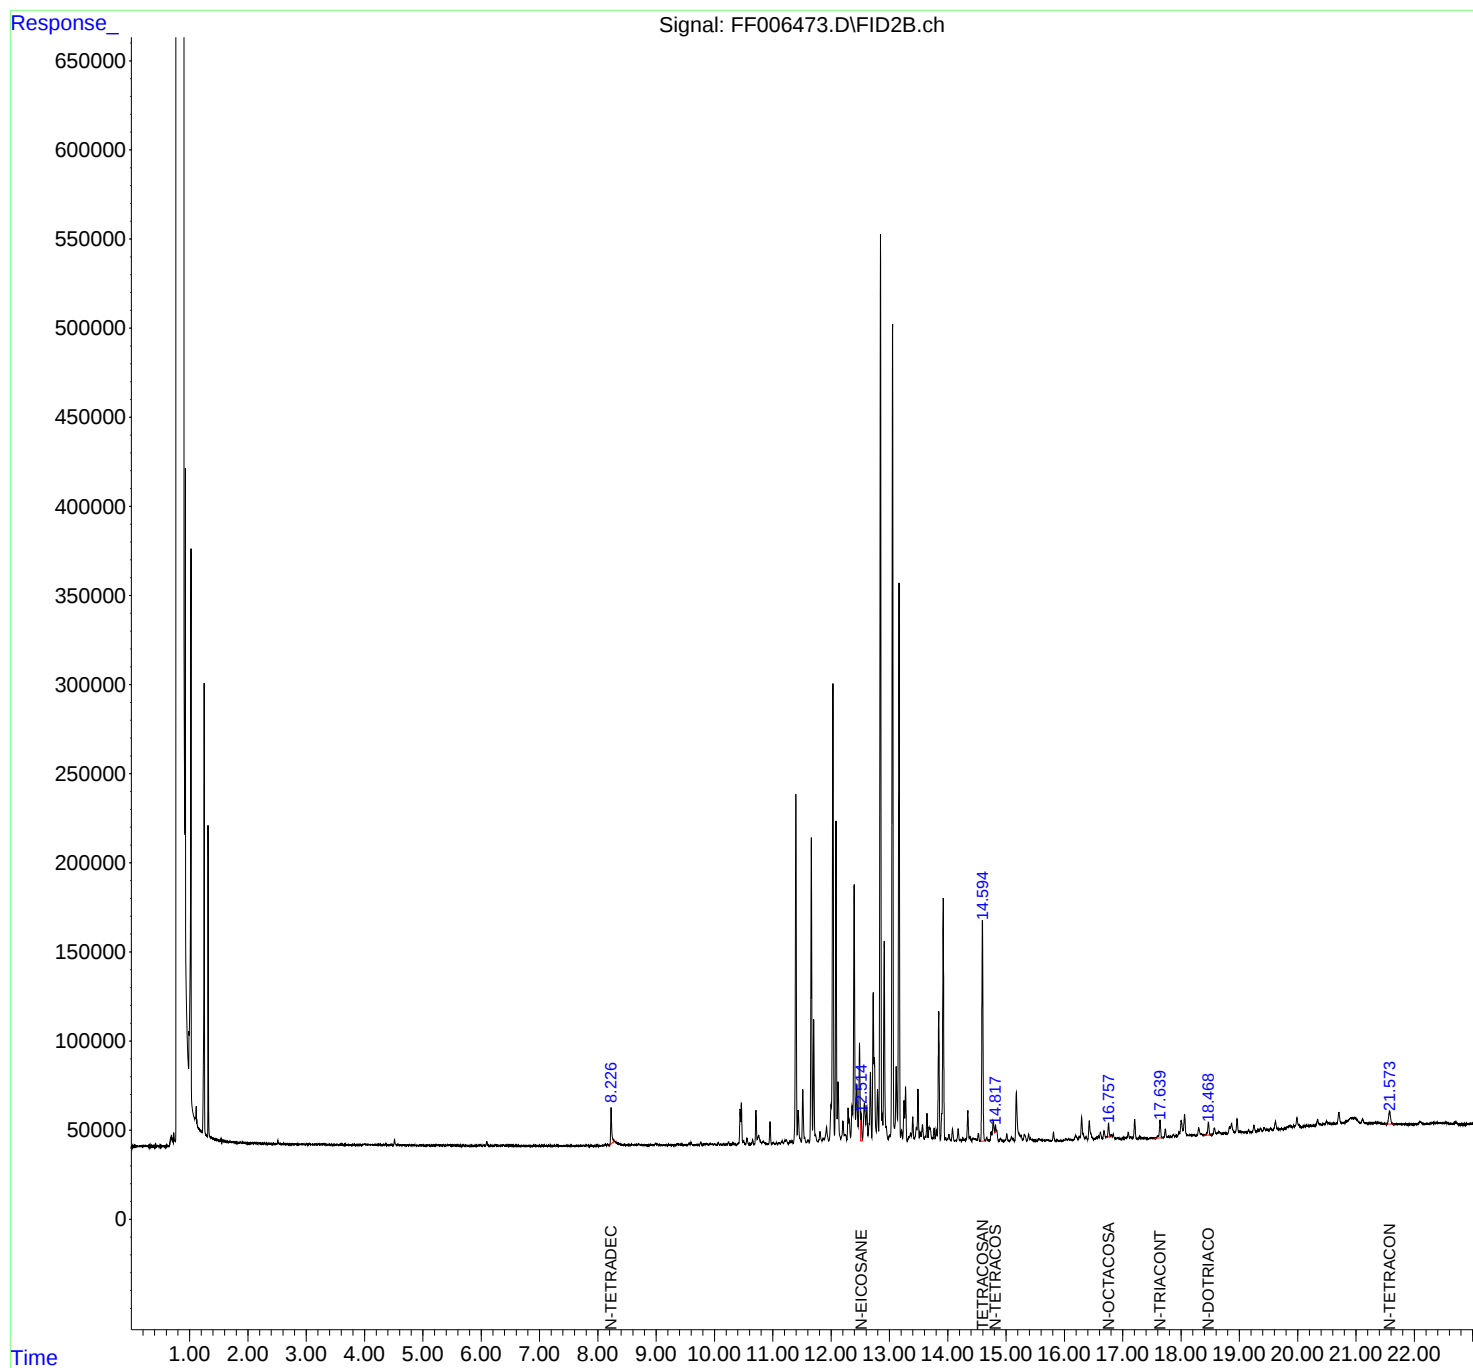


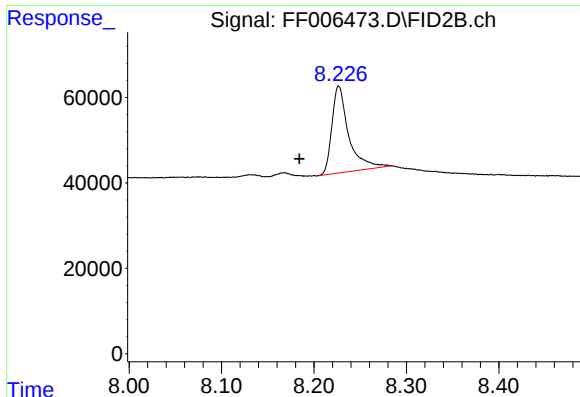

#4 N-TETRADECANE


R.T.: 8.227 min  
Delta R.T.: 0.042 min  
Response: 256094  
Conc: 1.86 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

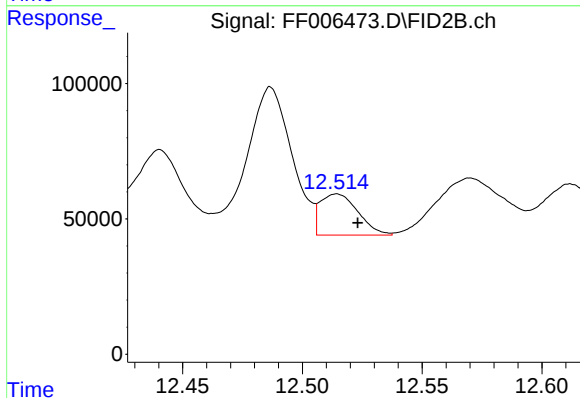


#7 N-EICOSANE

R.T.: 12.514 min  
Delta R.T.: -0.009 min  
Response: 167492  
Conc: 1.19 ug/ml

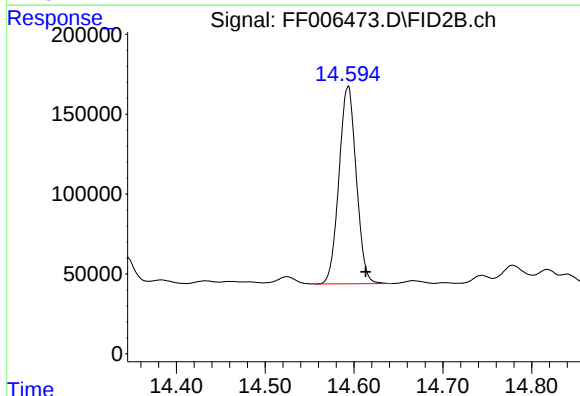


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.593 min  
Delta R.T.: -0.020 min  
Response: 1674290  
Conc: 13.74 ug/ml

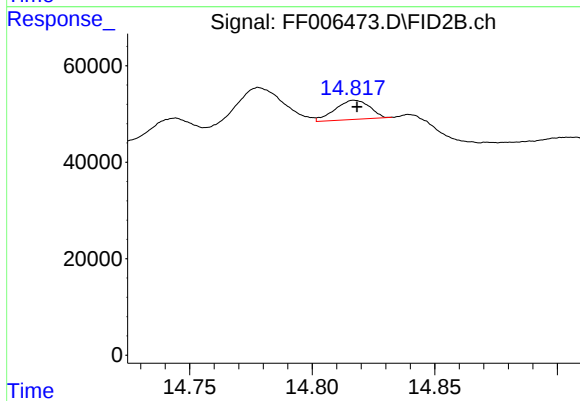

#10 N-TETRACOSANE


R.T.: 14.817 min  
Delta R.T.: 0.000 min  
Response: 38752  
Conc: 0.28 ug/ml

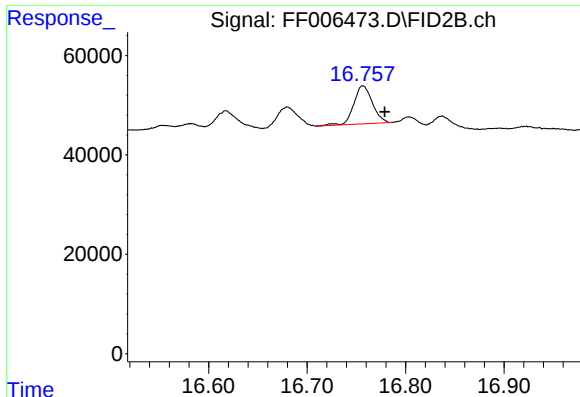

#12 N-OCTACOSANE


R.T.: 16.757 min  
Delta R.T.: -0.022 min  
Response: 100186  
Conc: 0.73 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

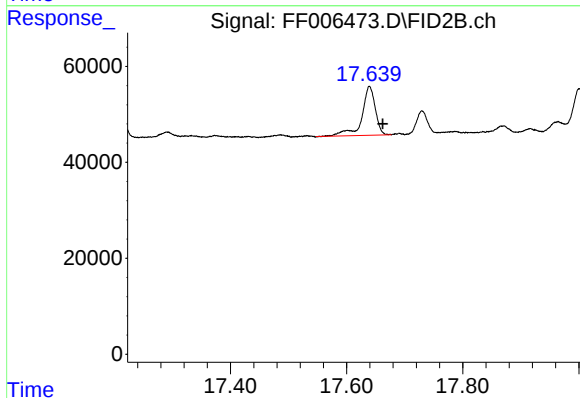


#13 N-TRIACONTANE

R.T.: 17.639 min  
Delta R.T.: -0.023 min  
Response: 162521  
Conc: 1.18 ug/ml

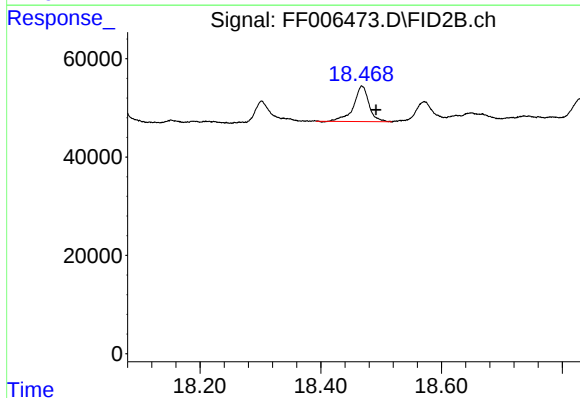

#14 N-DOTRIACONTANE

R.T.: 18.468 min  
Delta R.T.: -0.023 min  
Response: 127352  
Conc: 0.97 ug/ml

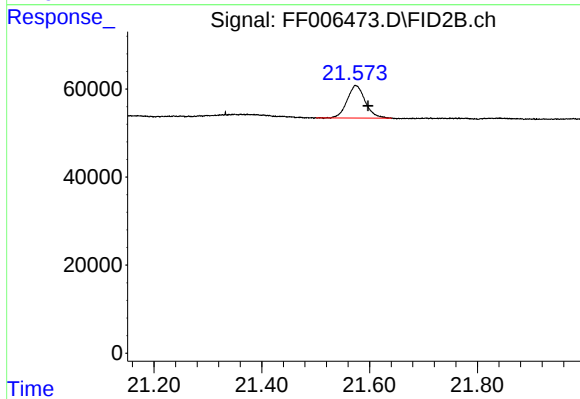

#18 N-TETRACONTANE

R.T.: 21.574 min  
Delta R.T.: -0.023 min  
Response: 171622  
Conc: 2.43 ug/ml