

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030220\
 Data File : FF006476.D
 Signal(s) : FID2B.ch
 Acq On : 02 Mar 2020 17:39
 Operator : DD\AJ
 Sample : L1743-10
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 03 00:52:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.594	2065352	16.953 ug/ml
Target Compounds			
4) N-TETRADECANE	8.227	437535	3.181 ug/ml
7) N-EICOSANE	12.565	479850	3.405 ug/ml
8) N-DOCOSANE	13.710	126295	0.899 ug/ml
10) N-TETRACOSANE	14.778	311023	2.226 ug/ml
11) N-HEXACOSANE	15.811	94157	0.682 ug/ml
12) N-OCTACOSANE	16.758	235429	1.706 ug/ml
13) N-TRIACONTANE	17.642	248952	1.800 ug/ml
14) N-DOTRIACONTANE	18.468	266585	2.026 ug/ml
15) N-TETRATRIACONTANE	19.248	83260	0.741 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030220\
Data File : FF006476.D
Signal(s) : FID2B.ch
Acq On : 02 Mar 2020 17:39
Operator : DD\AJ
Sample : L1743-10
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 03 00:52:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

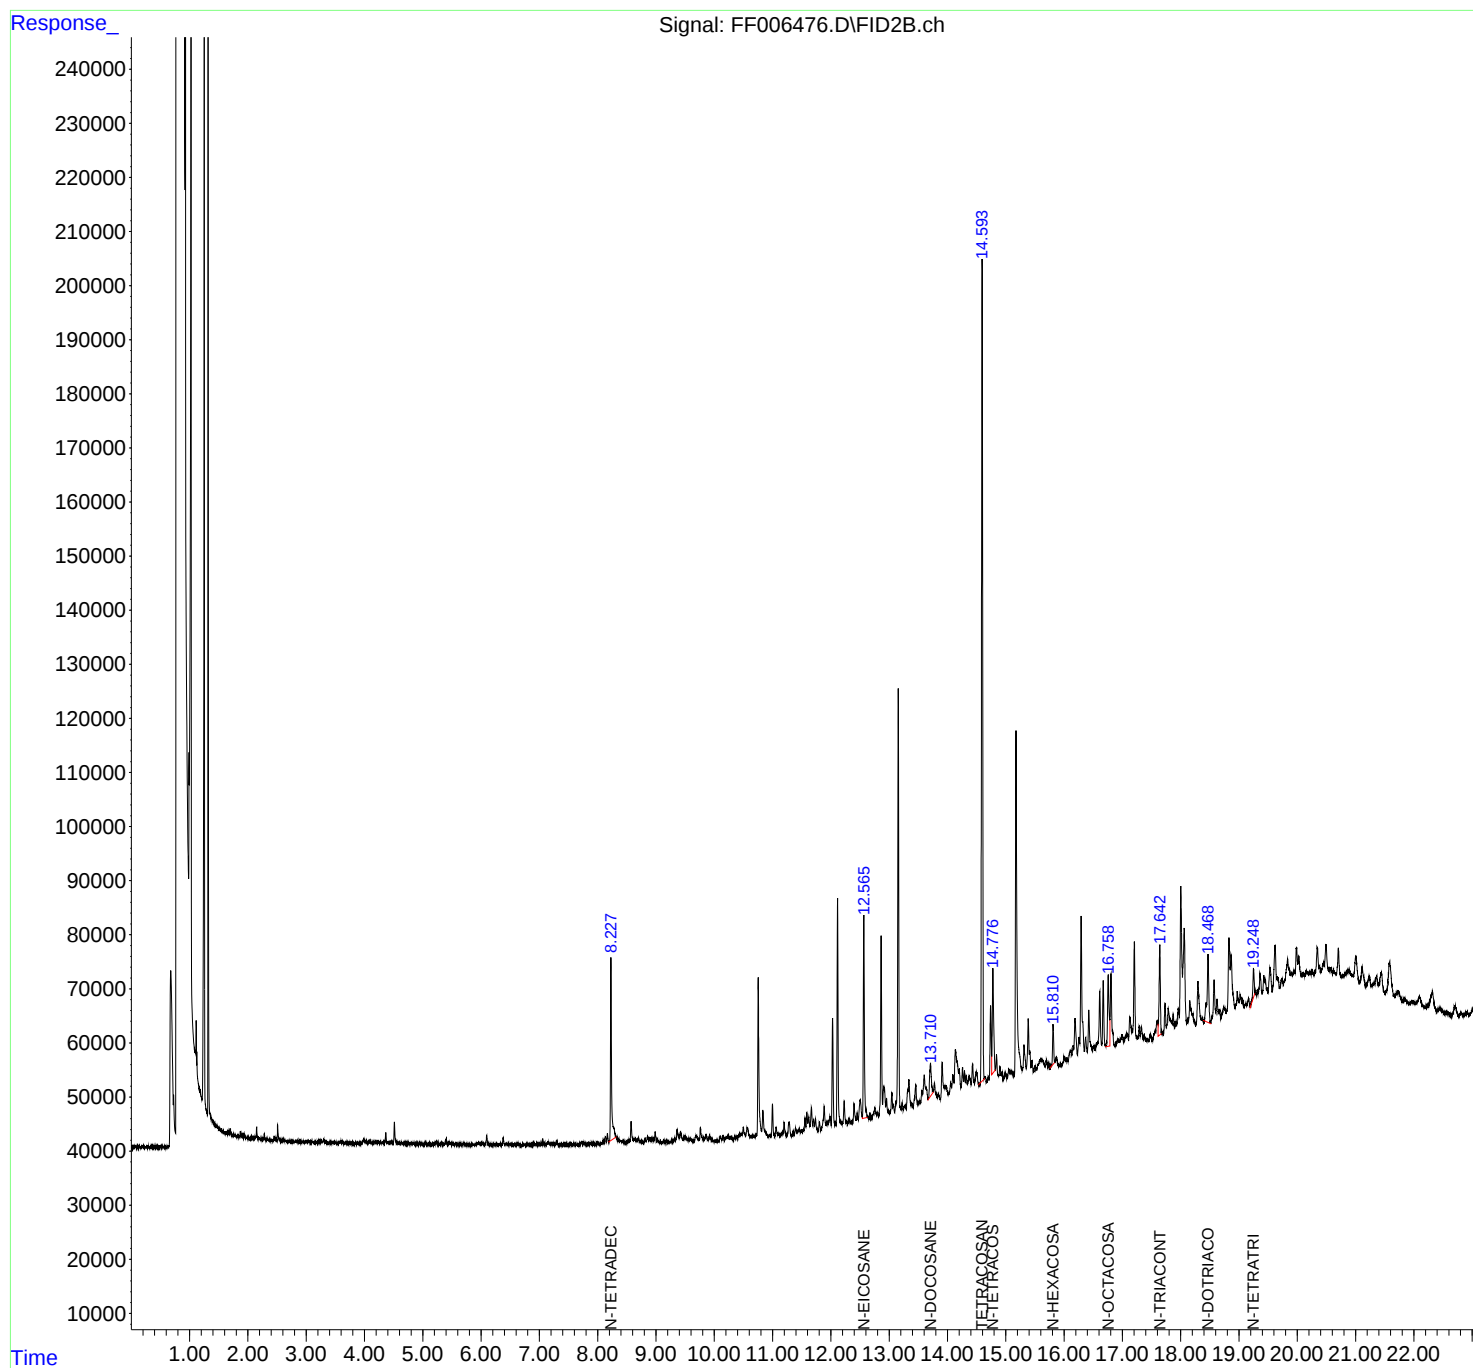


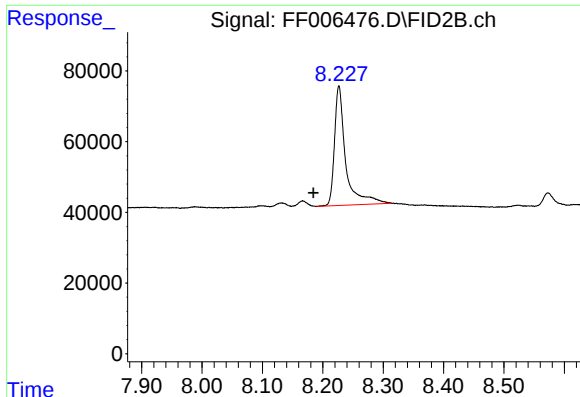

#4 N-TETRADECANE


R.T.: 8.227 min
Delta R.T.: 0.042 min
Response: 437535
Conc: 3.18 ug/ml

Instrument :
FID_F
ClientSampleId :

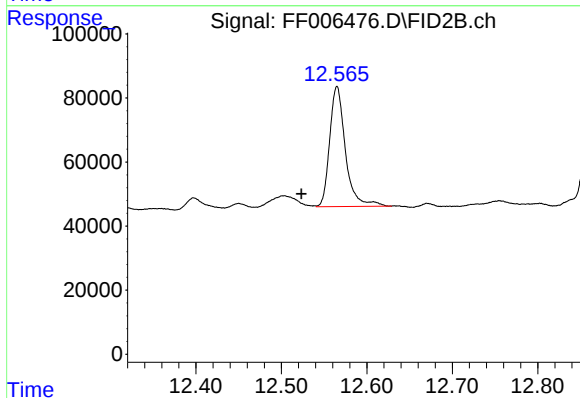


#7 N-EICOSANE

R.T.: 12.565 min
Delta R.T.: 0.042 min
Response: 479850
Conc: 3.40 ug/ml

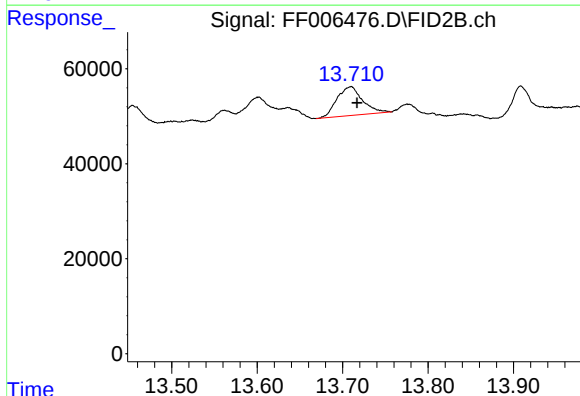


#8 N-DOCOSANE

R.T.: 13.710 min
Delta R.T.: -0.007 min
Response: 126295
Conc: 0.90 ug/ml

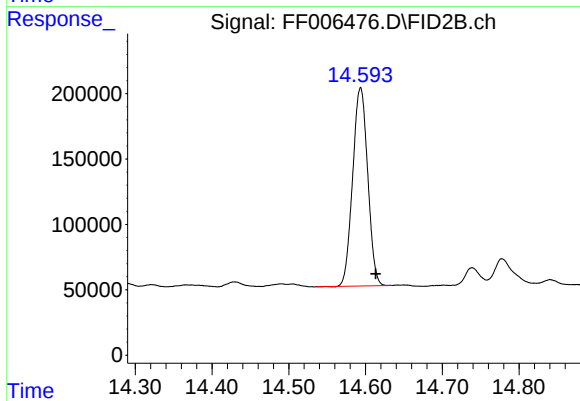

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.594 min
Delta R.T.: -0.020 min
Response: 2065352
Conc: 16.95 ug/ml

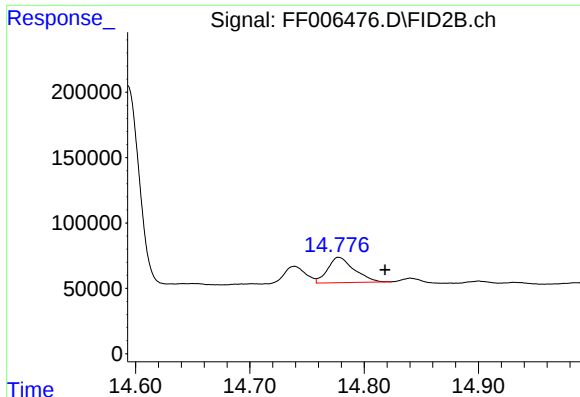

#10 N-TETRACOSANE


R.T.: 14.778 min
Delta R.T.: -0.040 min
Response: 311023
Conc: 2.23 ug/ml

Instrument :
FID_F
ClientSampleId :

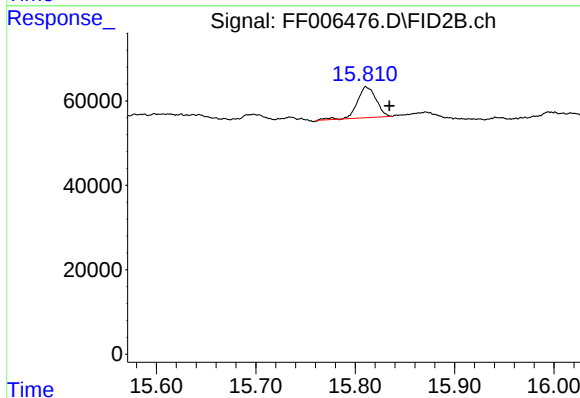


#11 N-HEXACOSANE

R.T.: 15.811 min
Delta R.T.: -0.023 min
Response: 94157
Conc: 0.68 ug/ml

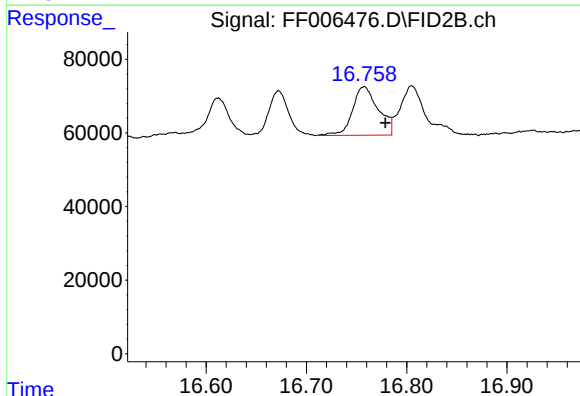


#12 N-OCTACOSANE

R.T.: 16.758 min
Delta R.T.: -0.021 min
Response: 235429
Conc: 1.71 ug/ml

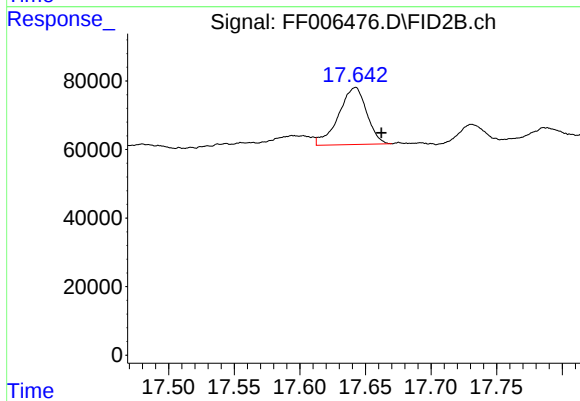

#13 N-TRIACONTANE


R.T.: 17.642 min
Delta R.T.: -0.020 min
Response: 248952
Conc: 1.80 ug/ml

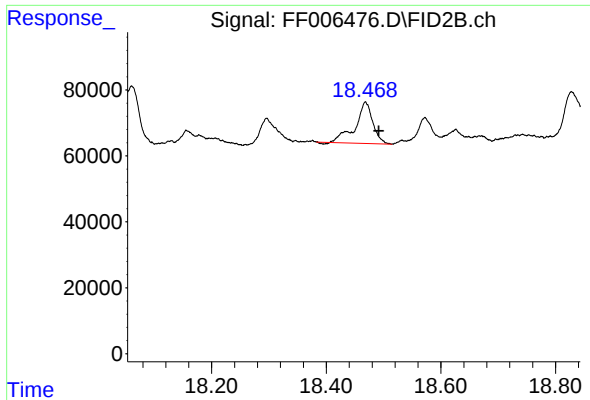

#14 N-DOTRIACONTANE

R.T.: 18.468 min
Delta R.T.: -0.023 min
Response: 266585
Conc: 2.03 ug/ml

Instrument :
FID_F
ClientSampleId :

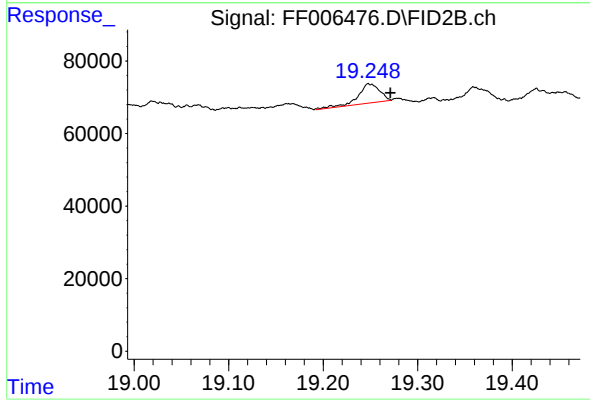

#15 N-TETRATRIACONTANE

R.T.: 19.248 min
Delta R.T.: -0.023 min
Response: 83260
Conc: 0.74 ug/ml