

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030220\
 Data File : FF006478.D
 Signal(s) : FID2B.ch
 Acq On : 02 Mar 2020 18:40
 Operator : DD\AJ
 Sample : L1743-16
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 03 00:52:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.594	2216716	18.195 ug/ml
Target Compounds			
4) N-TETRADECANE	8.226	432329	3.143 ug/ml
7) N-EICOSANE	12.567	140922	1.000 ug/ml
10) N-TETRACOSANE	14.778	210822	1.509 ug/ml
11) N-HEXACOSANE	15.812	119835	0.868 ug/ml
12) N-OCTACOSANE	16.758	164306	1.191 ug/ml
13) N-TRIACONTANE	17.642	321547	2.325 ug/ml
14) N-DOTRIACONTANE	18.466	287886	2.188 ug/ml
16) N-HEXATRIACONTANE	20.000	511760	5.288 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030220\
Data File : FF006478.D
Signal(s) : FID2B.ch
Acq On : 02 Mar 2020 18:40
Operator : DD\AJ
Sample : L1743-16
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 03 00:52:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

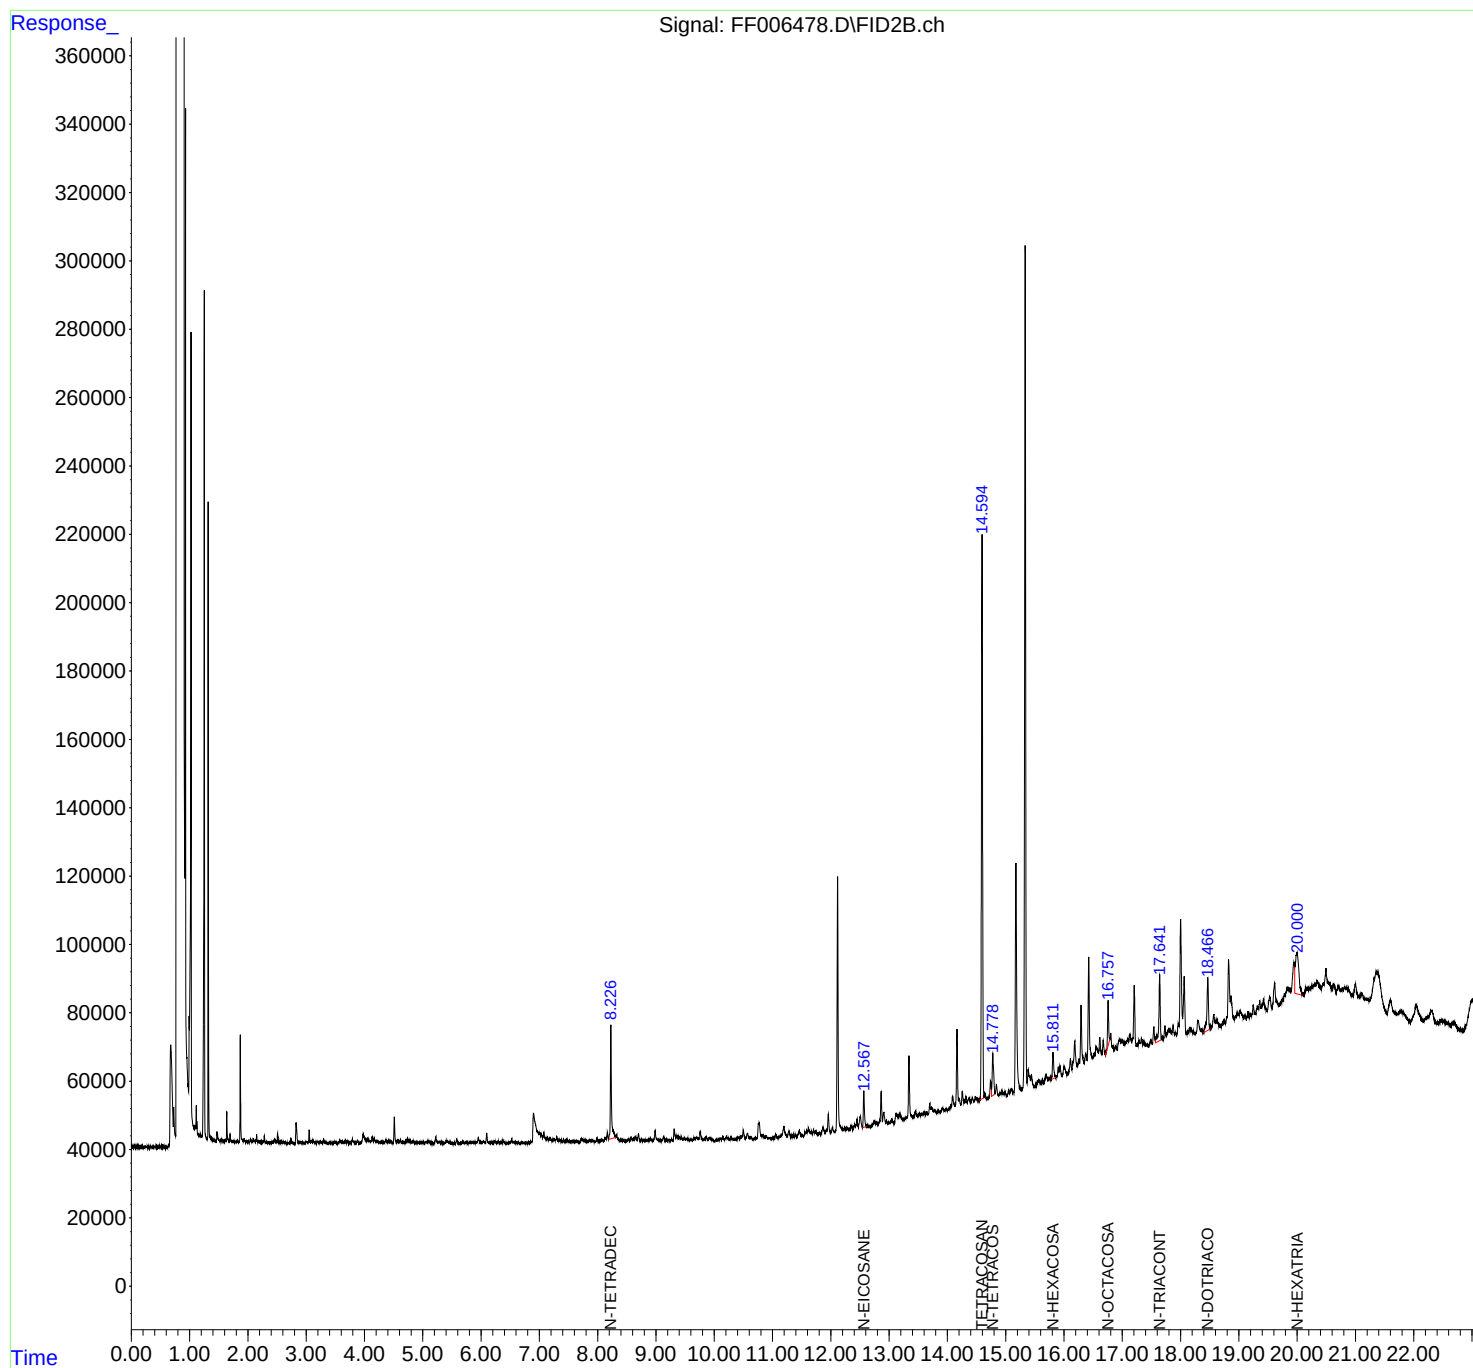


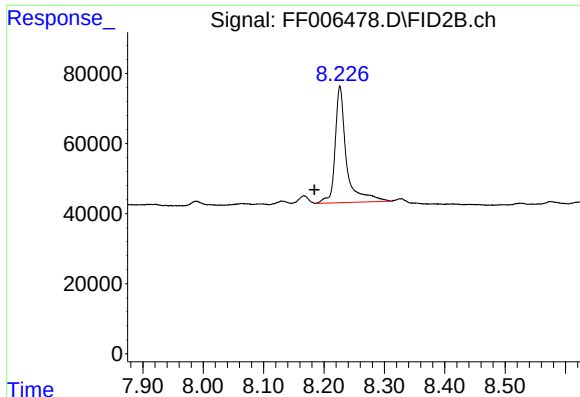

#4 N-TETRADECANE


R.T.: 8.226 min
Delta R.T.: 0.042 min
Response: 432329
Conc: 3.14 ug/ml

Instrument :
FID_F
ClientSampleId :

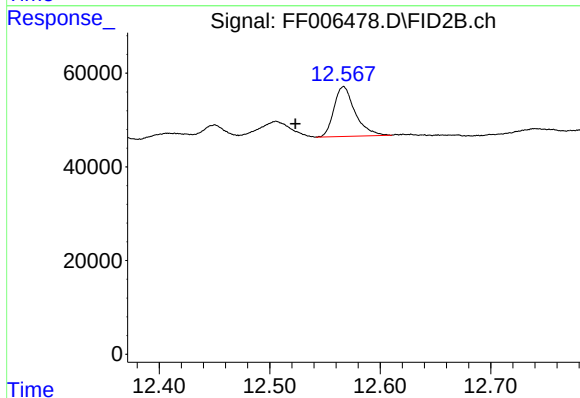


#7 N-EICOSANE

R.T.: 12.567 min
Delta R.T.: 0.044 min
Response: 140922
Conc: 1.00 ug/ml

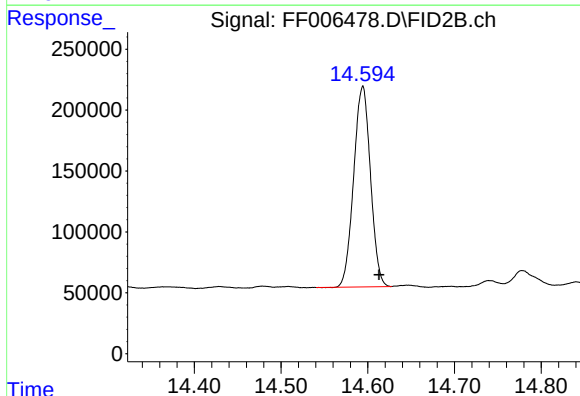


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.594 min
Delta R.T.: -0.019 min
Response: 2216716
Conc: 18.20 ug/ml

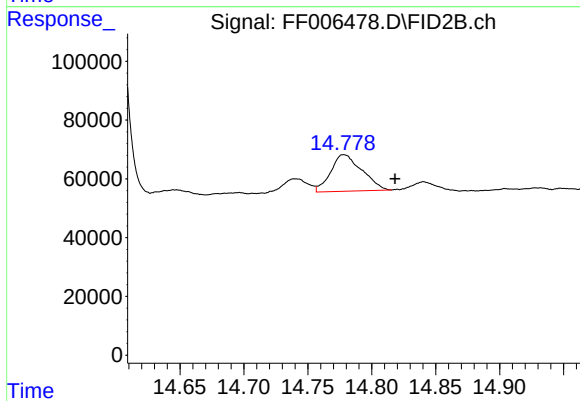

#10 N-TETRACOSANE


R.T.: 14.778 min
Delta R.T.: -0.040 min
Response: 210822
Conc: 1.51 ug/ml

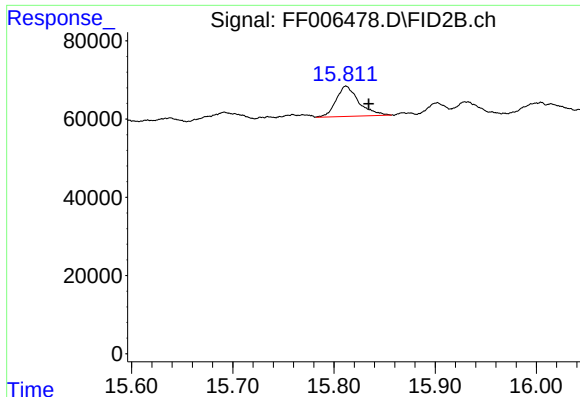

#11 N-HEXACOSANE


R.T.: 15.812 min
Delta R.T.: -0.022 min
Response: 119835
Conc: 0.87 ug/ml

Instrument :
FID_F
ClientSampleId :

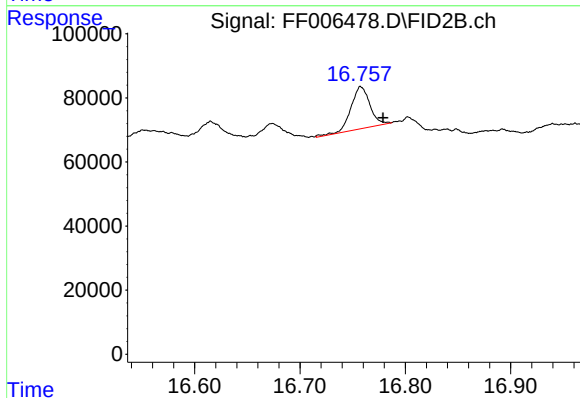


#12 N-OCTACOSANE

R.T.: 16.758 min
Delta R.T.: -0.021 min
Response: 164306
Conc: 1.19 ug/ml

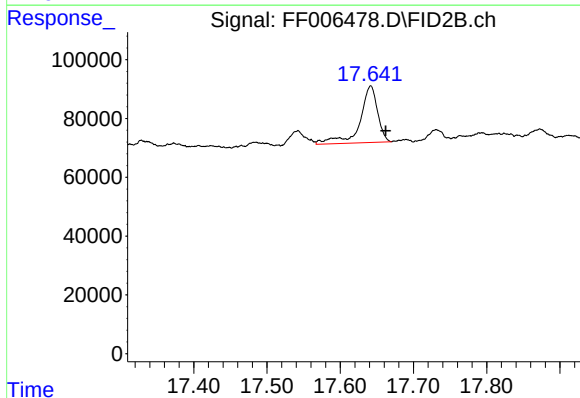


#13 N-TRIACONTANE

R.T.: 17.642 min
Delta R.T.: -0.021 min
Response: 321547
Conc: 2.33 ug/ml

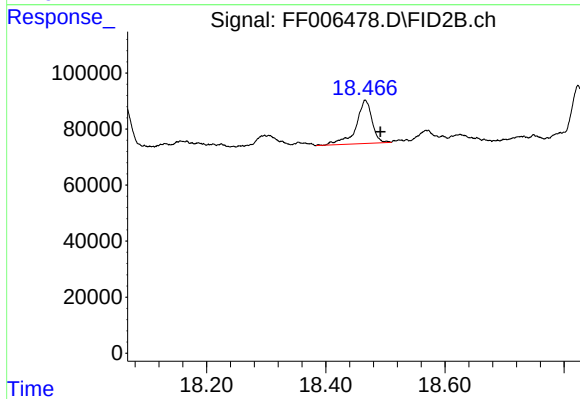

#14 N-DOTRIACONTANE

R.T.: 18.466 min
Delta R.T.: -0.025 min
Response: 287886
Conc: 2.19 ug/ml

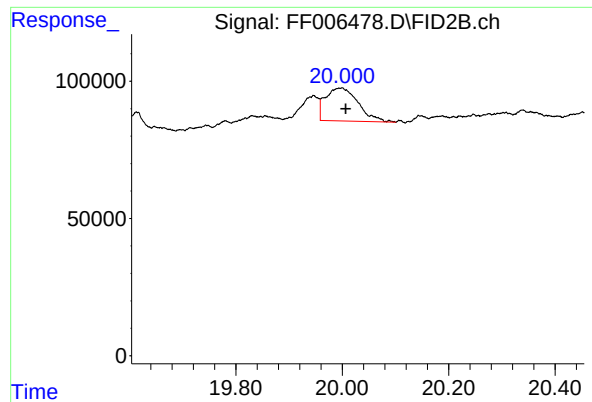

#16 N-HEXATRIACONTANE

R.T.: 20.000 min
Delta R.T.: -0.007 min
Response: 511760
Conc: 5.29 ug/ml

Instrument :
FID_F
ClientSampleId :