

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030220\
 Data File : FF006479.D
 Signal(s) : FID2B.ch
 Acq On : 02 Mar 2020 19:11
 Operator : DD\AJ
 Sample : L1743-18
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 03 00:52:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.595	2577933	21.160 ug/ml
Target Compounds			
4) N-TETRADECANE	8.226	315014	2.290 ug/ml
7) N-EICOSANE	12.566	359640	2.552 ug/ml
10) N-TETRACOSANE	14.778	332403	2.379 ug/ml
11) N-HEXACOSANE	15.815	108132	0.783 ug/ml
12) N-OCTACOSANE	16.758	271231	1.965 ug/ml
13) N-TRIACONTANE	17.641	357259	2.583 ug/ml
14) N-DOTRIACONTANE	18.464	296555	2.254 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030220\
Data File : FF006479.D
Signal(s) : FID2B.ch
Acq On : 02 Mar 2020 19:11
Operator : DD\AJ
Sample : L1743-18
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 03 00:52:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

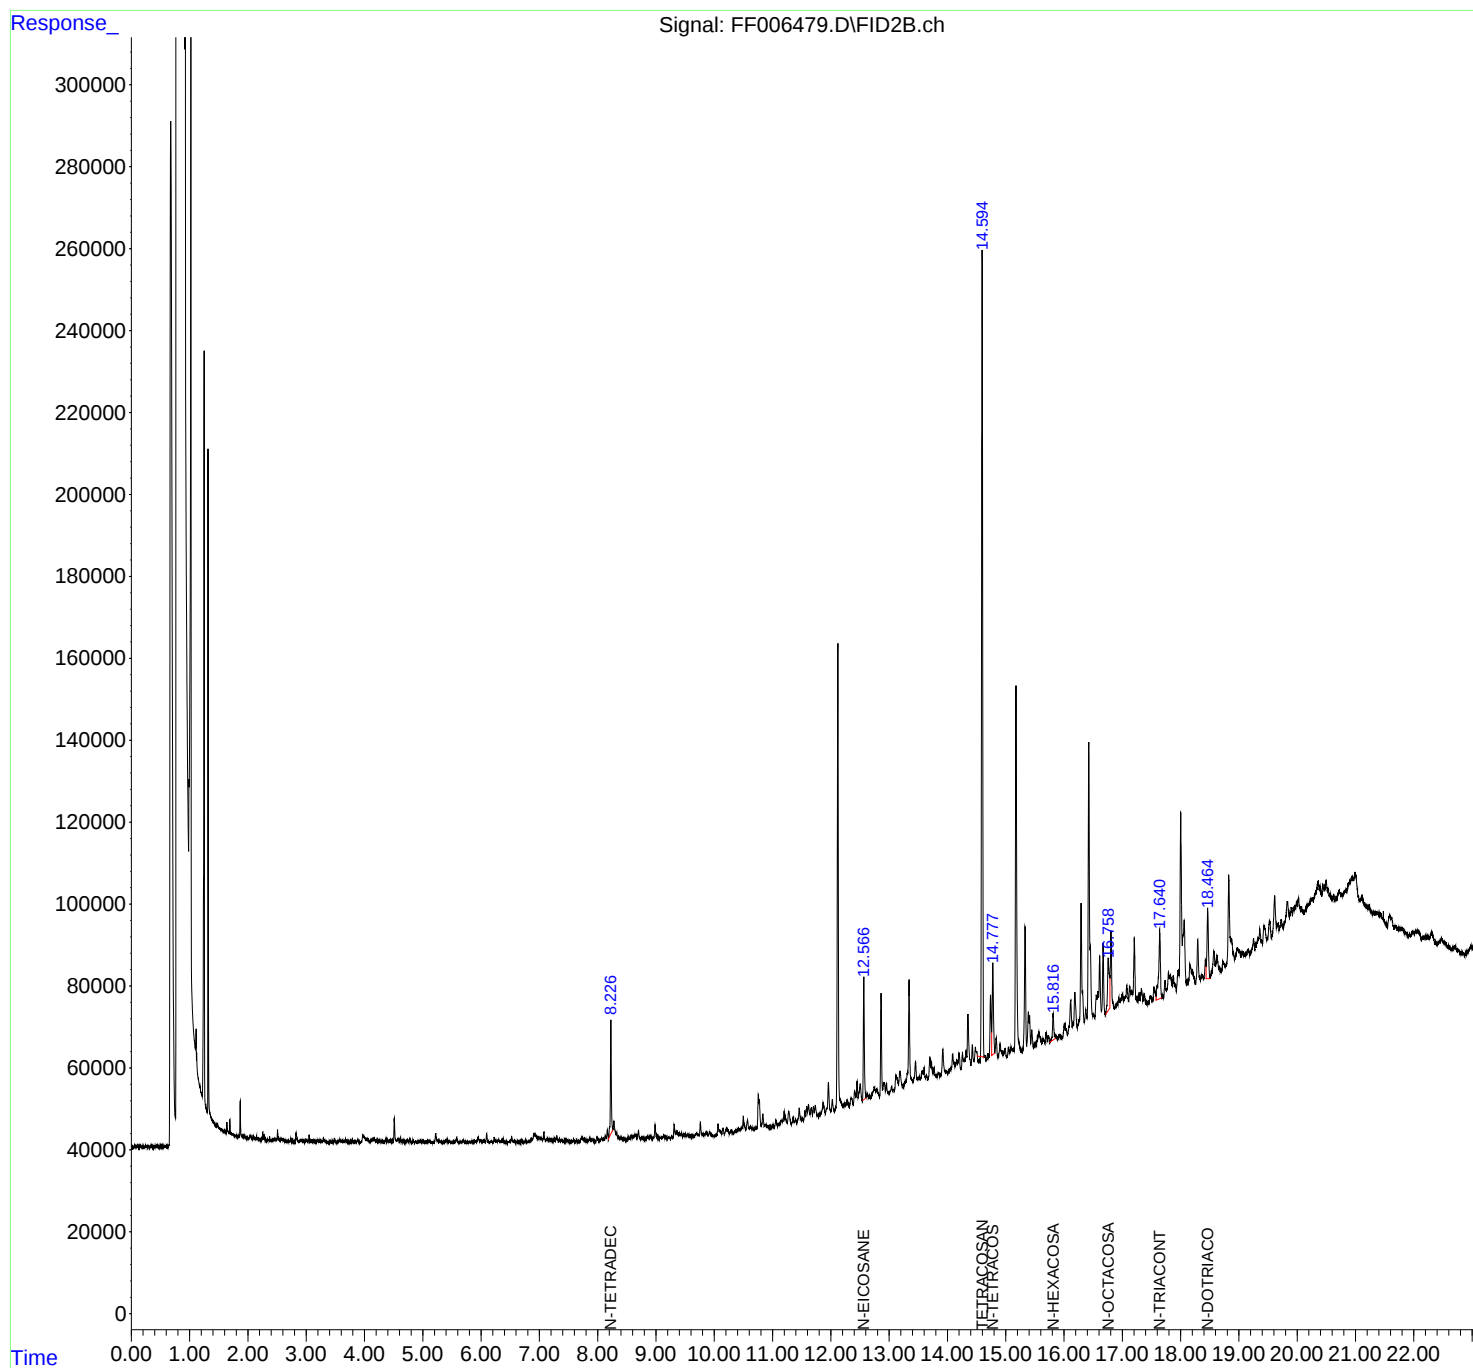


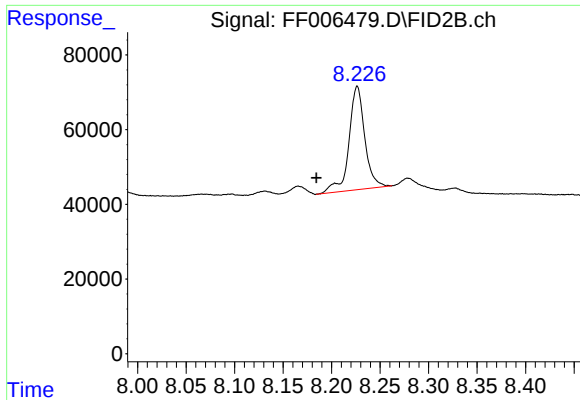

#4 N-TETRADECANE


R.T.: 8.226 min
Delta R.T.: 0.042 min
Response: 315014
Conc: 2.29 ug/ml

Instrument :
FID_F
ClientSampleId :

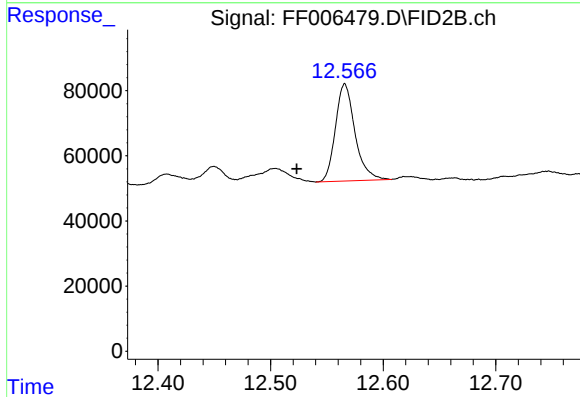


#7 N-EICOSANE

R.T.: 12.566 min
Delta R.T.: 0.043 min
Response: 359640
Conc: 2.55 ug/ml

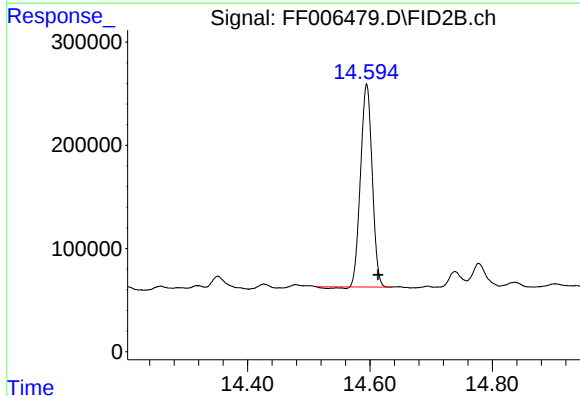


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.595 min
Delta R.T.: -0.018 min
Response: 2577933
Conc: 21.16 ug/ml

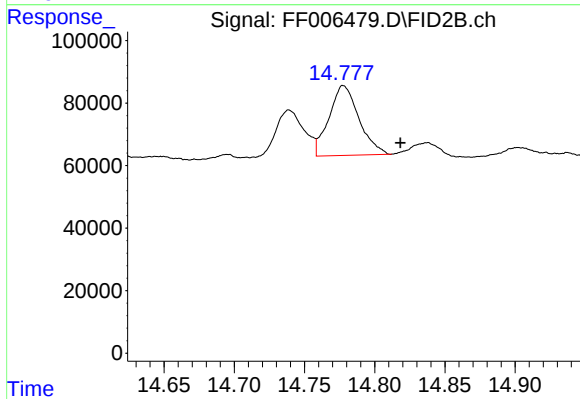

#10 N-TETRACOSANE


R.T.: 14.778 min
Delta R.T.: -0.040 min
Response: 332403
Conc: 2.38 ug/ml

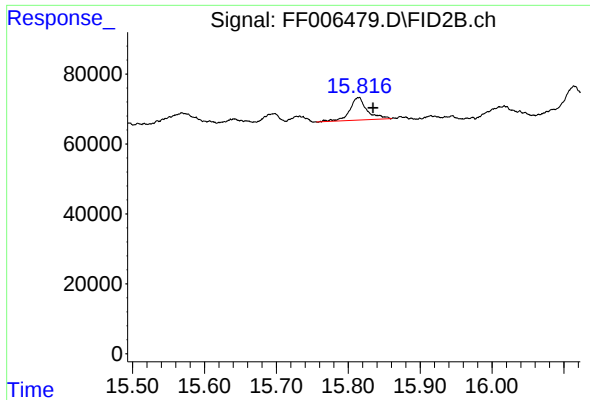

#11 N-HEXACOSANE


R.T.: 15.815 min
Delta R.T.: -0.020 min
Response: 108132
Conc: 0.78 ug/ml

Instrument :
FID_F
ClientSampleId :

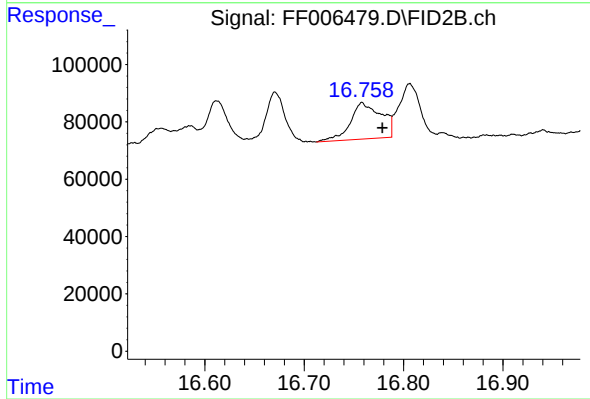


#12 N-OCTACOSANE

R.T.: 16.758 min
Delta R.T.: -0.021 min
Response: 271231
Conc: 1.97 ug/ml

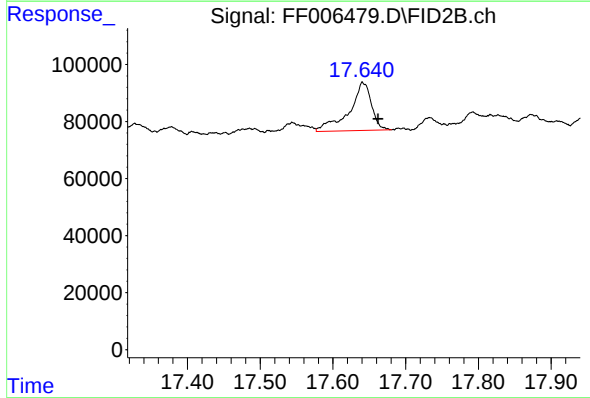

#13 N-TRIACONTANE

R.T.: 17.641 min
Delta R.T.: -0.021 min
Response: 357259
Conc: 2.58 ug/ml

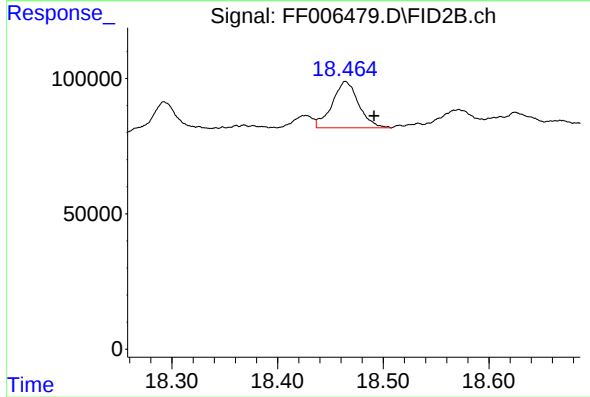

#14 N-DOTRIACONTANE

R.T.: 18.464 min
Delta R.T.: -0.027 min
Response: 296555
Conc: 2.25 ug/ml