

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030220\
Data File : FF006470.D
Signal(s) : FID2B.ch
Acq On : 02 Mar 2020 12:45
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 03 00:51:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.368	3687784	26.983 ug/ml
12) N-OCTACOSANE	16.757	3392448	24.582 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030220\
Data File : FF006470.D
Signal(s) : FID2B.ch
Acq On : 02 Mar 2020 12:45
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 03 00:51:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

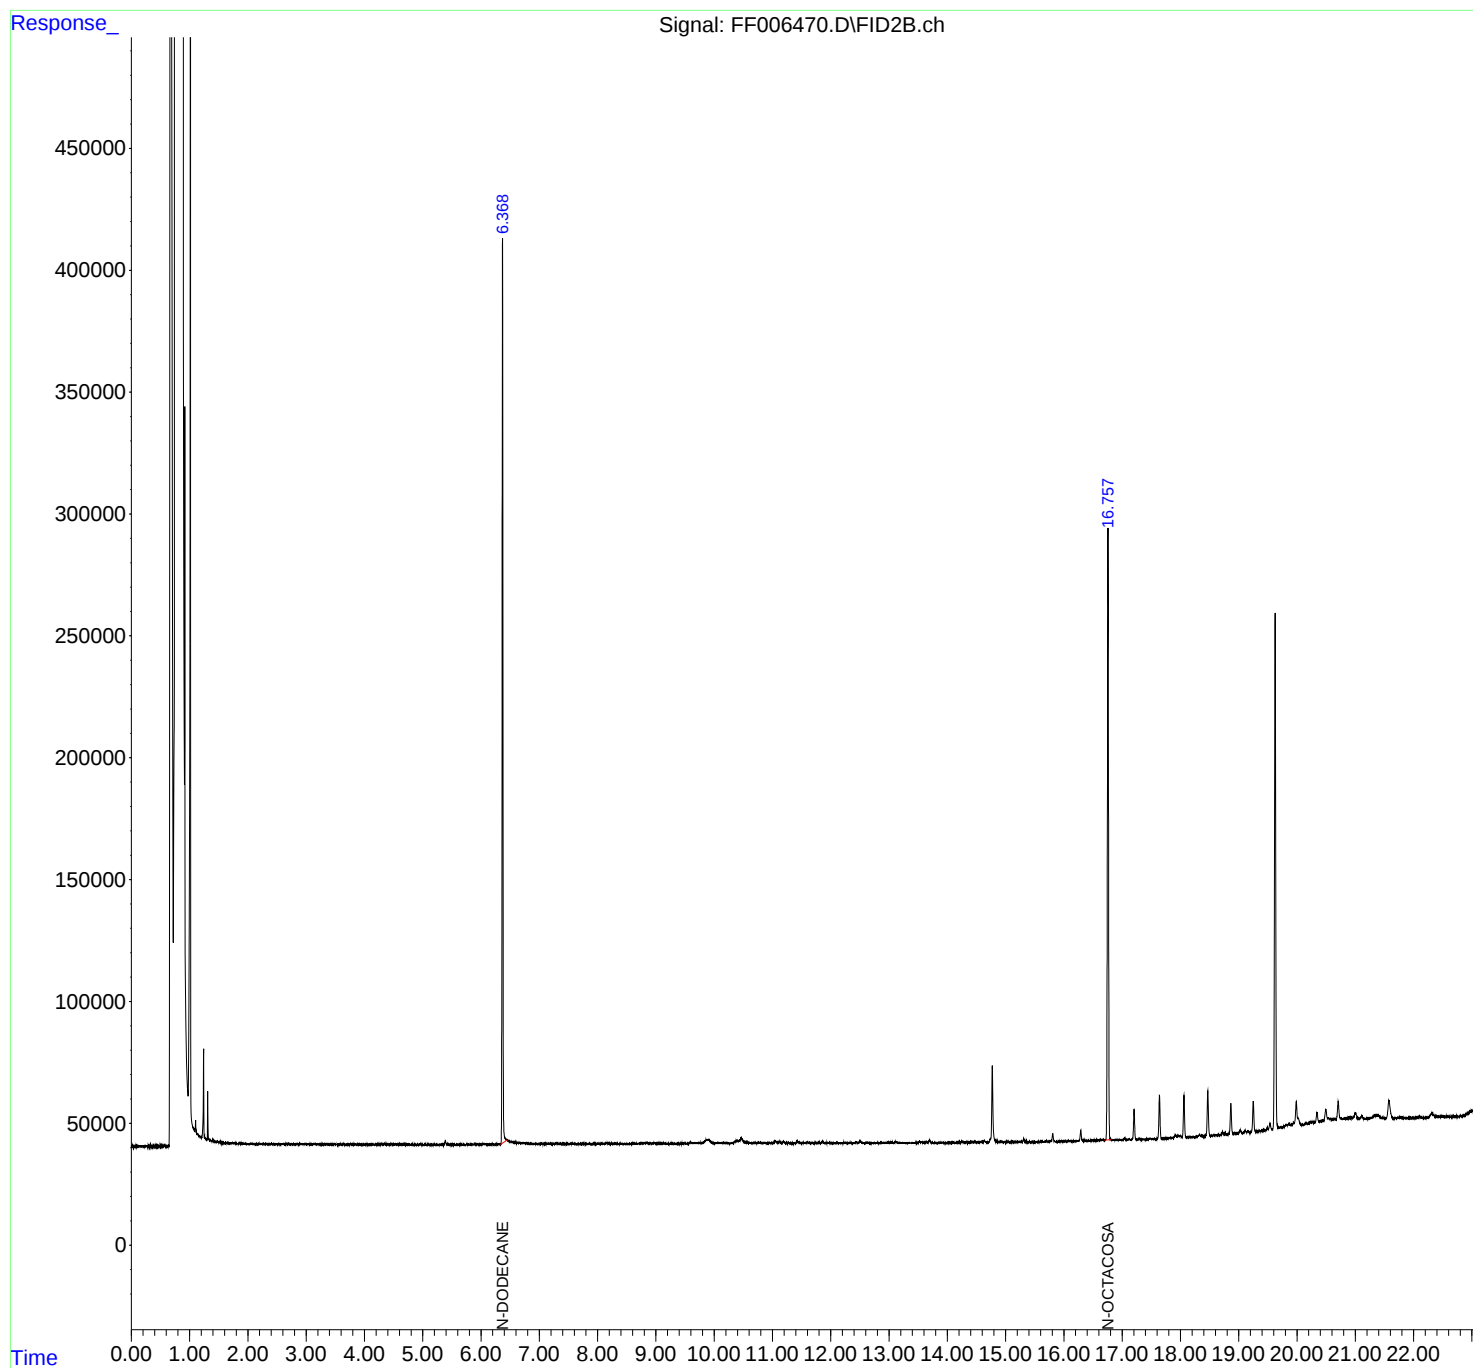


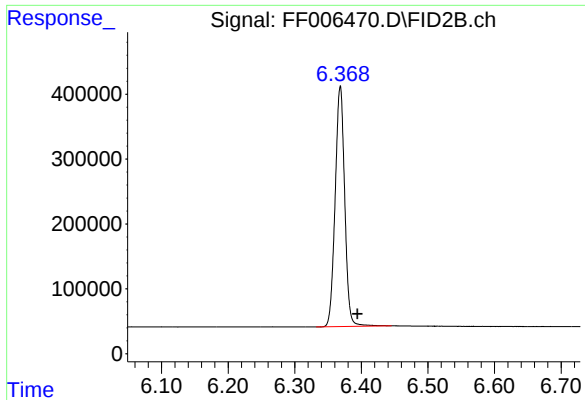

#3 N-DODECANE


R.T.: 6.368 min
Delta R.T.: -0.026 min
Response: 3687784
Conc: 26.98 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

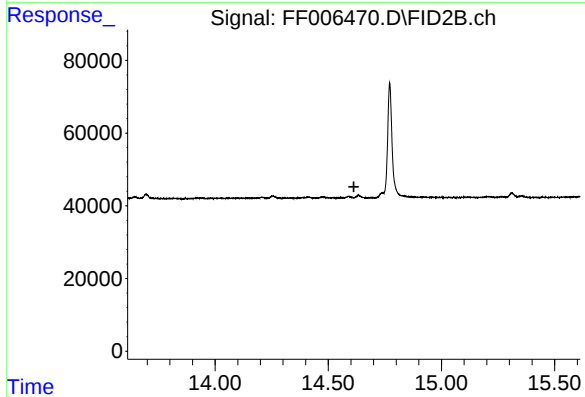

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.613 min
Response: 0
Conc: N.D.

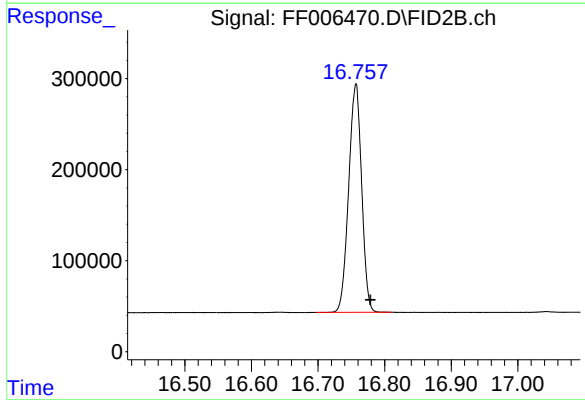

#12 N-OCTACOSANE

R.T.: 16.757 min
Delta R.T.: -0.022 min
Response: 3392448
Conc: 24.58 ug/ml