

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030220\
 Data File : FF006472.D
 Signal(s) : FID2B.ch
 Acq On : 02 Mar 2020 15:37
 Operator : DD\AJ
 Sample : PB127206BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB127206BS

Integration File: autoint1.e
 Quant Time: Mar 03 00:51:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.593	2492570	20.460 ug/ml
Target Compounds			
2) N-DECANE	4.363	3076935	23.040 ug/ml
3) N-DODECANE	6.377	3145406	23.014 ug/ml
4) N-TETRADECANE	8.166	3145263	22.866 ug/ml
5) N-HEXADECANE	9.761	3059911	21.810 ug/ml
6) N-OCTADECANE	11.198	3111800	22.124 ug/ml
7) N-EICOSANE	12.503	2979484	21.141 ug/ml
8) N-DOCOSANE	13.697	2920953	20.784 ug/ml
10) N-TETRACOSANE	14.795	2885401	20.649 ug/ml
11) N-HEXACOSANE	15.813	2759613	19.990 ug/ml
12) N-OCTACOSANE	16.758	2711953	19.651 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030220\
Data File : FF006472.D
Signal(s) : FID2B.ch
Acq On : 02 Mar 2020 15:37
Operator : DD\AJ
Sample : PB127206BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB127206BS

Integration File: autoint1.e
Quant Time: Mar 03 00:51:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

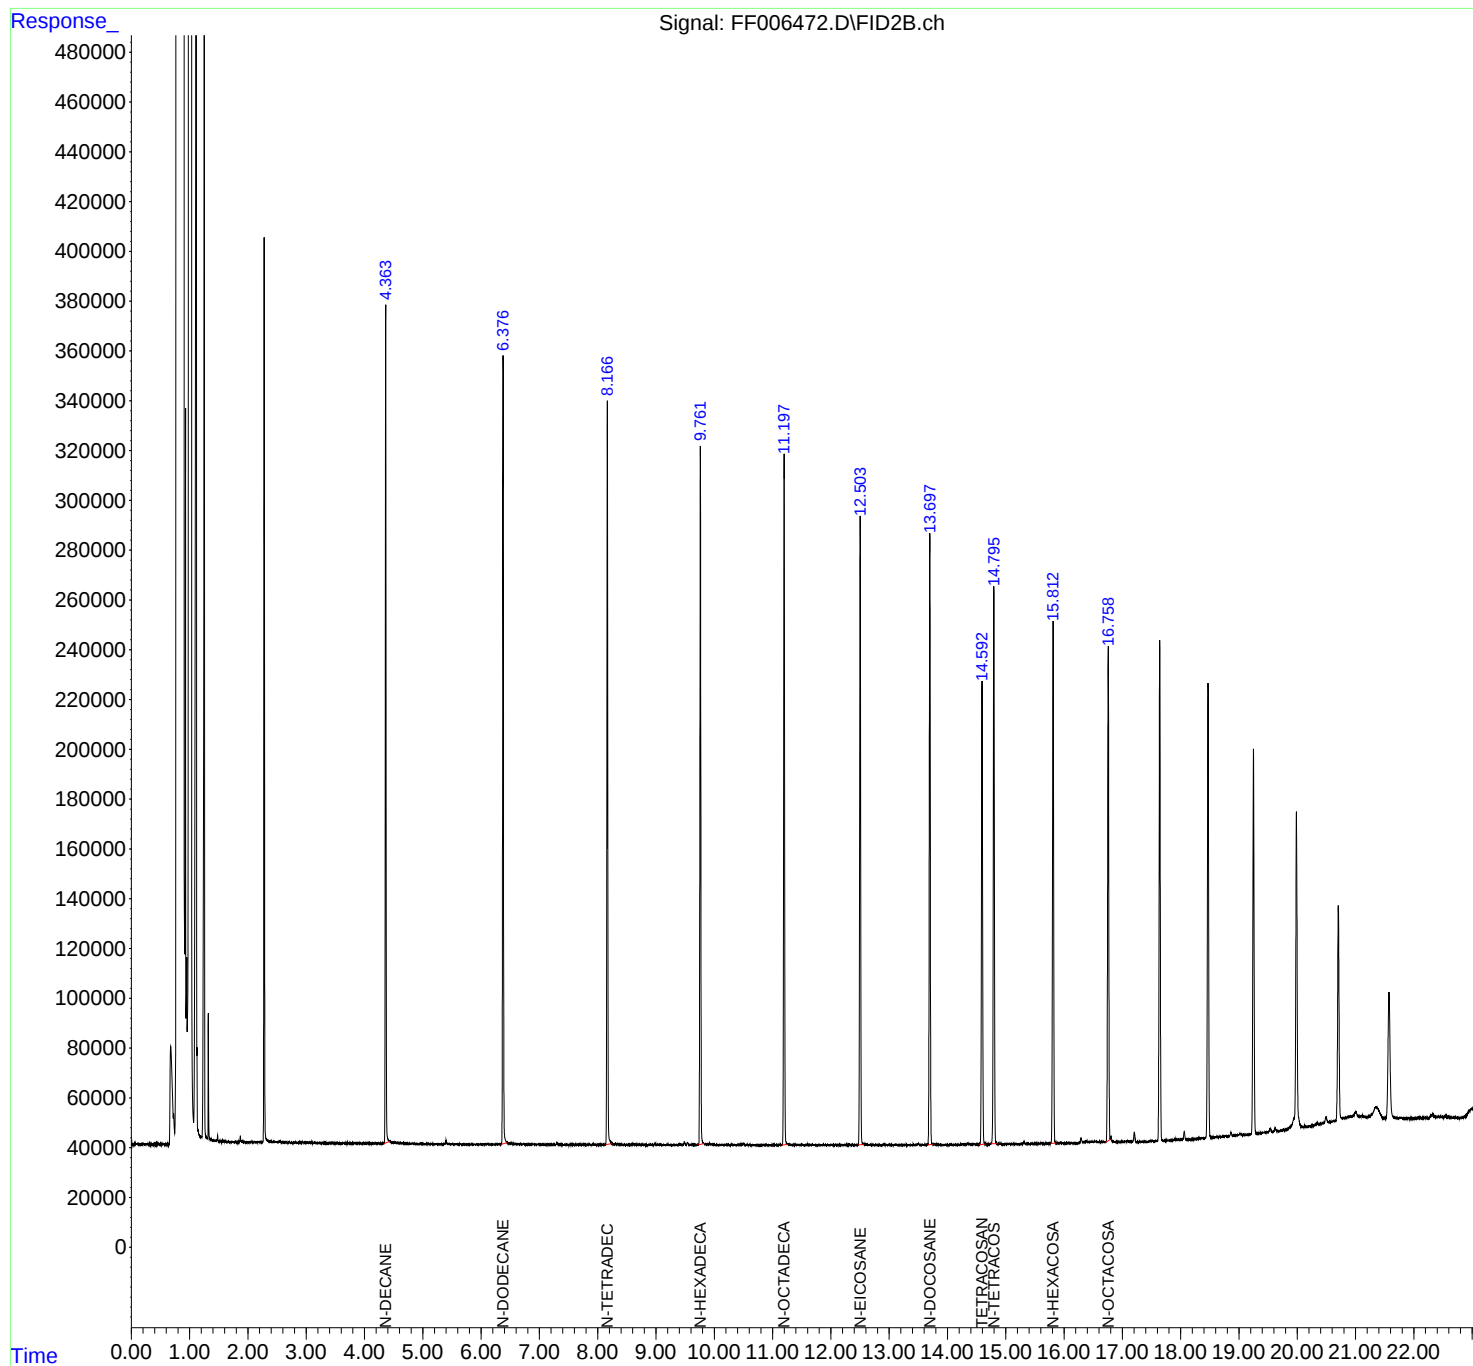


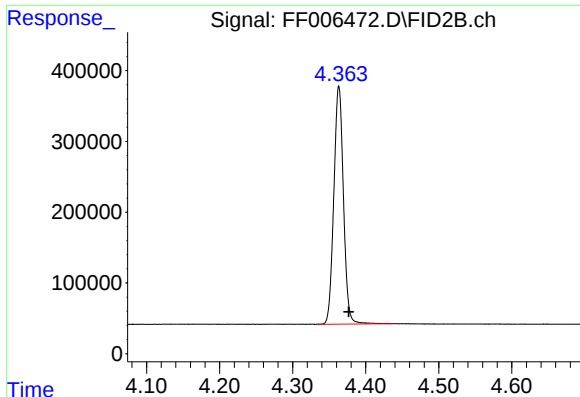

#2 N-DECANE


R.T.: 4.363 min
Delta R.T.: -0.013 min
Response: 3076935
Conc: 23.04 ug/ml

Instrument :
FID_F
ClientSampleId :
PB127206BS

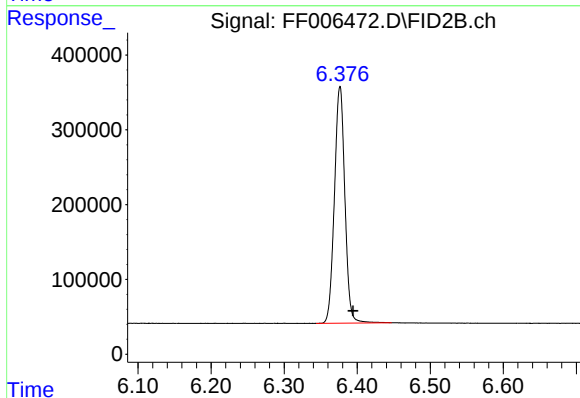


#3 N-DODECANE

R.T.: 6.377 min
Delta R.T.: -0.018 min
Response: 3145406
Conc: 23.01 ug/ml

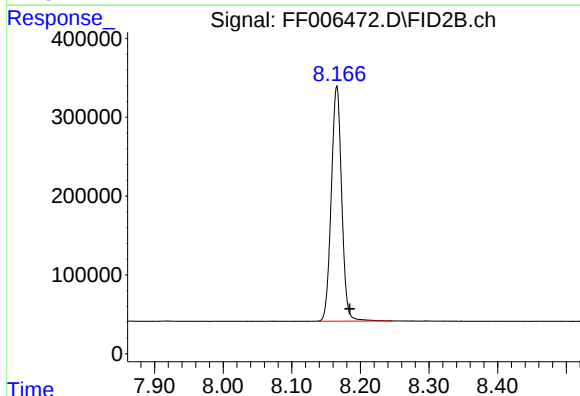


#4 N-TETRADECANE

R.T.: 8.166 min
Delta R.T.: -0.019 min
Response: 3145263
Conc: 22.87 ug/ml

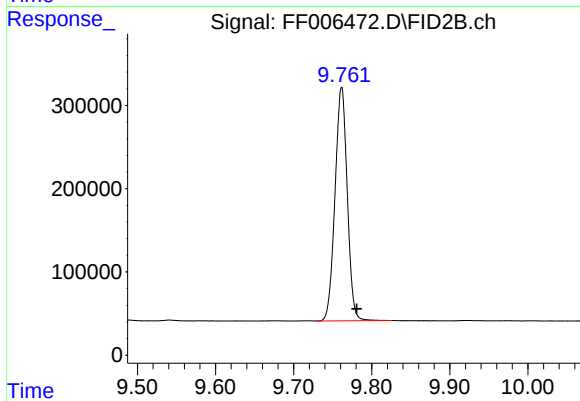

#5 N-HEXADECANE


R.T.: 9.761 min
Delta R.T.: -0.019 min
Response: 3059911
Conc: 21.81 ug/ml

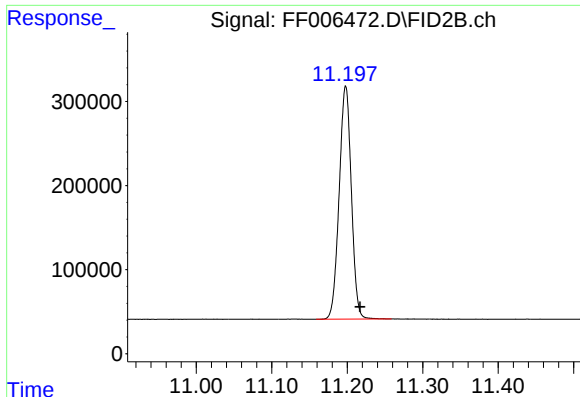

#6 N-OCTADECANE


R.T.: 11.198 min
Delta R.T.: -0.019 min
Response: 3111800
Conc: 22.12 ug/ml

Instrument :
FID_F
ClientSampleId :
PB127206BS

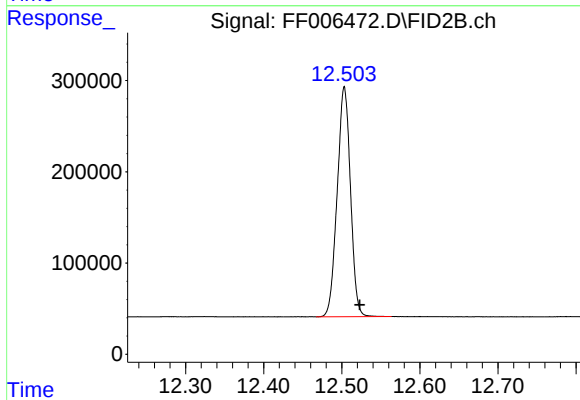


#7 N-EICOSANE

R.T.: 12.503 min
Delta R.T.: -0.020 min
Response: 2979484
Conc: 21.14 ug/ml

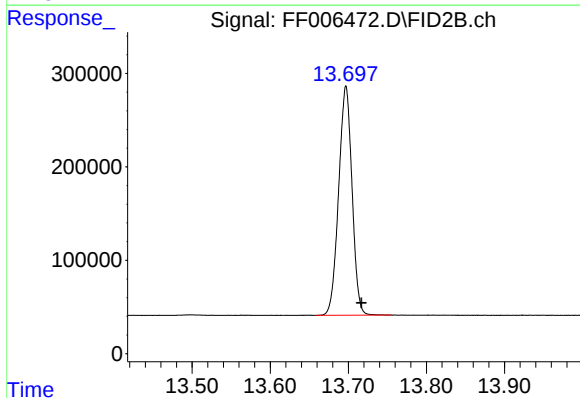


#8 N-DOCOSANE

R.T.: 13.697 min
Delta R.T.: -0.020 min
Response: 2920953
Conc: 20.78 ug/ml

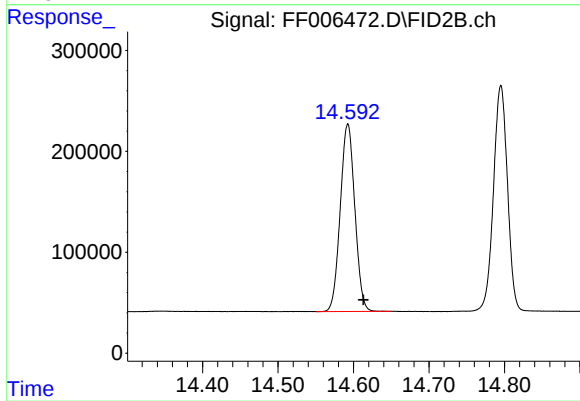

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.593 min
Delta R.T.: -0.021 min
Response: 2492570
Conc: 20.46 ug/ml

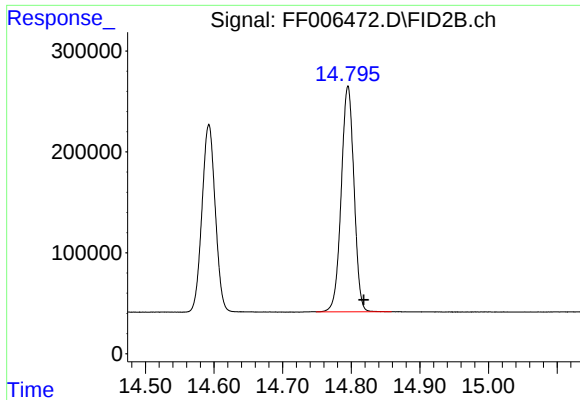

#10 N-TETRACOSANE


R.T.: 14.795 min
Delta R.T.: -0.023 min
Response: 2885401
Conc: 20.65 ug/ml

Instrument :
FID_F
ClientSampleId :
PB127206BS

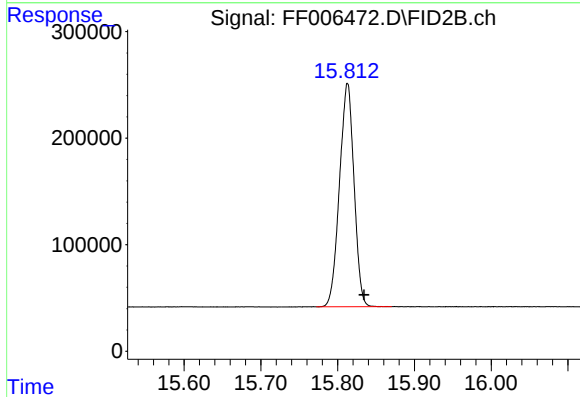

#11 N-HEXACOSANE

R.T.: 15.813 min
Delta R.T.: -0.021 min
Response: 2759613
Conc: 19.99 ug/ml

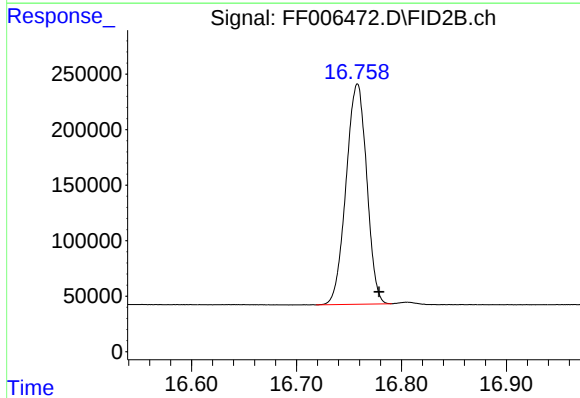

#12 N-OCTACOSANE

R.T.: 16.758 min
Delta R.T.: -0.021 min
Response: 2711953
Conc: 19.65 ug/ml