

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030320\
 Data File : FF006487.D
 Signal(s) : FID2B.ch
 Acq On : 03 Mar 2020 14:46
 Operator : DD\AJ
 Sample : L1762-04MS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 04 00:42:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
 Quant Title :
 QLast Update : Tue Feb 11 10:27:03 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.594	2049075	16.819 ug/ml
Target Compounds			
2) N-DECANE	4.363	2676072	20.038 ug/ml
3) N-DODECANE	6.377	2810023	20.560 ug/ml
4) N-TETRADECANE	8.166	2794168	20.314 ug/ml
5) N-HEXADECANE	9.762	2832047	20.186 ug/ml
6) N-OCTADECANE	11.199	2915165	20.726 ug/ml
7) N-EICOSANE	12.505	2855011	20.258 ug/ml
8) N-DOCOSANE	13.698	2812777	20.014 ug/ml
10) N-TETRACOSANE	14.796	2938213	21.027 ug/ml
11) N-HEXACOSANE	15.812	2706831	19.608 ug/ml
12) N-OCTACOSANE	16.758	2834756	20.541 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030320\
Data File : FF006487.D
Signal(s) : FID2B.ch
Acq On : 03 Mar 2020 14:46
Operator : DD\AJ
Sample : L1762-04MS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 04 00:42:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF021020.M
Quant Title :
QLast Update : Tue Feb 11 10:27:03 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

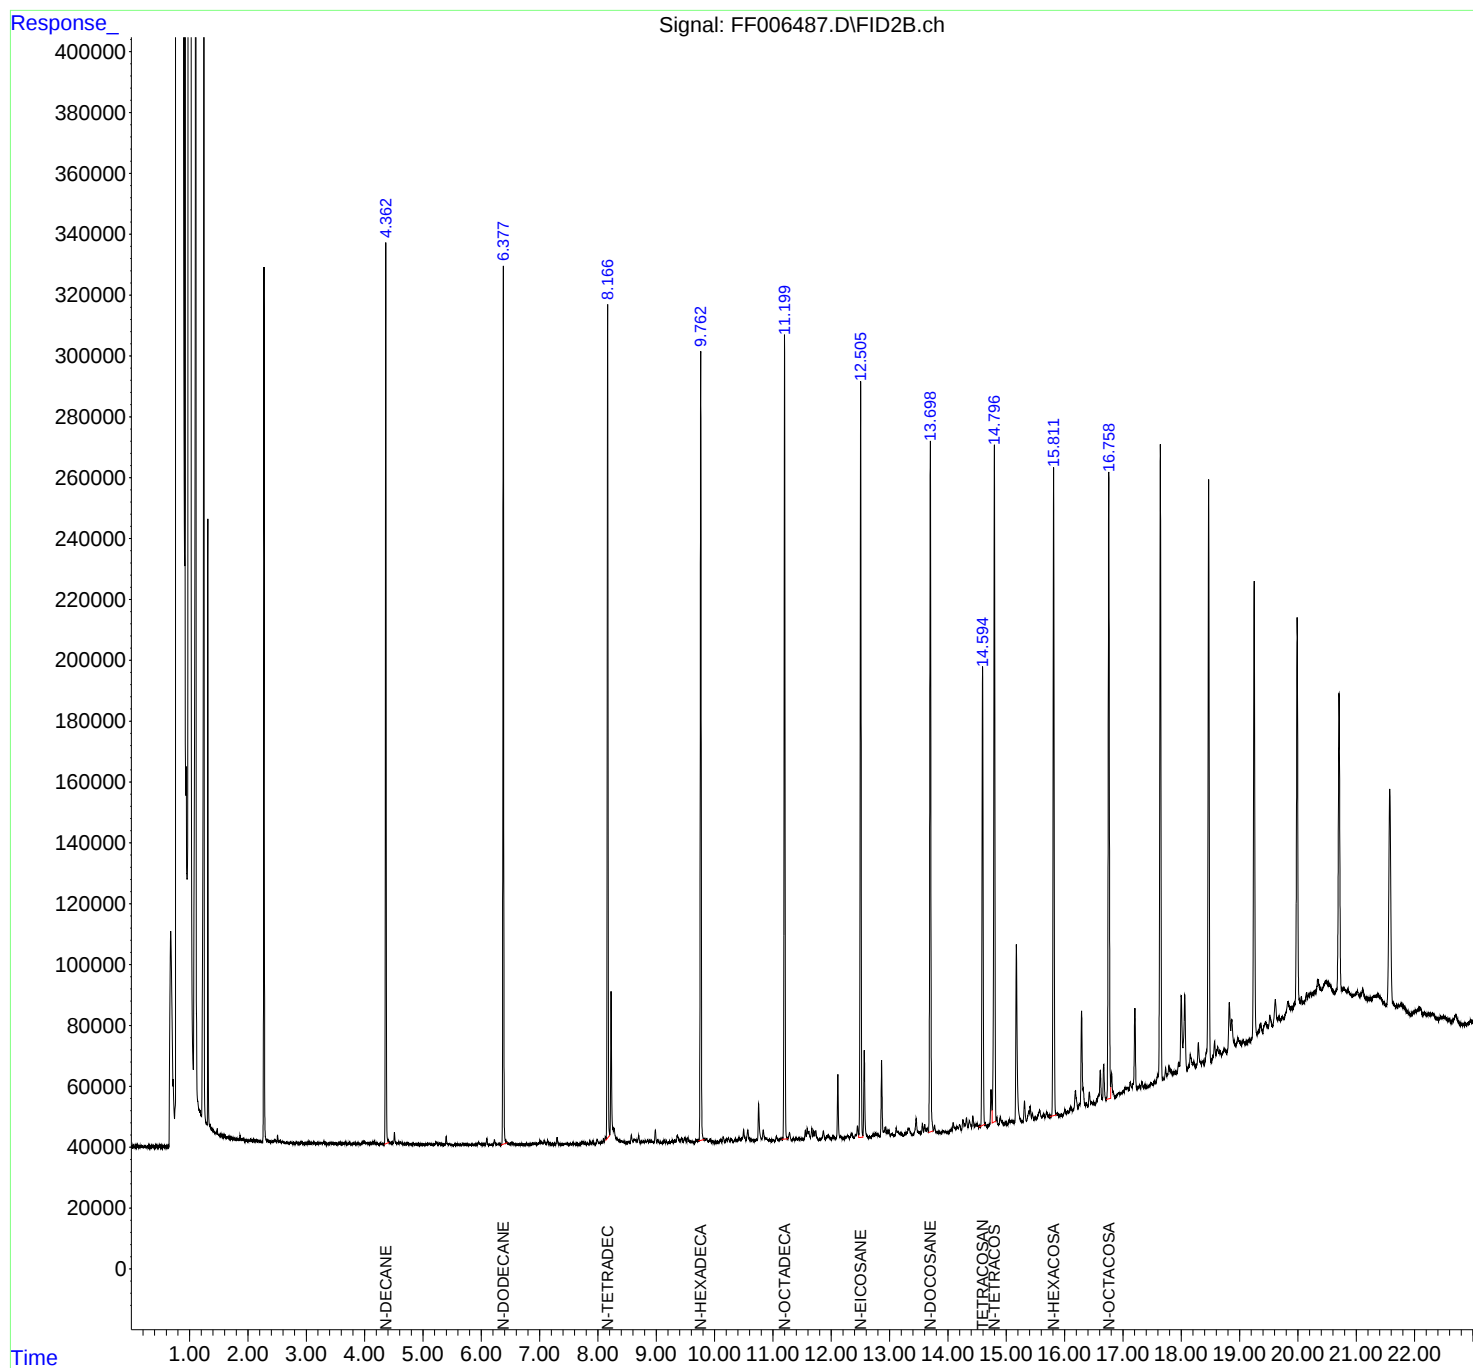

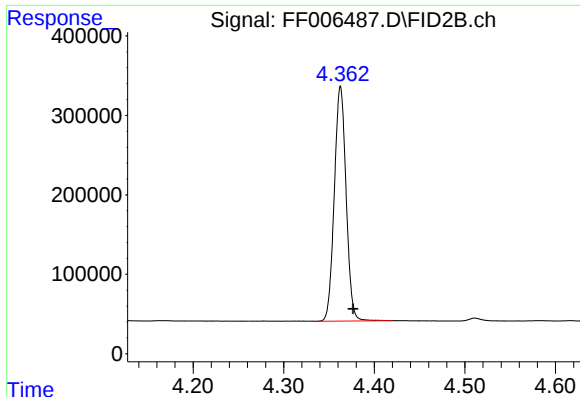


#2 N-DECANE

R.T.: 4.363 min
Delta R.T.: -0.014 min
Response: 2676072
Conc: 20.04 ug/ml

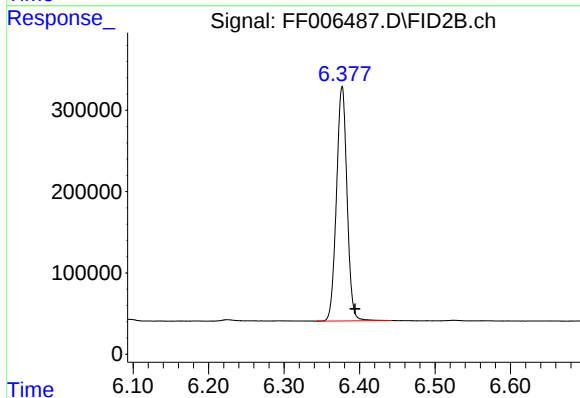


#3 N-DODECANE

R.T.: 6.377 min
Delta R.T.: -0.017 min
Response: 2810023
Conc: 20.56 ug/ml

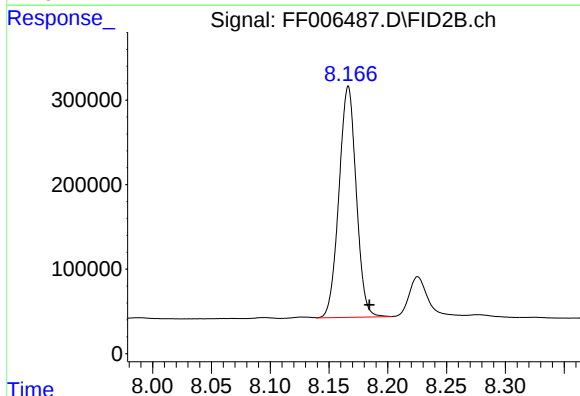


#4 N-TETRADECANE

R.T.: 8.166 min
Delta R.T.: -0.018 min
Response: 2794168
Conc: 20.31 ug/ml

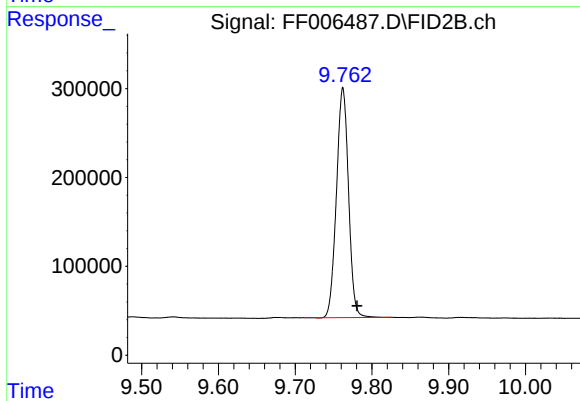


#5 N-HEXADECANE

R.T.: 9.762 min
Delta R.T.: -0.018 min
Response: 2832047
Conc: 20.19 ug/ml

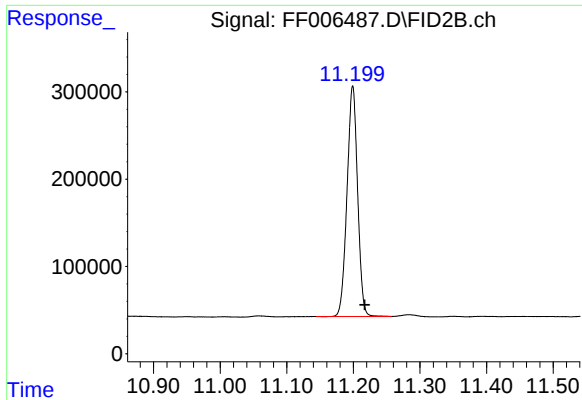


#6 N-OCTADECANE

R.T.: 11.199 min
Delta R.T.: -0.018 min
Response: 2915165
Conc: 20.73 ug/ml

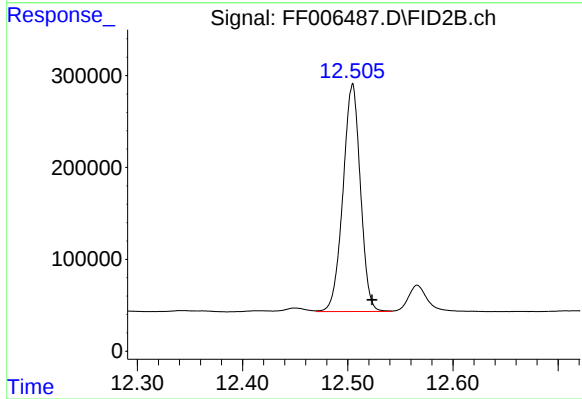


#7 N-EICOSANE

R.T.: 12.505 min
Delta R.T.: -0.019 min
Response: 2855011
Conc: 20.26 ug/ml

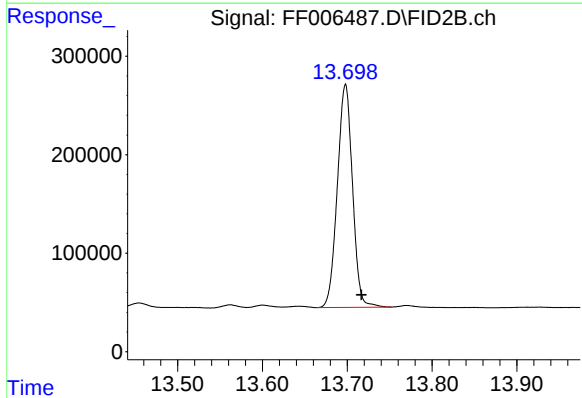


#8 N-DOCOSANE

R.T.: 13.698 min
Delta R.T.: -0.019 min
Response: 2812777
Conc: 20.01 ug/ml

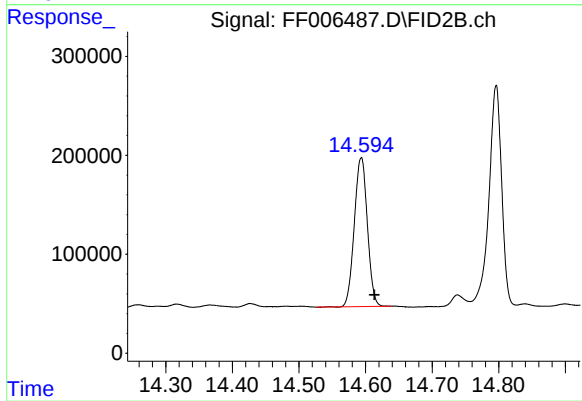


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.594 min
Delta R.T.: -0.020 min
Response: 2049075
Conc: 16.82 ug/ml

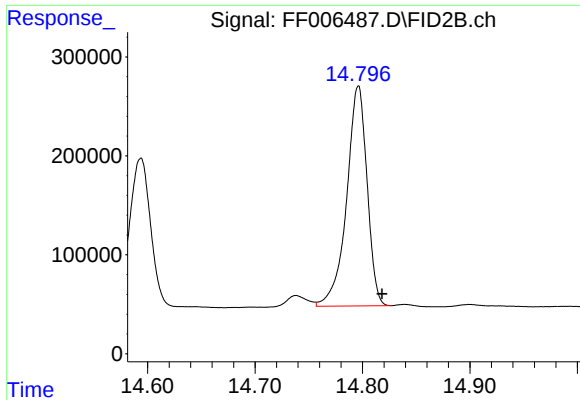


#10 N-TETRACOSANE

R.T.: 14.796 min
Delta R.T.: -0.022 min
Response: 2938213
Conc: 21.03 ug/ml

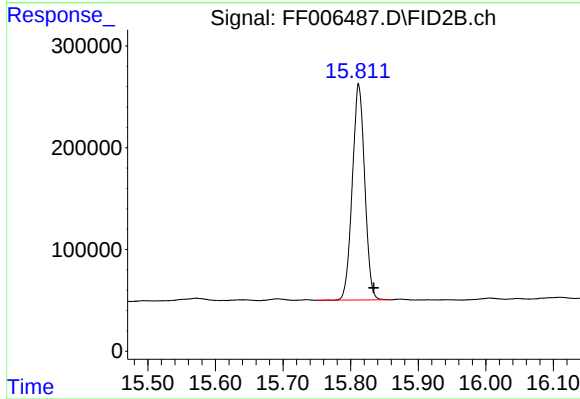

#11 N-HEXACOSANE

R.T.: 15.812 min
Delta R.T.: -0.022 min
Response: 2706831
Conc: 19.61 ug/ml

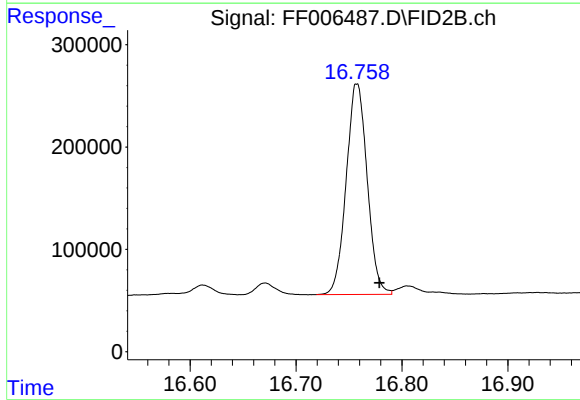

#12 N-OCTACOSANE

R.T.: 16.758 min
Delta R.T.: -0.021 min
Response: 2834756
Conc: 20.54 ug/ml