

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030419\
 Data File : FF003696.D
 Signal(s) : FID2B.ch
 Acq On : 04 Mar 2019 18:38
 Operator : AJ\SJ
 Sample : K1665-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 04 23:56:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.594	1770135	12.714 ug/ml
Target Compounds			
4) N-TETRADECANE	8.197f	277197	1.729 ug/ml
7) N-EICOSANE	12.544	1207622	7.382 ug/ml
10) N-TETRACOSANE	14.774	450433	2.847 ug/ml
11) N-HEXACOSANE	15.821	109729	0.711 ug/ml
12) N-OCTACOSANE	16.775	193351	1.280 ug/ml
13) N-TRIACONTANE	17.664	221551	1.506 ug/ml
14) N-DOTRIACONTANE	18.502	246996	1.737 ug/ml
16) N-HEXATRIACONTANE	20.077	506273	3.880 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030419\
Data File : FF003696.D
Signal(s) : FID2B.ch
Acq On : 04 Mar 2019 18:38
Operator : AJ\SJ
Sample : K1665-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 04 23:56:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

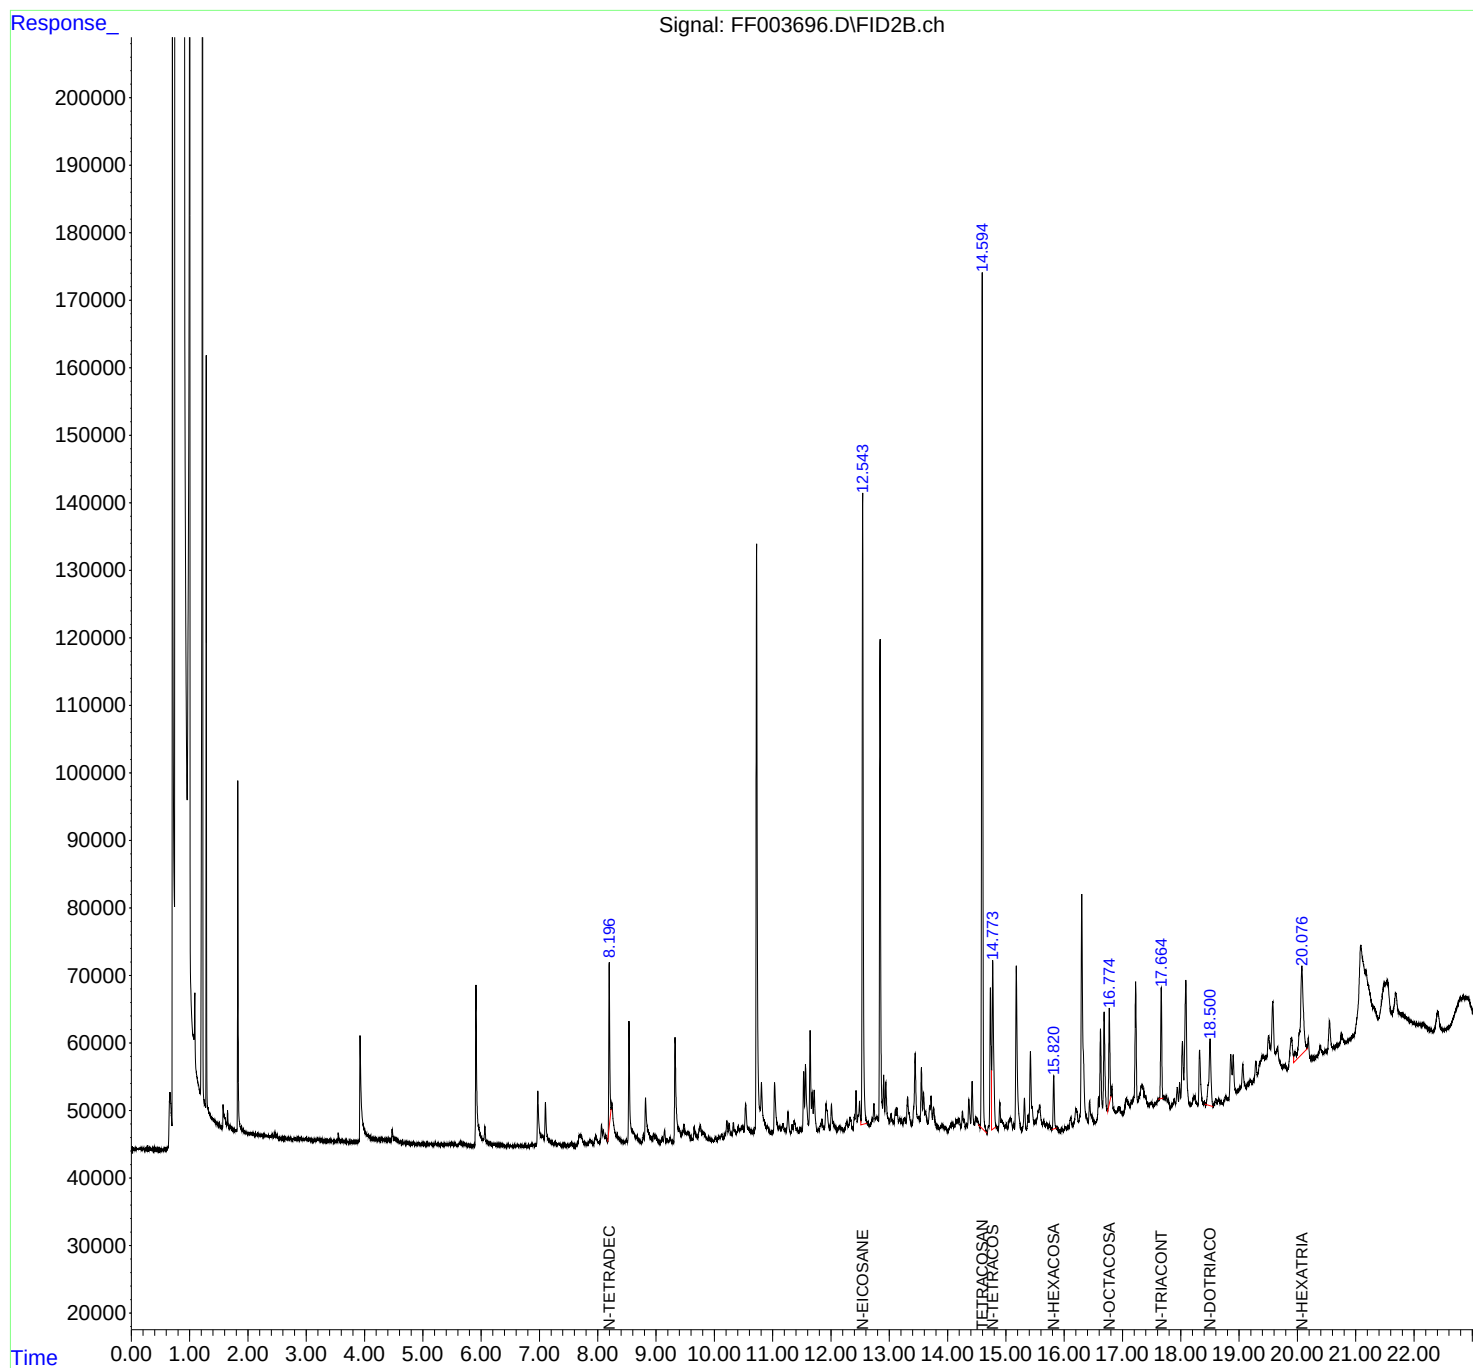

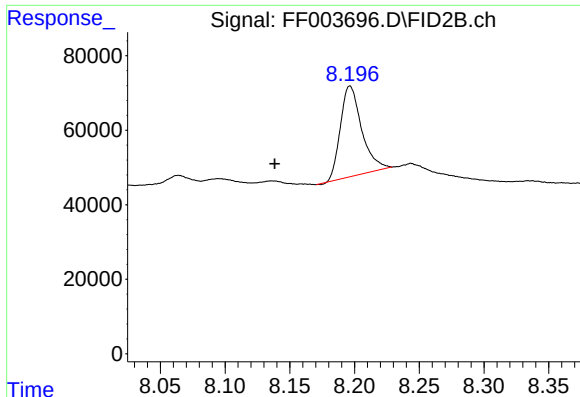


#4 N-TETRADECANE

R.T.: 8.197 min
Delta R.T.: 0.058 min
Response: 277197
Conc: 1.73 ug/ml

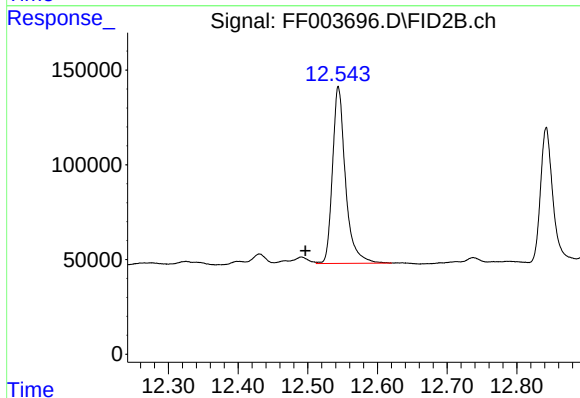


#7 N-EICOSANE

R.T.: 12.544 min
Delta R.T.: 0.047 min
Response: 1207622
Conc: 7.38 ug/ml

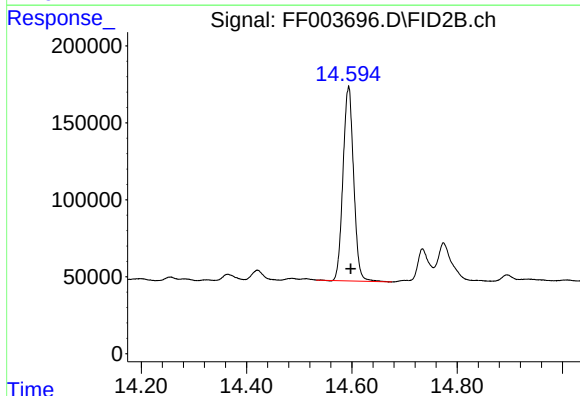


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.594 min
Delta R.T.: -0.004 min
Response: 1770135
Conc: 12.71 ug/ml

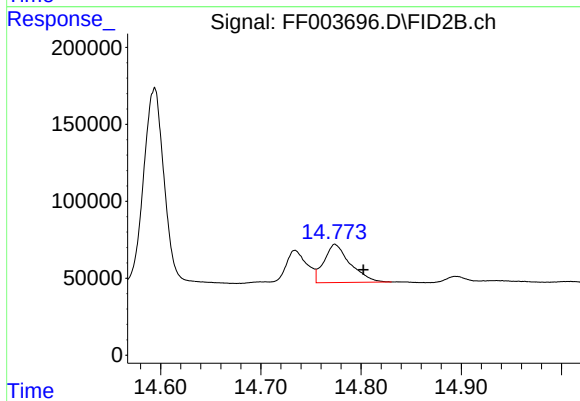


#10 N-TETRACOSANE

R.T.: 14.774 min
Delta R.T.: -0.028 min
Response: 450433
Conc: 2.85 ug/ml

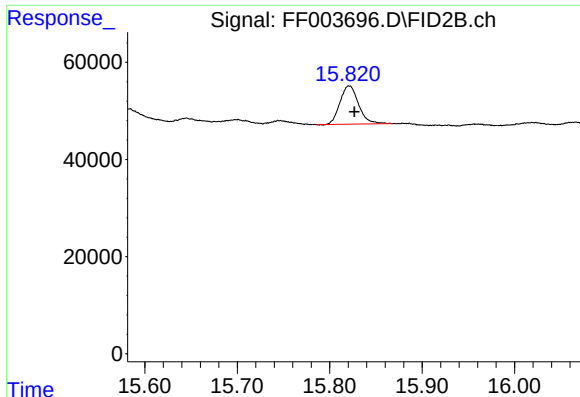


#11 N-HEXACOSANE

R.T.: 15.821 min
Delta R.T.: -0.006 min
Response: 109729
Conc: 0.71 ug/ml

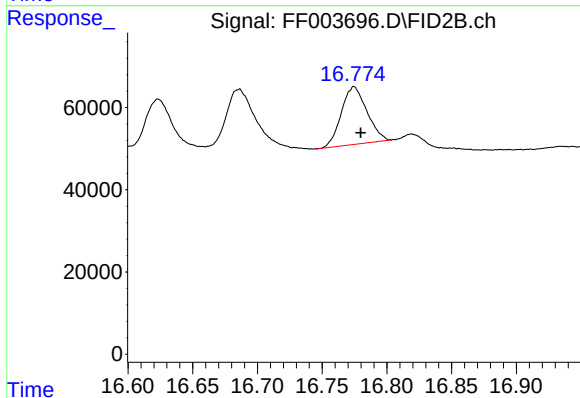


#12 N-OCTACOSANE

R.T.: 16.775 min
Delta R.T.: -0.005 min
Response: 193351
Conc: 1.28 ug/ml

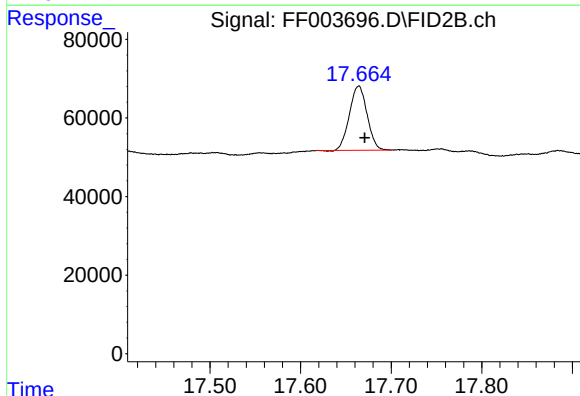


#13 N-TRIACONTANE

R.T.: 17.664 min
Delta R.T.: -0.007 min
Response: 221551
Conc: 1.51 ug/ml

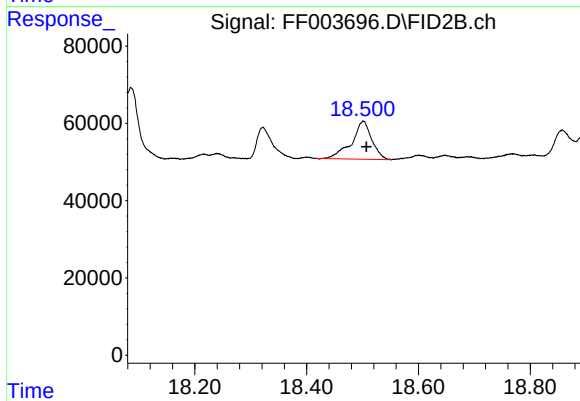

#14 N-DOTRIACONTANE

R.T.: 18.502 min
Delta R.T.: -0.005 min
Response: 246996
Conc: 1.74 ug/ml

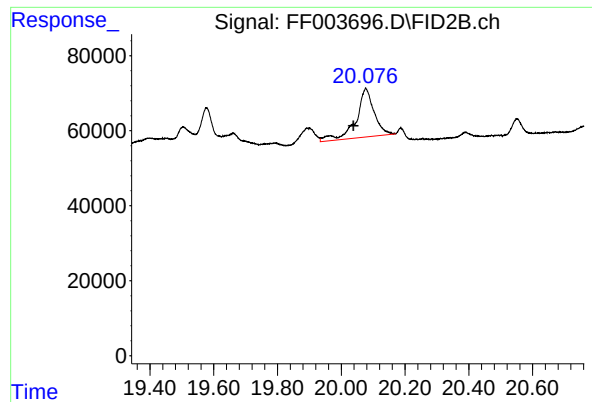

#16 N-HEXATRIACONTANE

R.T.: 20.077 min
Delta R.T.: 0.039 min
Response: 506273
Conc: 3.88 ug/ml