

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030419\
 Data File : FF003699.D
 Signal(s) : FID2B.ch
 Acq On : 04 Mar 2019 20:08
 Operator : AJ\SJ
 Sample : K1665-03
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 04 23:57:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.592	2359733	16.949 ug/ml
Target Compounds			
4) N-TETRADECANE	8.195f	511529	3.190 ug/ml
7) N-EICOSANE	12.546	270264	1.652 ug/ml
10) N-TETRACOSANE	14.793	135049	0.854 ug/ml
11) N-HEXACOSANE	15.818	295068	1.912 ug/ml
12) N-OCTACOSANE	16.772	605184	4.005 ug/ml
13) N-TRIACONTANE	17.662	703281	4.781 ug/ml
14) N-DOTRIACONTANE	18.495	579371	4.074 ug/ml
16) N-HEXATRIACONTANE	20.072	506406	3.881 ug/ml
18) N-TETRACONTANE	21.680	417605	3.357 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030419\
Data File : FF003699.D
Signal(s) : FID2B.ch
Acq On : 04 Mar 2019 20:08
Operator : AJ\SJ
Sample : K1665-03
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 04 23:57:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

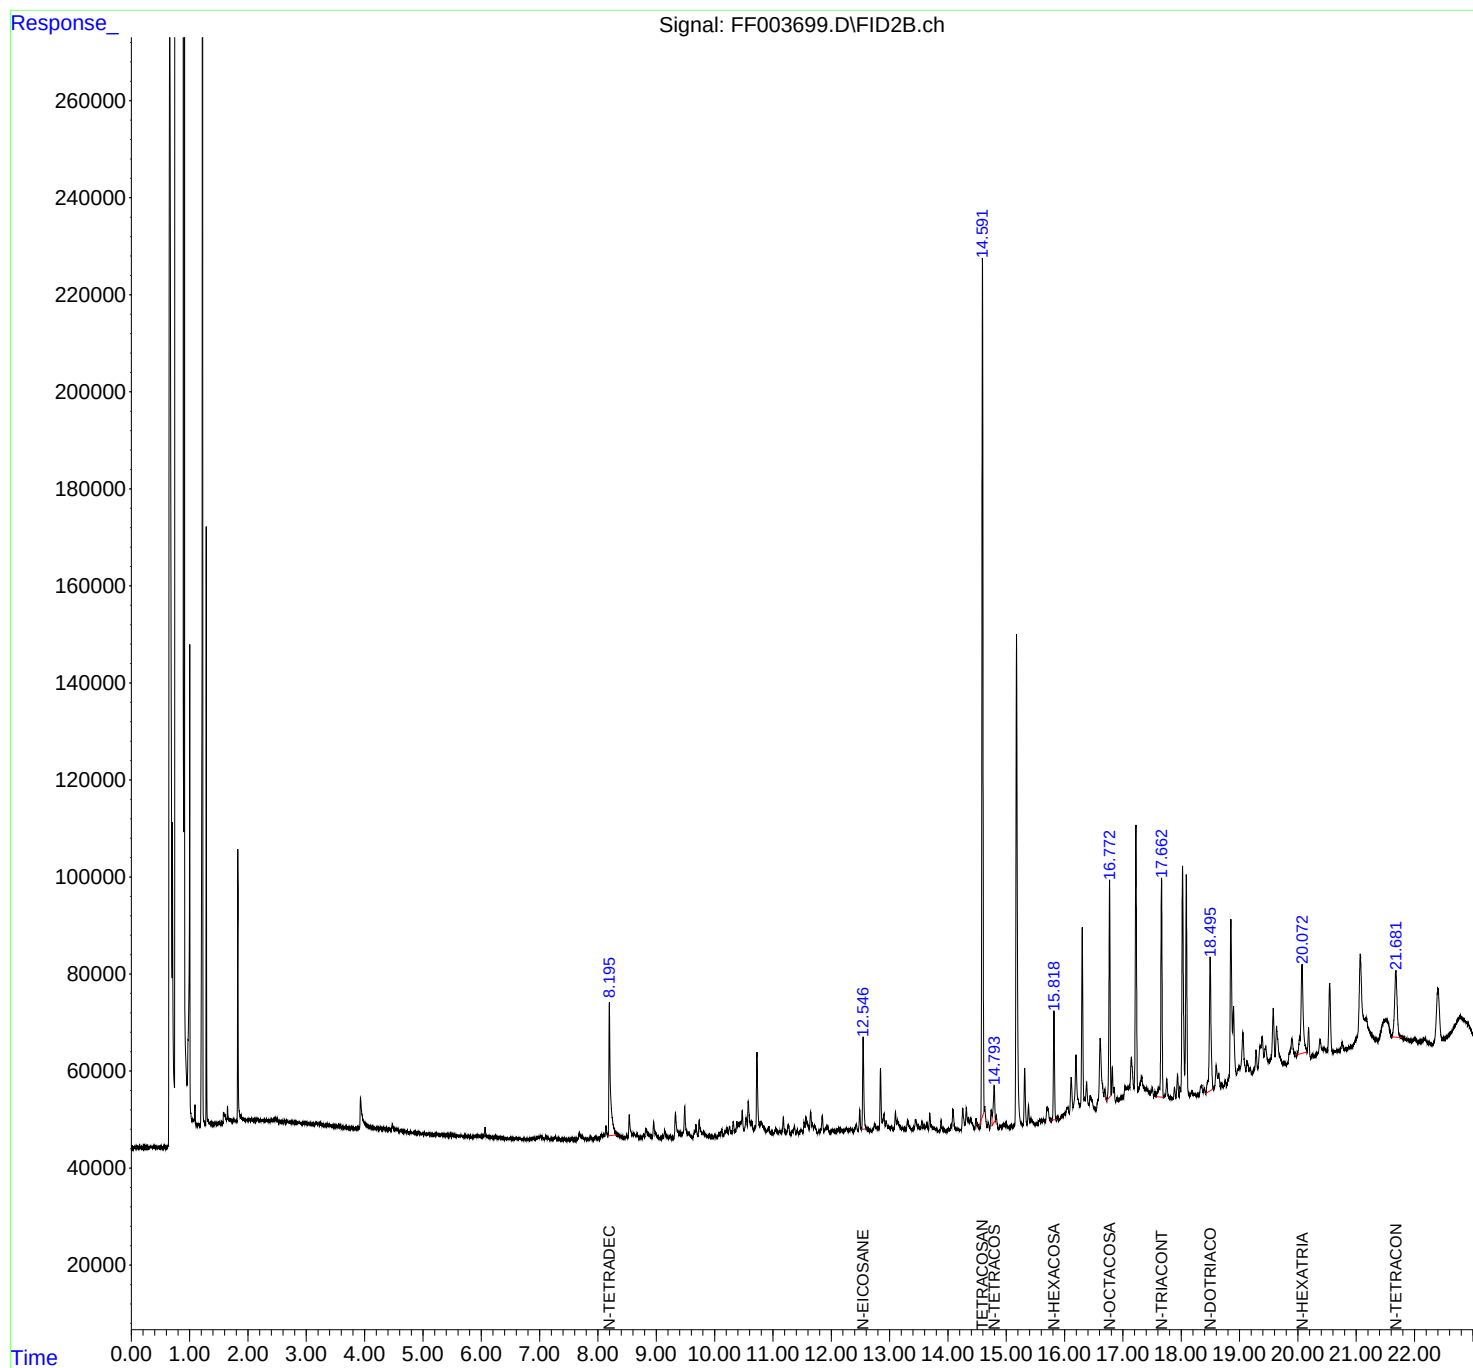

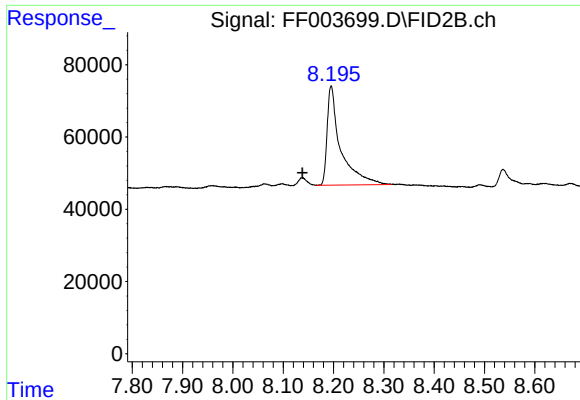


#4 N-TETRADECANE

R.T.: 8.195 min
Delta R.T.: 0.057 min
Response: 511529
Conc: 3.19 ug/ml

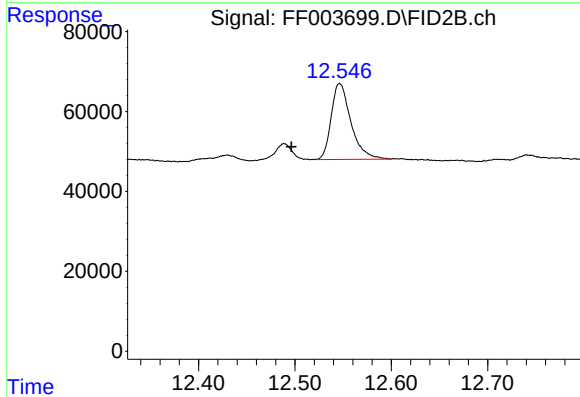


#7 N-EICOSANE

R.T.: 12.546 min
Delta R.T.: 0.050 min
Response: 270264
Conc: 1.65 ug/ml

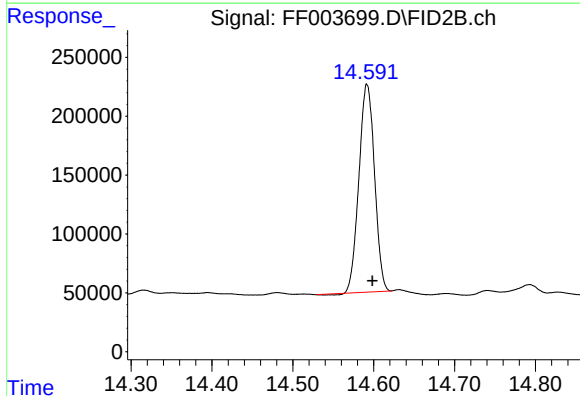


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.592 min
Delta R.T.: -0.006 min
Response: 2359733
Conc: 16.95 ug/ml

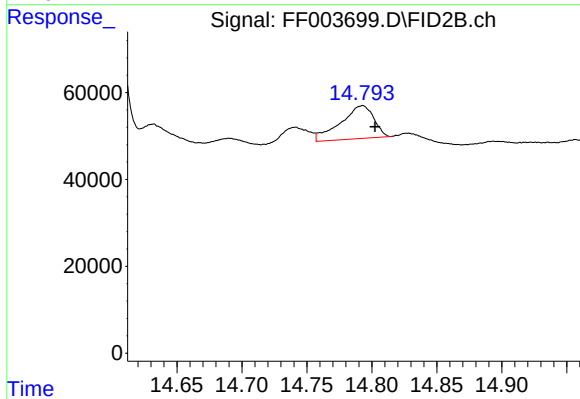


#10 N-TETRACOSANE

R.T.: 14.793 min
Delta R.T.: -0.010 min
Response: 135049
Conc: 0.85 ug/ml

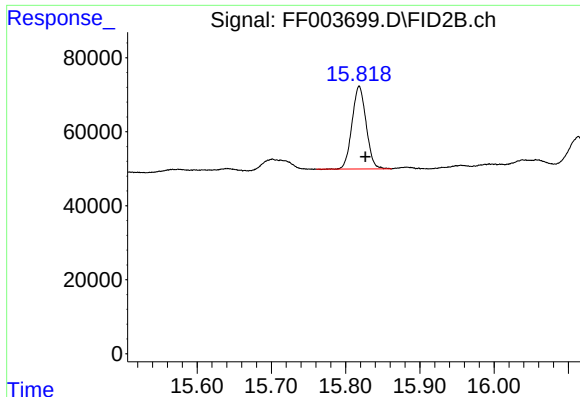


#11 N-HEXACOSANE

R.T.: 15.818 min
Delta R.T.: -0.009 min
Response: 295068
Conc: 1.91 ug/ml

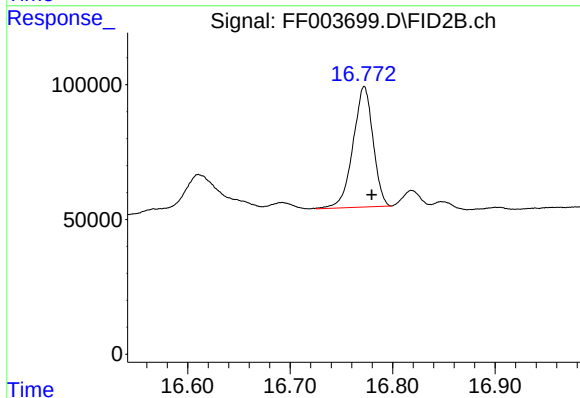


#12 N-OCTACOSANE

R.T.: 16.772 min
Delta R.T.: -0.007 min
Response: 605184
Conc: 4.00 ug/ml

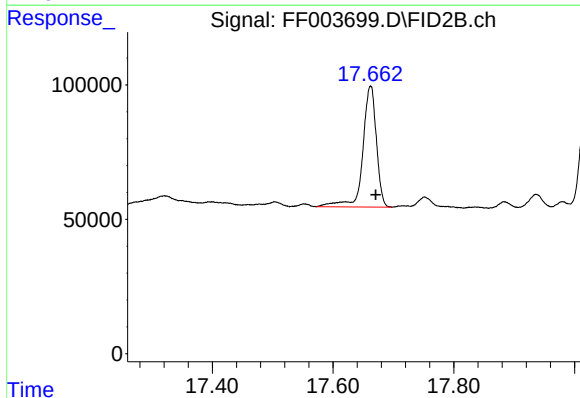


#13 N-TRIACONTANE

R.T.: 17.662 min
Delta R.T.: -0.009 min
Response: 703281
Conc: 4.78 ug/ml

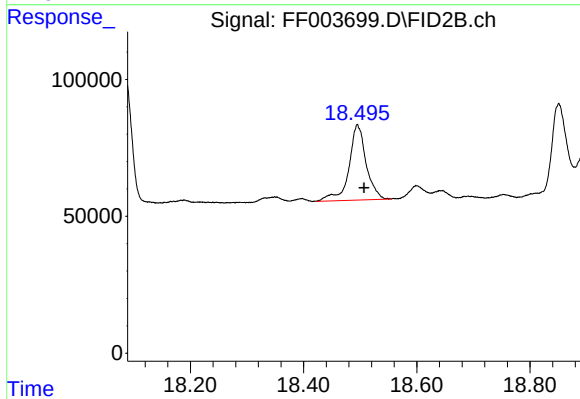


#14 N-DOTRIACONTANE

R.T.: 18.495 min
Delta R.T.: -0.012 min
Response: 579371
Conc: 4.07 ug/ml

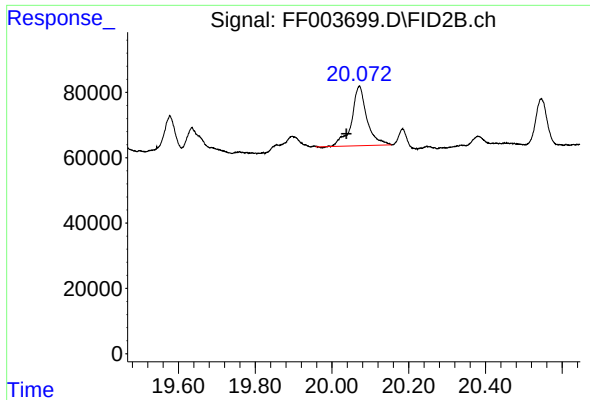

#16 N-HEXATRIACONTANE

R.T.: 20.072 min
Delta R.T.: 0.034 min
Response: 506406
Conc: 3.88 ug/ml

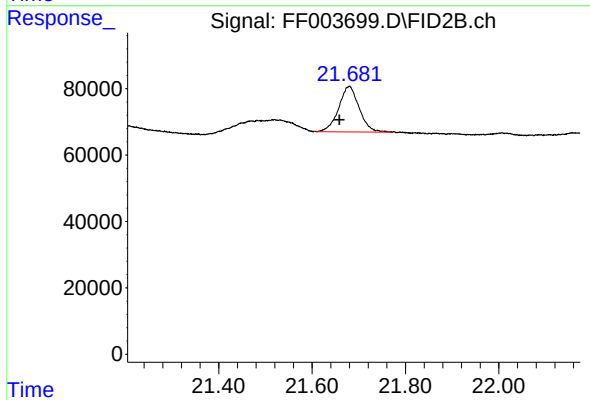

#18 N-TETRACONTANE

R.T.: 21.680 min
Delta R.T.: 0.021 min
Response: 417605
Conc: 3.36 ug/ml