

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030419\
 Data File : FF003700.D
 Signal(s) : FID2B.ch
 Acq On : 04 Mar 2019 20:38
 Operator : AJ\SJ
 Sample : K1665-05
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 04 23:57:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.592	2266527	16.279 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.194f	596869	3.723 ug/ml
7)	N-EICOSANE	12.542	1079446	6.598 ug/ml
10)	N-TETRACOSANE	14.770	343848	2.173 ug/ml
11)	N-HEXACOSANE	15.818	149067	0.966 ug/ml
12)	N-OCTACOSANE	16.772	296141	1.960 ug/ml
13)	N-TRIACONTANE	17.661	346108	2.353 ug/ml
14)	N-DOTRIACONTANE	18.497	348650	2.452 ug/ml
16)	N-HEXATRIACONTANE	20.072	507365	3.888 ug/ml
18)	N-TETRACONTANE	21.677	281692	2.264 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030419\
Data File : FF003700.D
Signal(s) : FID2B.ch
Acq On : 04 Mar 2019 20:38
Operator : AJ\SJ
Sample : K1665-05
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 04 23:57:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

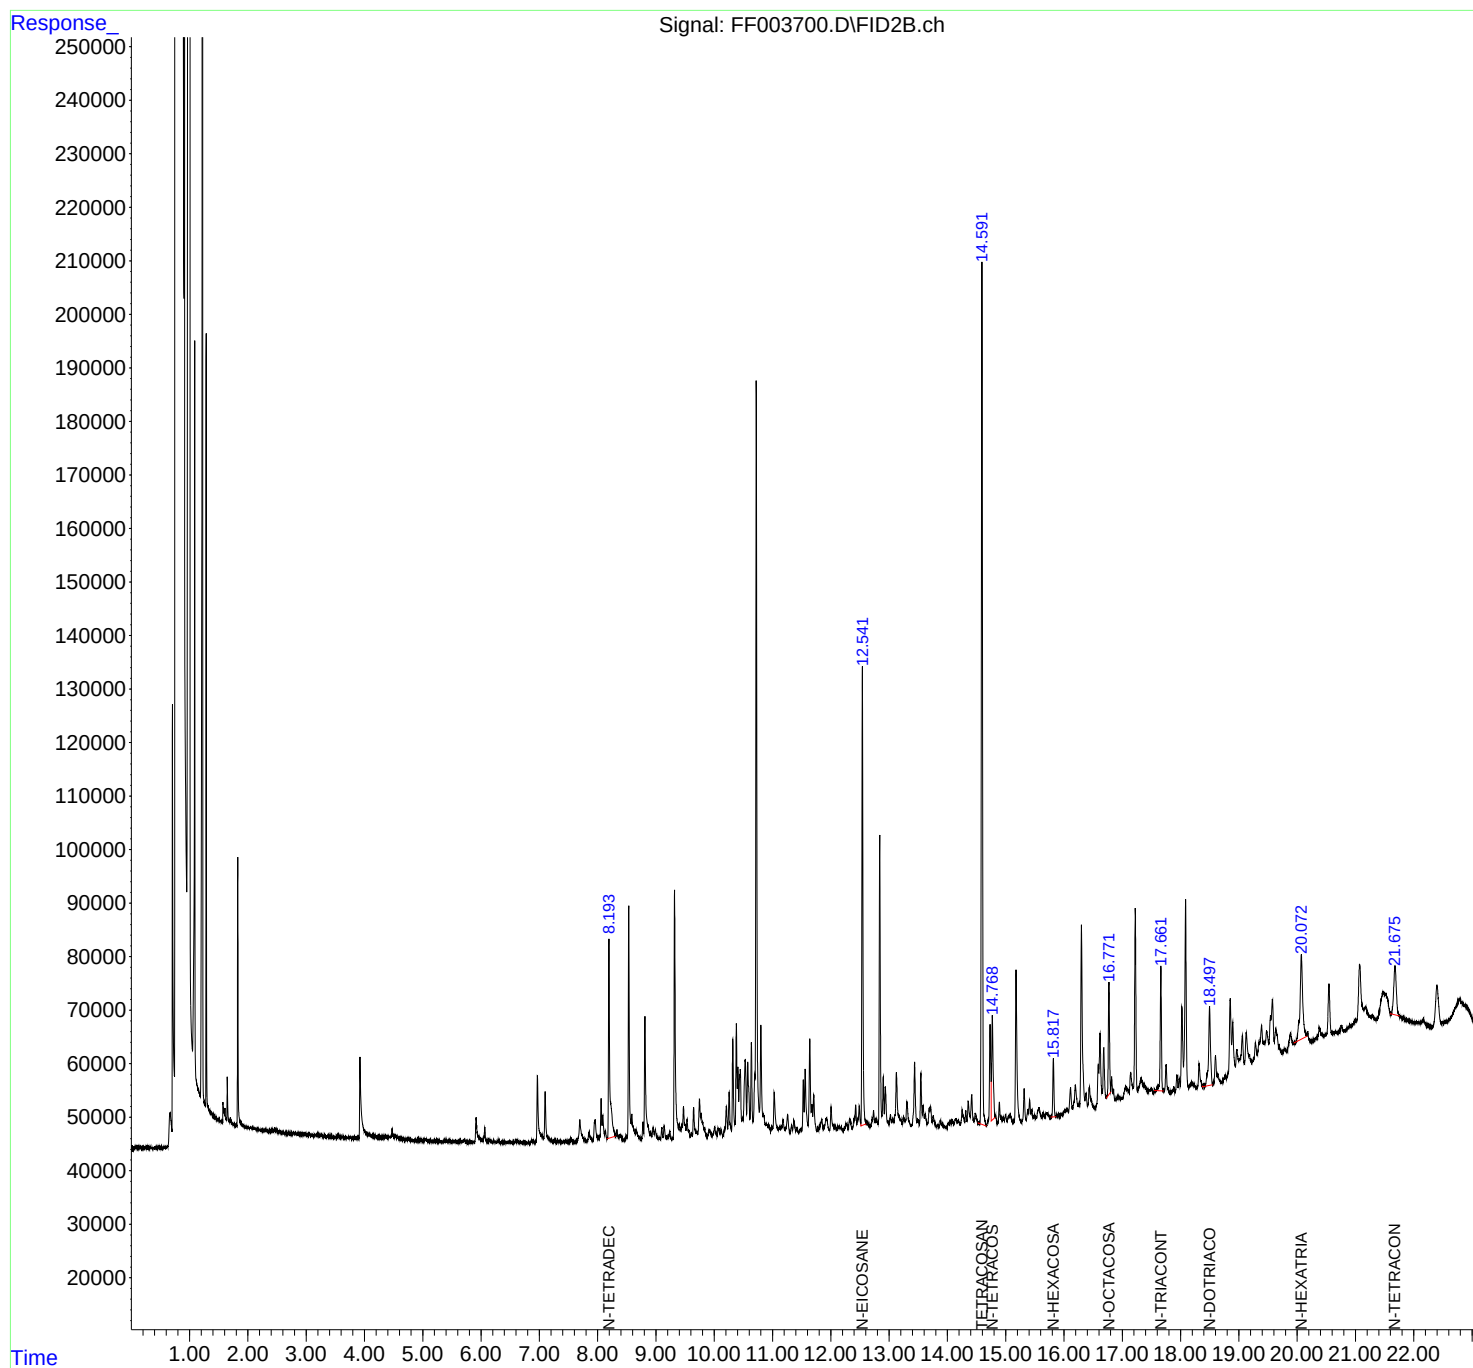

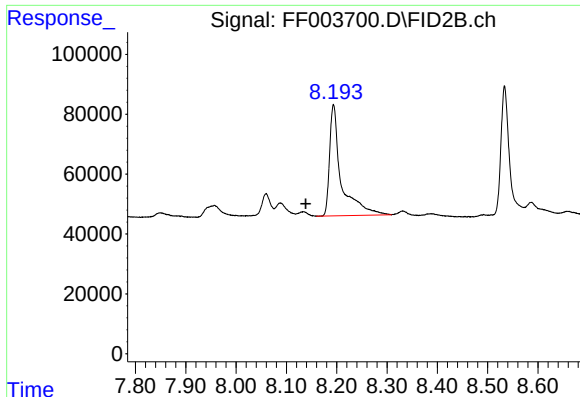


#4 N-TETRADECANE

R.T.: 8.194 min
Delta R.T.: 0.055 min
Response: 596869
Conc: 3.72 ug/ml

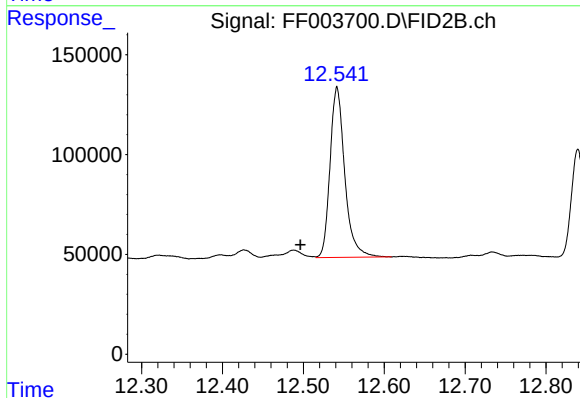


#7 N-EICOSANE

R.T.: 12.542 min
Delta R.T.: 0.045 min
Response: 1079446
Conc: 6.60 ug/ml

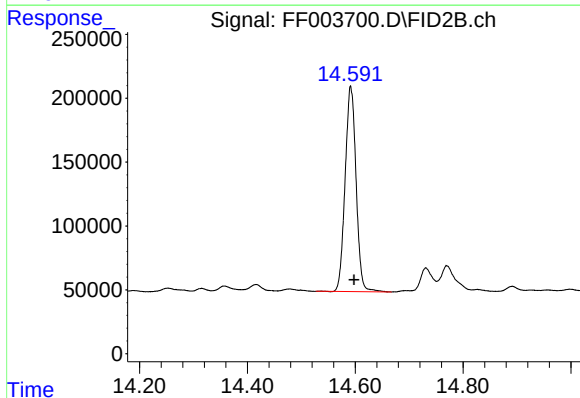


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.592 min
Delta R.T.: -0.007 min
Response: 2266527
Conc: 16.28 ug/ml

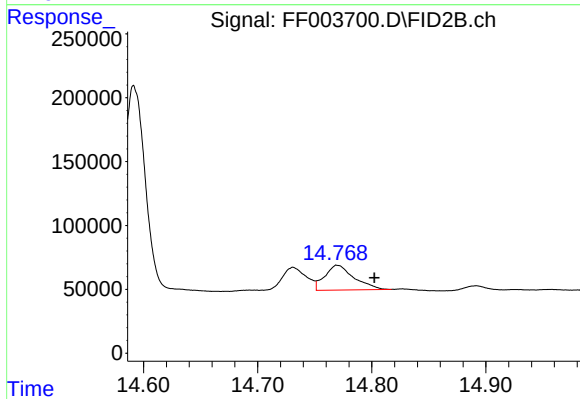


#10 N-TETRACOSANE

R.T.: 14.770 min
Delta R.T.: -0.033 min
Response: 343848
Conc: 2.17 ug/ml

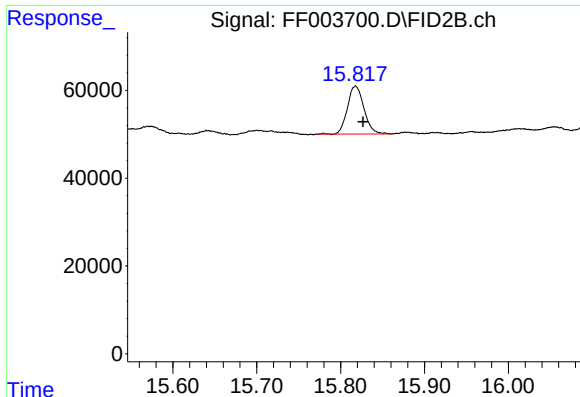


#11 N-HEXACOSANE

R.T.: 15.818 min
Delta R.T.: -0.009 min
Response: 149067
Conc: 0.97 ug/ml

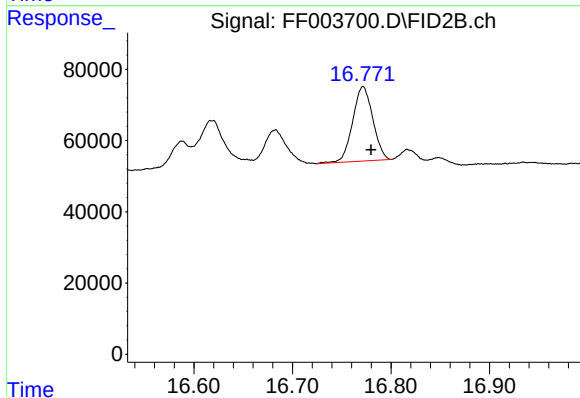


#12 N-OCTACOSANE

R.T.: 16.772 min
Delta R.T.: -0.008 min
Response: 296141
Conc: 1.96 ug/ml

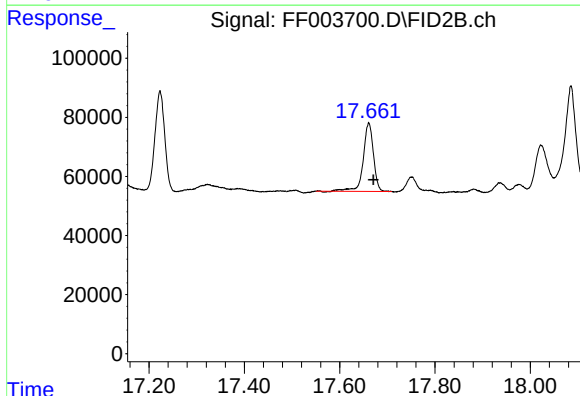


#13 N-TRIACONTANE

R.T.: 17.661 min
Delta R.T.: -0.009 min
Response: 346108
Conc: 2.35 ug/ml

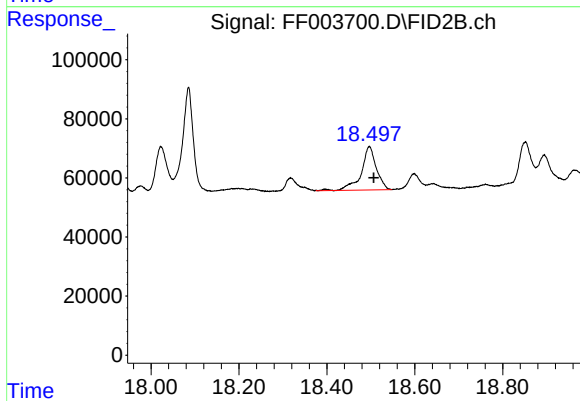


#14 N-DOTRIACONTANE

R.T.: 18.497 min
Delta R.T.: -0.010 min
Response: 348650
Conc: 2.45 ug/ml

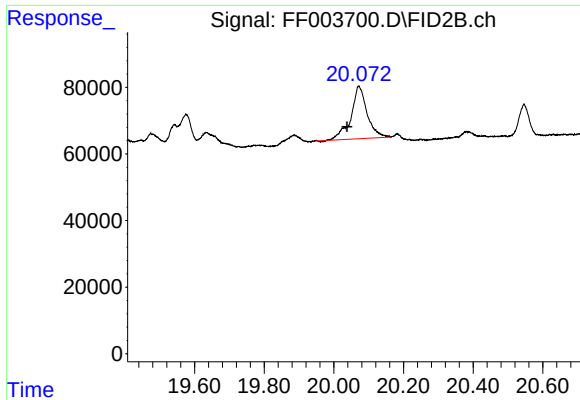

#16 N-HEXATRIACONTANE

R.T.: 20.072 min
Delta R.T.: 0.034 min
Response: 507365
Conc: 3.89 ug/ml

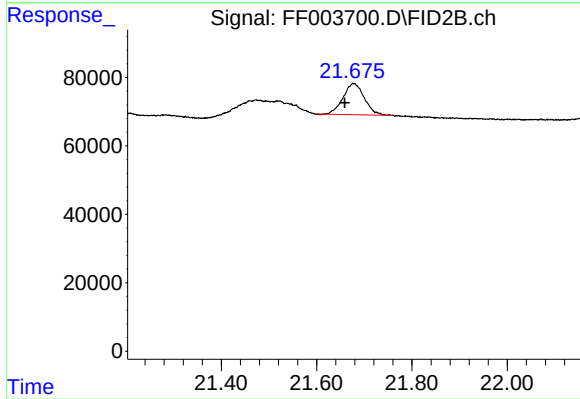

#18 N-TETRACONTANE

R.T.: 21.677 min
Delta R.T.: 0.019 min
Response: 281692
Conc: 2.26 ug/ml