

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030419\
 Data File : FF003701.D
 Signal(s) : FID2B.ch
 Acq On : 04 Mar 2019 21:08
 Operator : AJ\SJ
 Sample : K1665-07
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 04 23:57:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.592	2385916	17.137 ug/ml
Target Compounds			
4) N-TETRADECANE	8.196f	472948	2.950 ug/ml
7) N-EICOSANE	12.549f	102476	0.626 ug/ml
10) N-TETRACOSANE	14.792	126405	0.799 ug/ml
11) N-HEXACOSANE	15.818	166609	1.079 ug/ml
12) N-OCTACOSANE	16.770	274182	1.814 ug/ml
13) N-TRIACONTANE	17.661	322236	2.191 ug/ml
14) N-DOTRIACONTANE	18.497	315877	2.221 ug/ml
16) N-HEXATRIACONTANE	20.069	604978	4.637 ug/ml
18) N-TETRACONTANE	21.675	615428	4.947 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030419\
Data File : FF003701.D
Signal(s) : FID2B.ch
Acq On : 04 Mar 2019 21:08
Operator : AJ\SJ
Sample : K1665-07
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 04 23:57:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

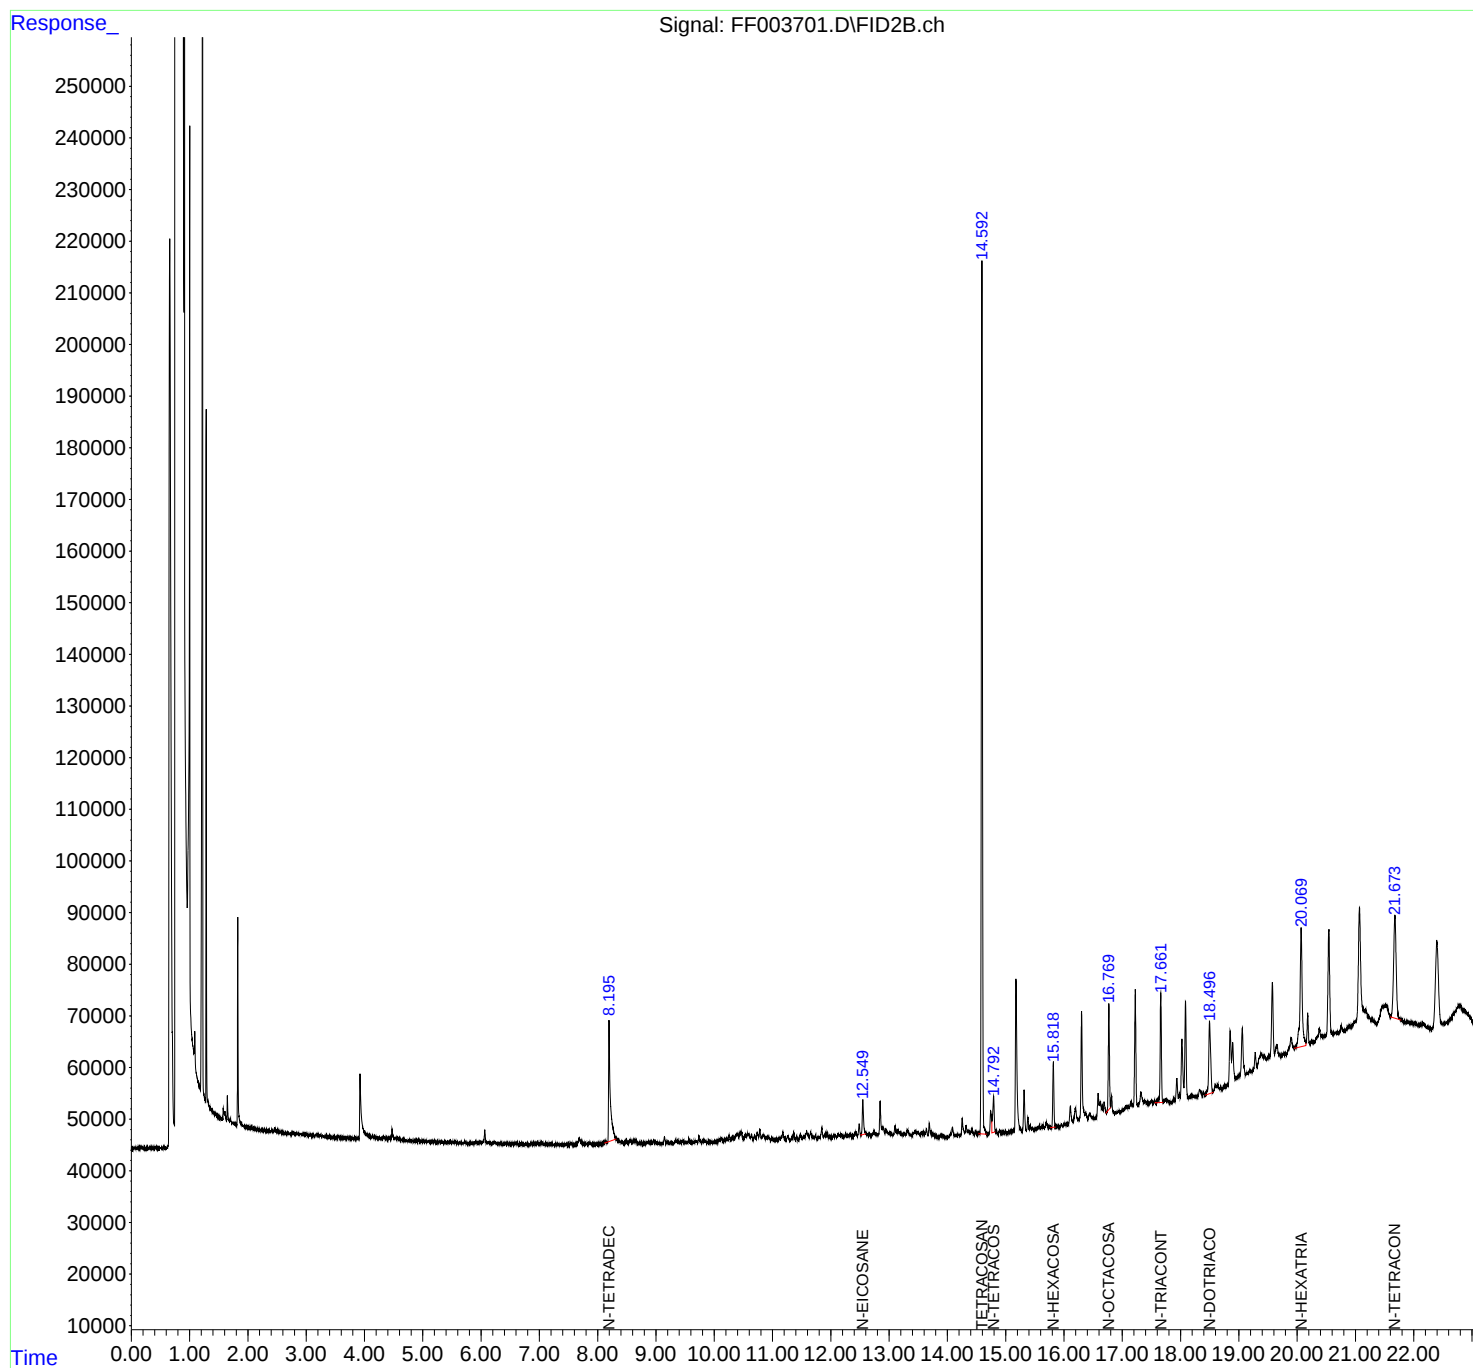

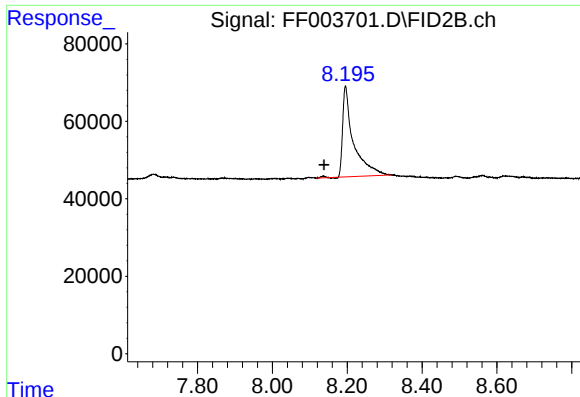


#4 N-TETRADECANE

R.T.: 8.196 min
Delta R.T.: 0.057 min
Response: 472948
Conc: 2.95 ug/ml

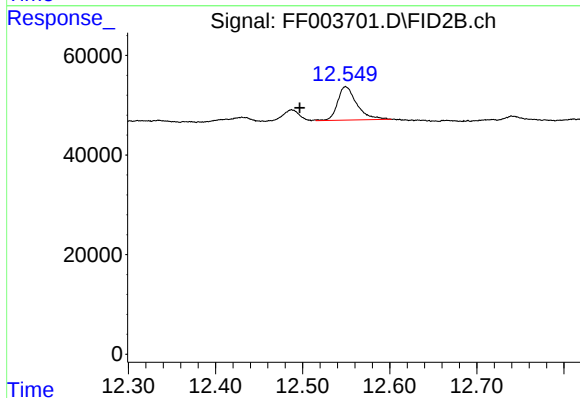


#7 N-EICOSANE

R.T.: 12.549 min
Delta R.T.: 0.053 min
Response: 102476
Conc: 0.63 ug/ml

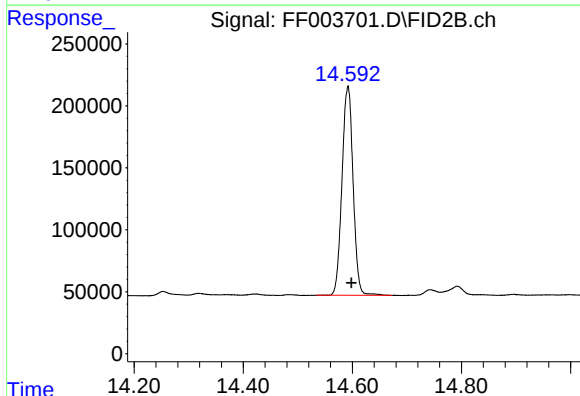


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.592 min
Delta R.T.: -0.006 min
Response: 2385916
Conc: 17.14 ug/ml

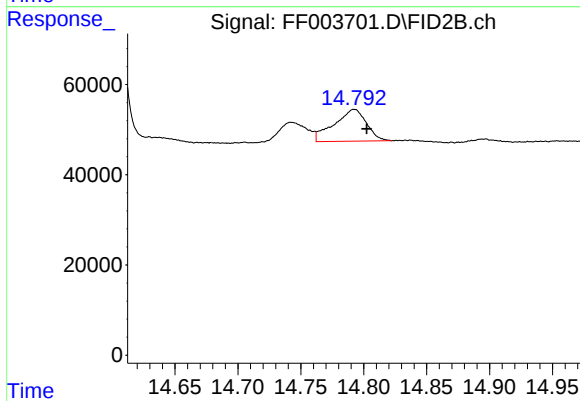


#10 N-TETRACOSANE

R.T.: 14.792 min
Delta R.T.: -0.010 min
Response: 126405
Conc: 0.80 ug/ml

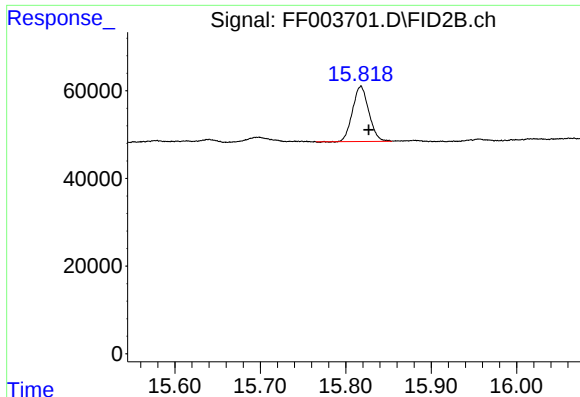


#11 N-HEXACOSANE

R.T.: 15.818 min
Delta R.T.: -0.009 min
Response: 166609
Conc: 1.08 ug/ml

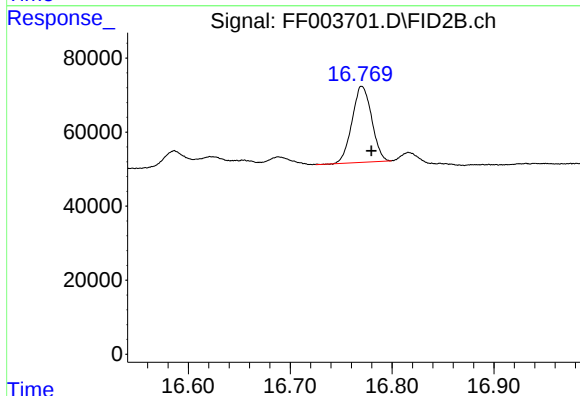


#12 N-OCTACOSANE

R.T.: 16.770 min
Delta R.T.: -0.009 min
Response: 274182
Conc: 1.81 ug/ml

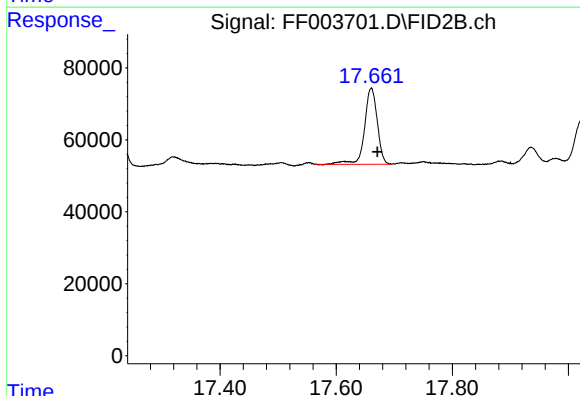


#13 N-TRIACONTANE

R.T.: 17.661 min
Delta R.T.: -0.010 min
Response: 322236
Conc: 2.19 ug/ml

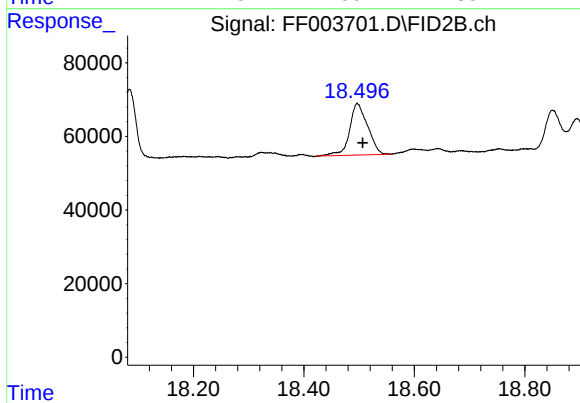


#14 N-DOTRIACONTANE

R.T.: 18.497 min
Delta R.T.: -0.010 min
Response: 315877
Conc: 2.22 ug/ml

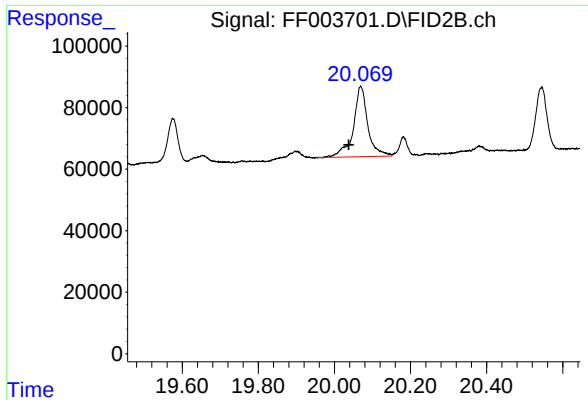

#16 N-HEXATRIACONTANE

R.T.: 20.069 min
Delta R.T.: 0.031 min
Response: 604978
Conc: 4.64 ug/ml

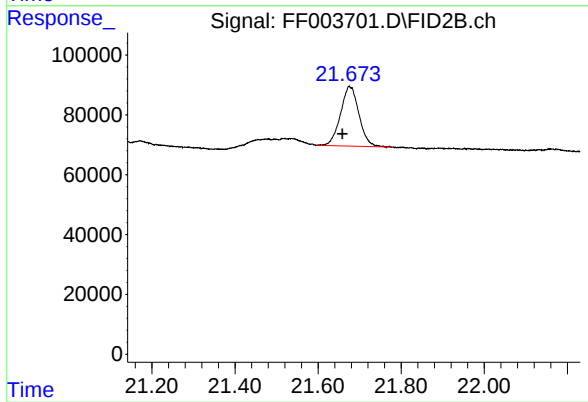

#18 N-TETRACONTANE

R.T.: 21.675 min
Delta R.T.: 0.016 min
Response: 615428
Conc: 4.95 ug/ml