

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030419\
 Data File : FF003719.D
 Signal(s) : FID2B.ch
 Acq On : 05 Mar 2019 06:08
 Operator : AJ\SJ
 Sample : K1715-06 10X
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 05 07:12:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.594	168351	1.209 ug/ml
Target Compounds			
11) N-HEXACOSANE	15.823	110965	0.719 ug/ml
12) N-OCTACOSANE	16.778	285478	1.889 ug/ml
13) N-TRIACONTANE	17.666	379658	2.581 ug/ml
14) N-DOTRIACONTANE	18.504	392048	2.757 ug/ml
15) N-TETRATRIACONTANE	19.295	175716	1.312 ug/ml
16) N-HEXATRIACONTANE	20.080	2089272	16.012 ug/ml
17) N-OCTATRIACONTANE	20.771	173635	1.504 ug/ml
18) N-TETRACONTANE	21.691	938591	7.544 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030419\
Data File : FF003719.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2019 06:08
Operator : AJ\SJ
Sample : K1715-06 10X
Misc :
ALS Vial : 78 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 05 07:12:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

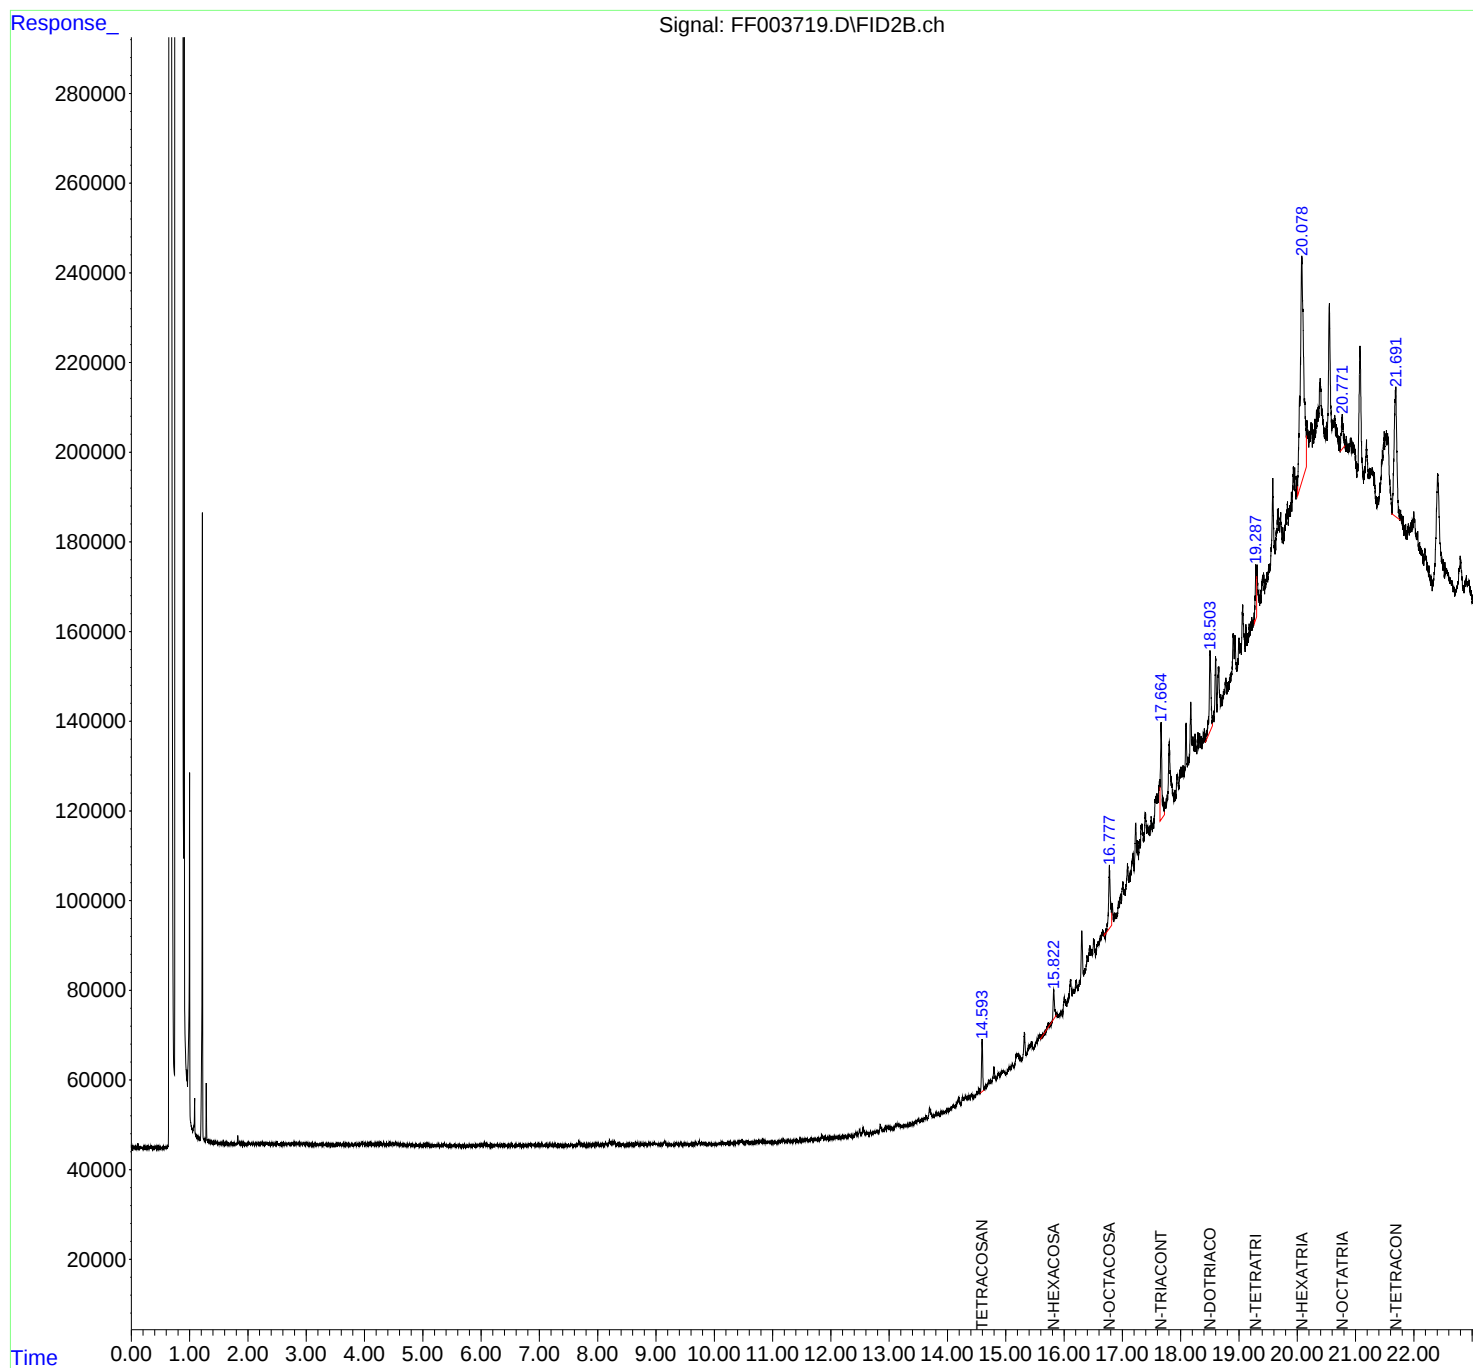

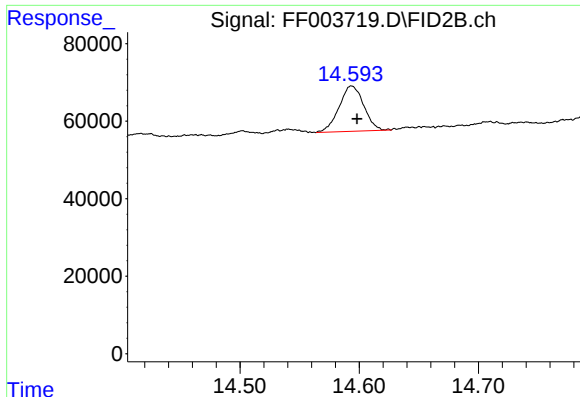


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.594 min
Delta R.T.: -0.005 min
Response: 168351
Conc: 1.21 ug/ml

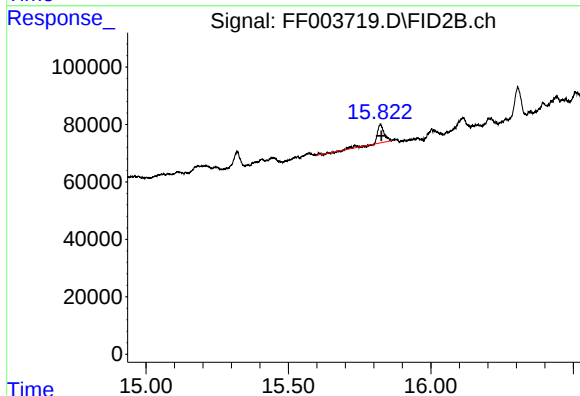


#11 N-HEXACOSANE

R.T.: 15.823 min
Delta R.T.: -0.003 min
Response: 110965
Conc: 0.72 ug/ml

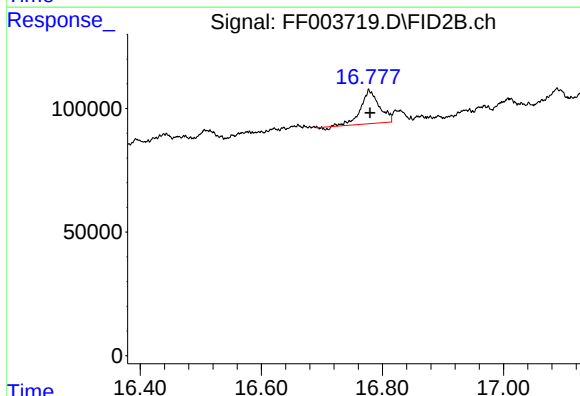


#12 N-OCTACOSANE

R.T.: 16.778 min
Delta R.T.: -0.002 min
Response: 285478
Conc: 1.89 ug/ml

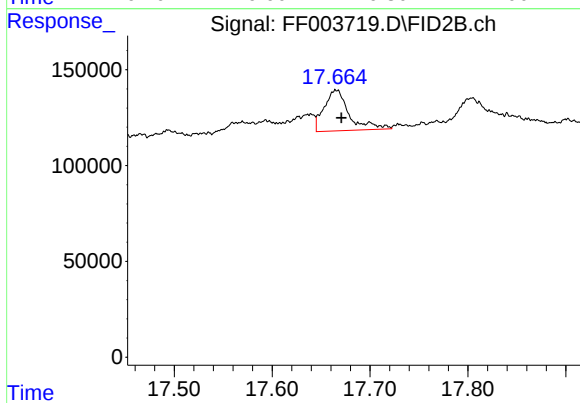


#13 N-TRIACONTANE

R.T.: 17.666 min
Delta R.T.: -0.005 min
Response: 379658
Conc: 2.58 ug/ml

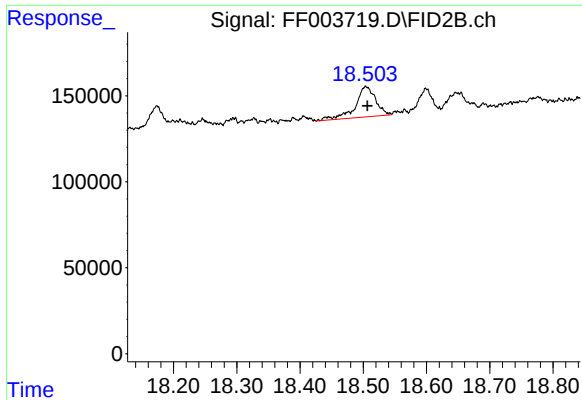


#14 N-DOTRIACONTANE

R.T.: 18.504 min
Delta R.T.: -0.003 min
Response: 392048
Conc: 2.76 ug/ml

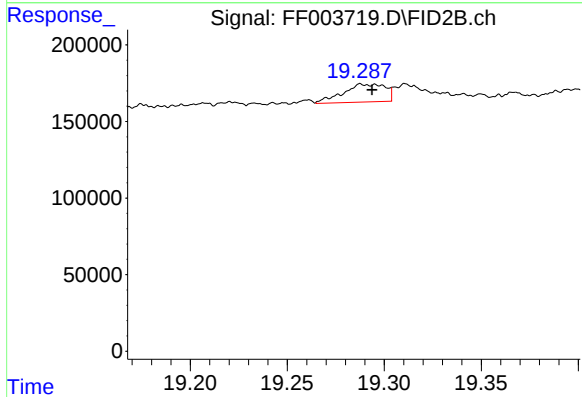


#15 N-TETRATRIACONTANE

R.T.: 19.295 min
Delta R.T.: 0.002 min
Response: 175716
Conc: 1.31 ug/ml

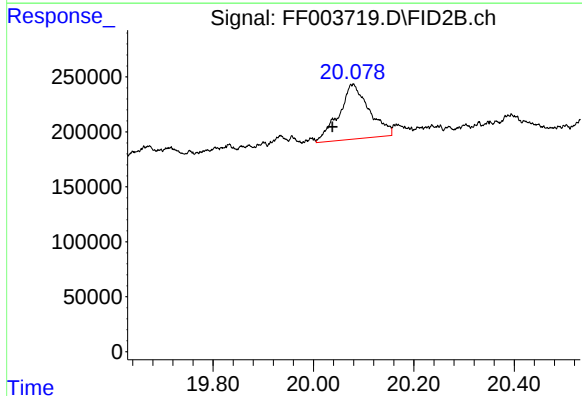


#16 N-HEXATRIACONTANE

R.T.: 20.080 min
Delta R.T.: 0.042 min
Response: 2089272
Conc: 16.01 ug/ml

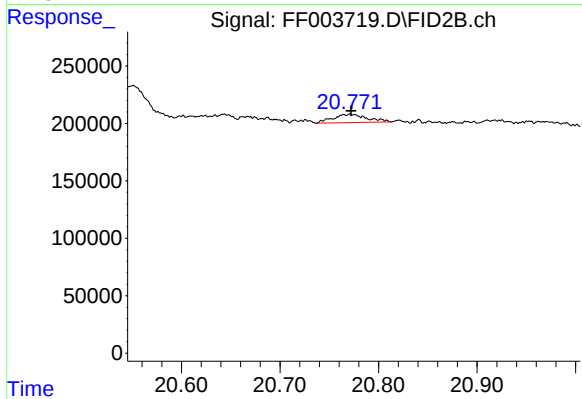

#17 N-OCTATRIACONTANE

R.T.: 20.771 min
Delta R.T.: 0.000 min
Response: 173635
Conc: 1.50 ug/ml

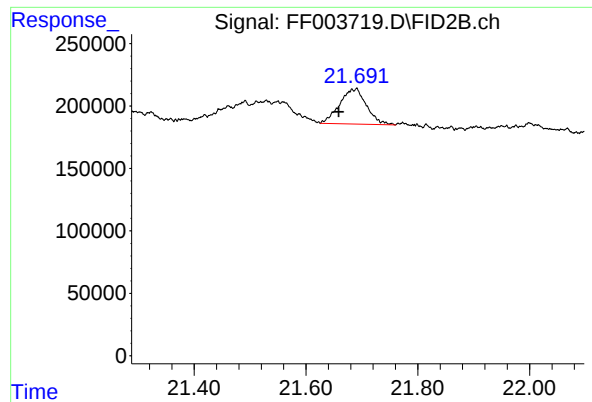

#18 N-TETRACONTANE

R.T.: 21.691 min
Delta R.T.: 0.032 min
Response: 938591
Conc: 7.54 ug/ml