

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030419\
 Data File : FF003695.D
 Signal(s) : FID2B.ch
 Acq On : 04 Mar 2019 18:08
 Operator : AJ\SJ
 Sample : PB117553BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 04 23:56:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.594	1911506	13.729 ug/ml
Target Compounds			
2) N-DECANE	4.323	2239583	14.560 ug/ml
3) N-DODECANE	6.343	2301108	14.745 ug/ml
4) N-TETRADECANE	8.136	2403052	14.988 ug/ml
5) N-HEXADECANE	9.737	2449678	15.041 ug/ml
6) N-OCTADECANE	11.180	2461157	14.938 ug/ml
7) N-EICOSANE	12.491	2448789	14.969 ug/ml
8) N-DOCOSANE	13.692	2408692	14.925 ug/ml
10) N-TETRACOSANE	14.798	2372777	14.997 ug/ml
11) N-HEXACOSANE	15.823	2283302	14.794 ug/ml
12) N-OCTACOSANE	16.775	2218094	14.678 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030419\
Data File : FF03695.D
Signal(s) : FID2B.ch
Acq On : 04 Mar 2019 18:08
Operator : AJ\SJ
Sample : PB117553BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 04 23:56:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

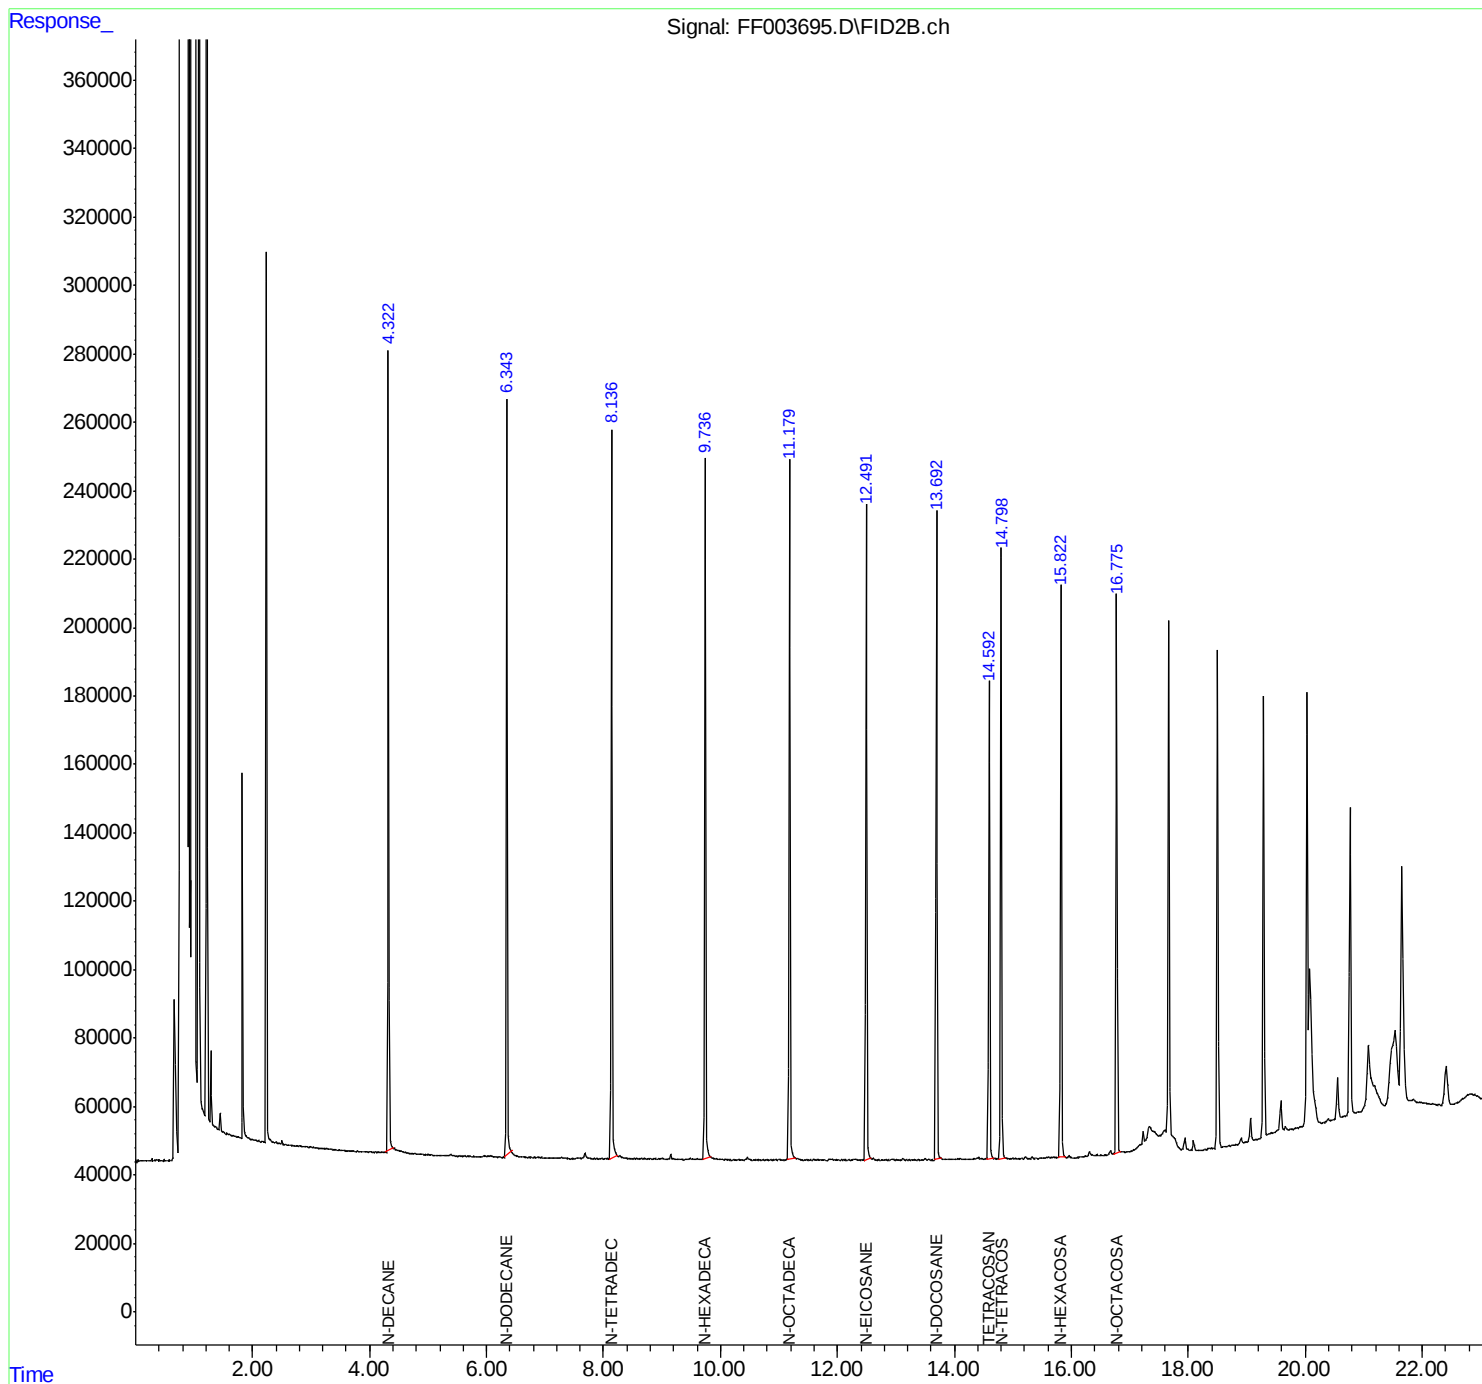

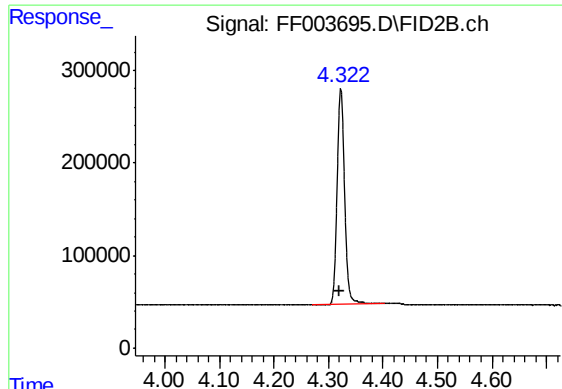


#2 N-DECANE

R.T.: 4.323 min
Delta R.T.: 0.002 min
Response: 2239583
Conc: 14.56 ug/ml

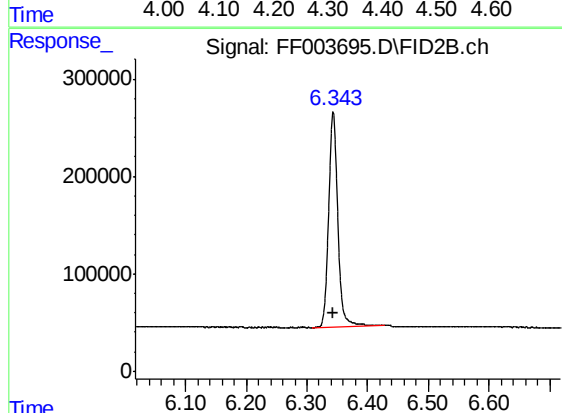


#3 N-DODECANE

R.T.: 6.343 min
Delta R.T.: 0.000 min
Response: 2301108
Conc: 14.74 ug/ml

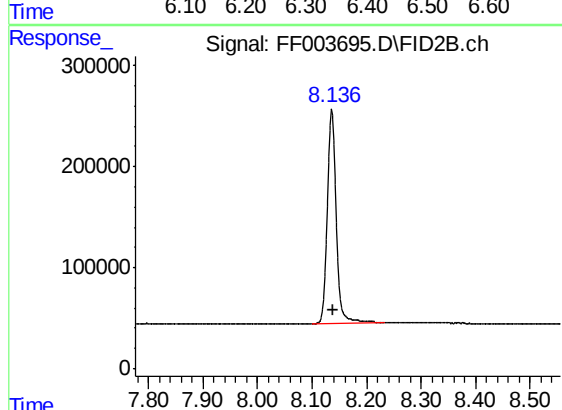


#4 N-TETRADECANE

R.T.: 8.136 min
Delta R.T.: -0.002 min
Response: 2403052
Conc: 14.99 ug/ml

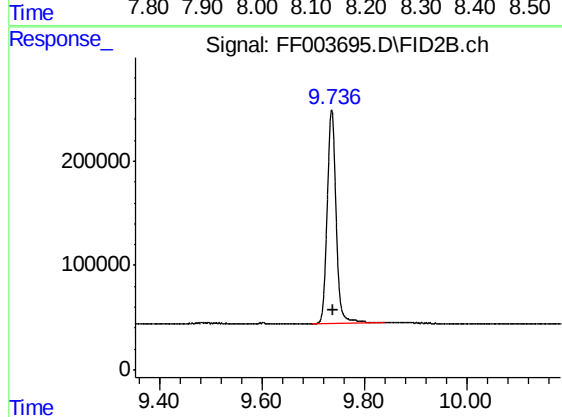


#5 N-HEXADECANE

R.T.: 9.737 min
Delta R.T.: -0.004 min
Response: 2449678
Conc: 15.04 ug/ml

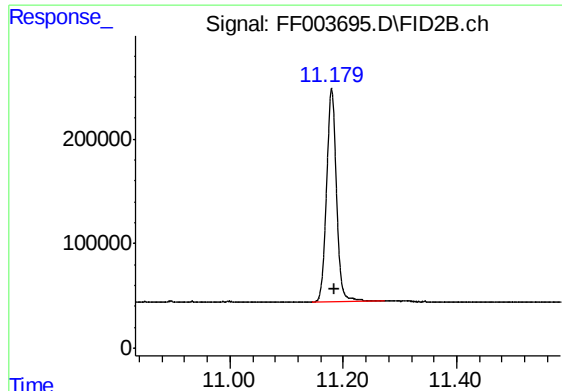


#6 N-OCTADECANE

R.T.: 11.180 min
Delta R.T.: -0.004 min
Response: 2461157
Conc: 14.94 ug/ml

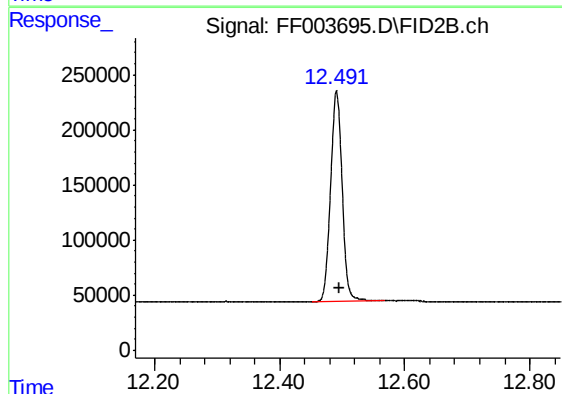


#7 N-EICOSANE

R.T.: 12.491 min
Delta R.T.: -0.005 min
Response: 2448789
Conc: 14.97 ug/ml

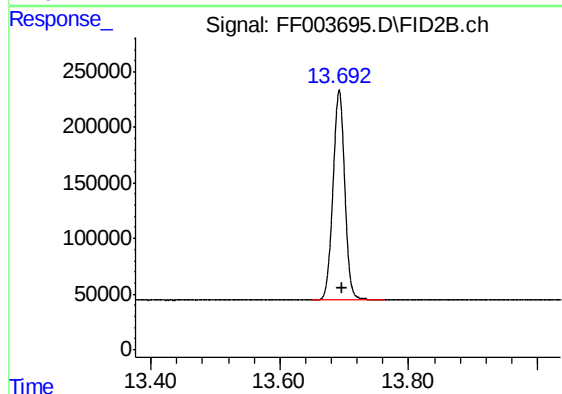


#8 N-DOCOSANE

R.T.: 13.692 min
Delta R.T.: -0.004 min
Response: 2408692
Conc: 14.92 ug/ml

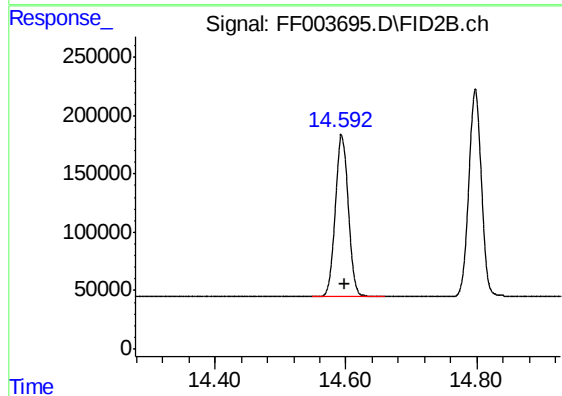


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.594 min
Delta R.T.: -0.005 min
Response: 1911506
Conc: 13.73 ug/ml

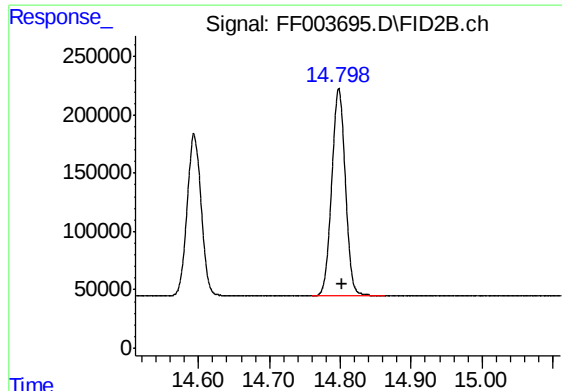


#10 N-TETRACOSANE

R.T.: 14.798 min
Delta R.T.: -0.004 min
Response: 2372777
Conc: 15.00 ug/ml

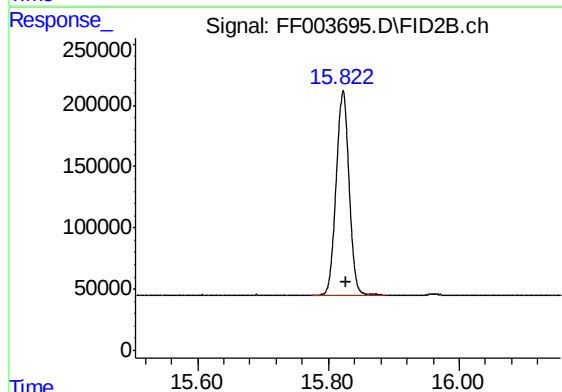

#11 N-HEXACOSANE

R.T.: 15.823 min
Delta R.T.: -0.004 min
Response: 2283302
Conc: 14.79 ug/ml

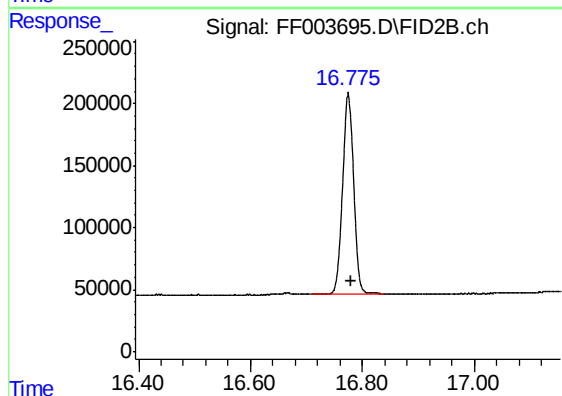

#12 N-OCTACOSANE

R.T.: 16.775 min
Delta R.T.: -0.005 min
Response: 2218094
Conc: 14.68 ug/ml