

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030419\
 Data File : FF003698.D
 Signal(s) : FID2B.ch
 Acq On : 04 Mar 2019 19:38
 Operator : AJ\SJ
 Sample : K1665-01MSD
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 04 23:57:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.593	2199219	15.796 ug/ml
Target Compounds			
2) N-DECANE	4.322	2261856	14.705 ug/ml
3) N-DODECANE	6.343	2398749	15.370 ug/ml
4) N-TETRADECANE	8.135	2477417	15.452 ug/ml
5) N-HEXADECANE	9.736	2678098	16.443 ug/ml
6) N-OCTADECANE	11.179	2665128	16.176 ug/ml
7) N-EICOSANE	12.490	2714384	16.592 ug/ml
8) N-DOCOSANE	13.691	2667912	16.531 ug/ml
10) N-TETRACOSANE	14.797	3237163	20.460 ug/ml
11) N-HEXACOSANE	15.820	2723160	17.644 ug/ml
12) N-OCTACOSANE	16.773	2851751	18.872 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030419\
Data File : FF03698.D
Signal(s) : FID2B.ch
Acq On : 04 Mar 2019 19:38
Operator : AJ\SJ
Sample : K1665-01MSD
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 04 23:57:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

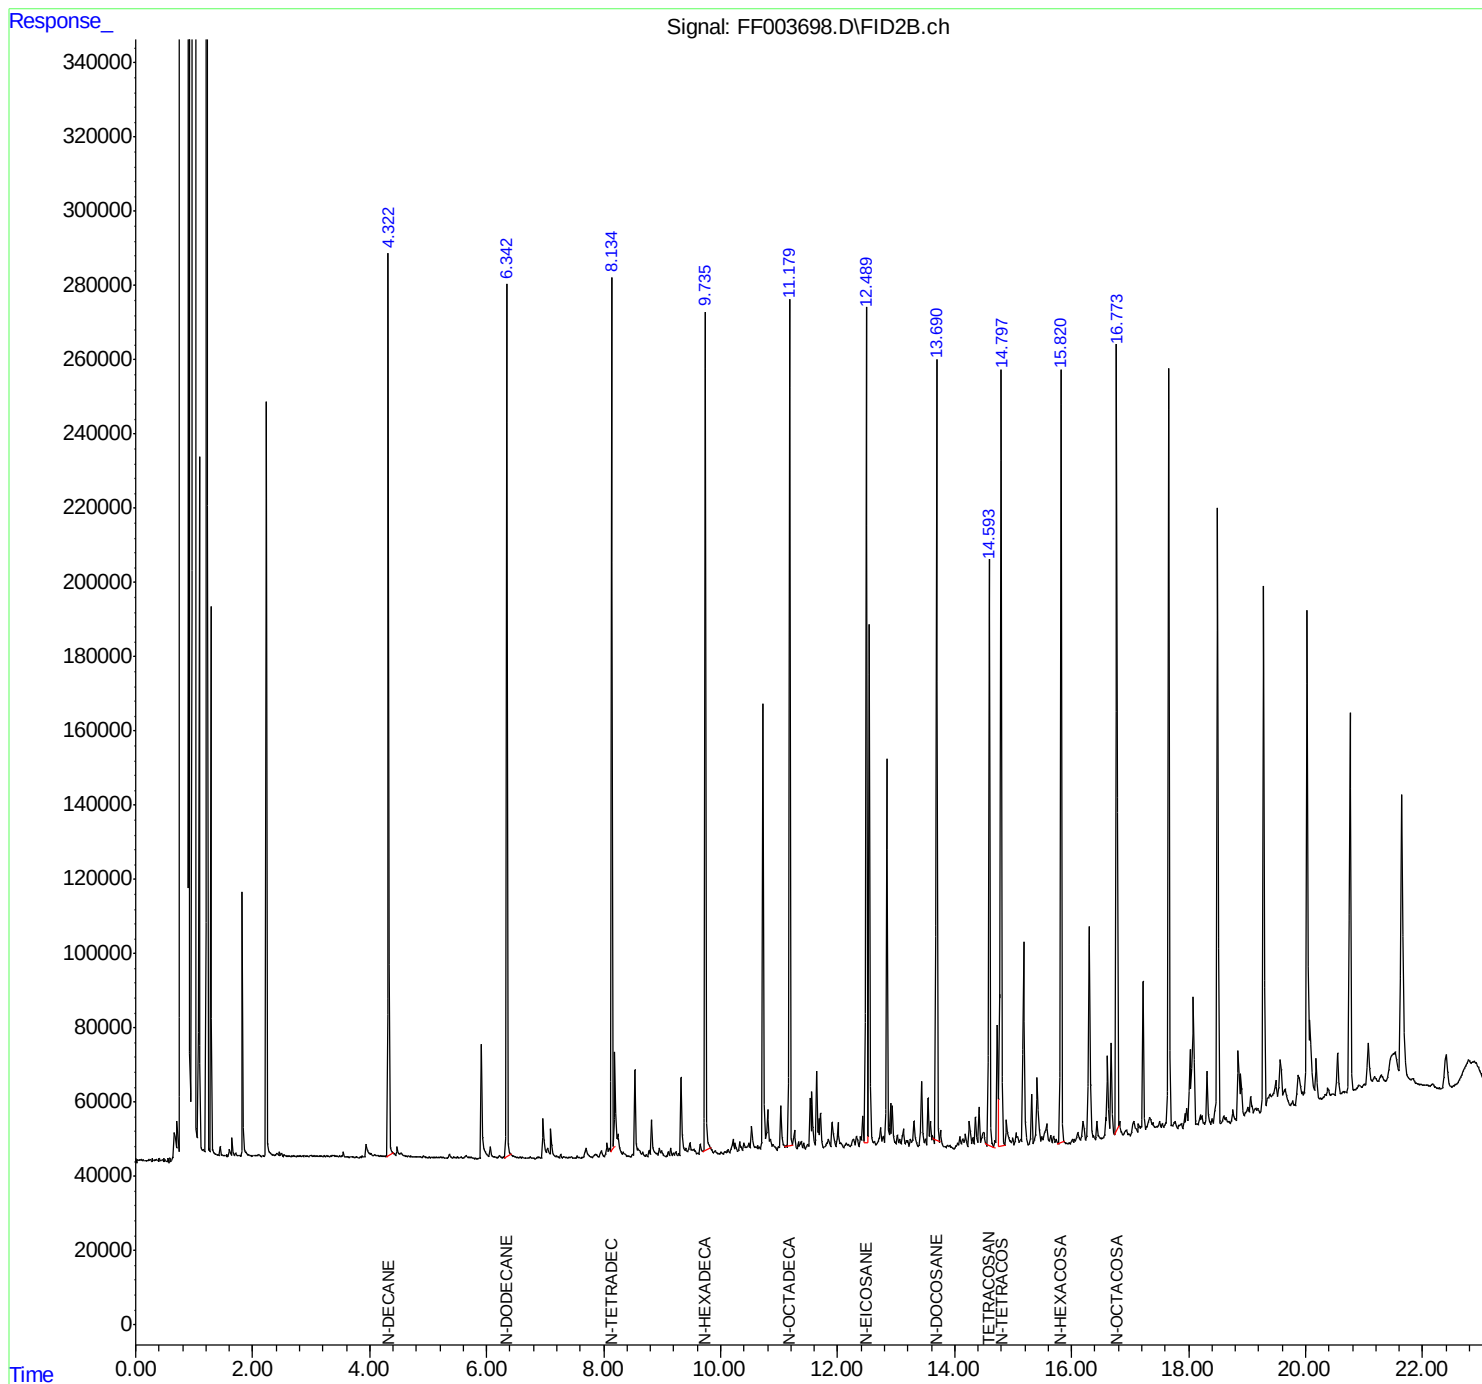

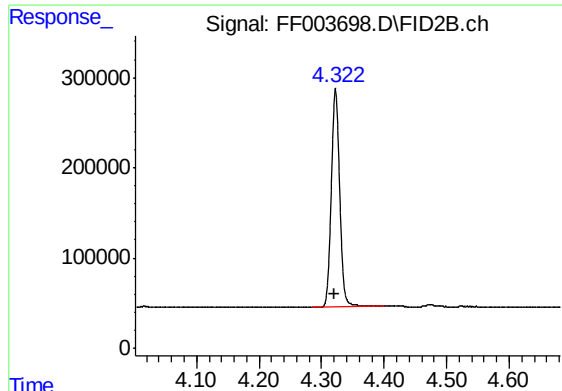


#2 N-DECANE

R.T.: 4.322 min
Delta R.T.: 0.002 min
Response: 2261856
Conc: 14.70 ug/ml

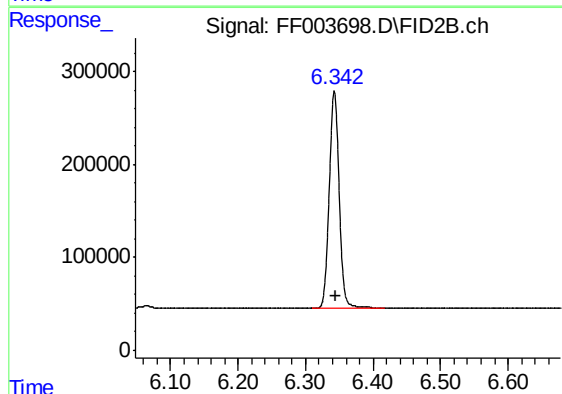


#3 N-DODECANE

R.T.: 6.343 min
Delta R.T.: -0.001 min
Response: 2398749
Conc: 15.37 ug/ml

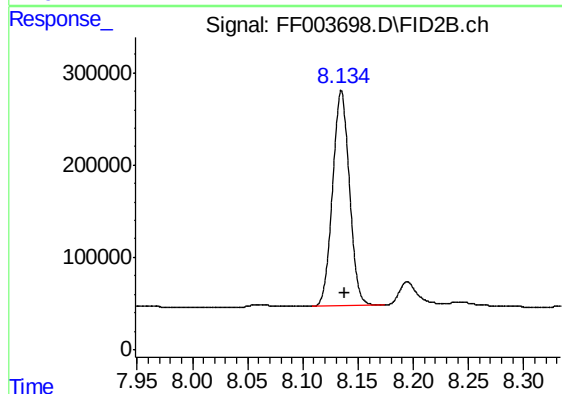


#4 N-TETRADECANE

R.T.: 8.135 min
Delta R.T.: -0.003 min
Response: 2477417
Conc: 15.45 ug/ml

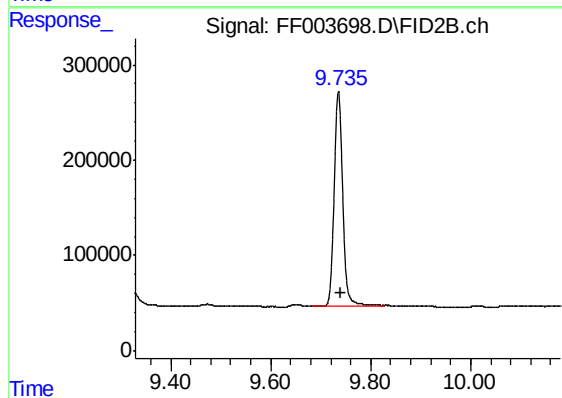


#5 N-HEXADECANE

R.T.: 9.736 min
Delta R.T.: -0.005 min
Response: 2678098
Conc: 16.44 ug/ml

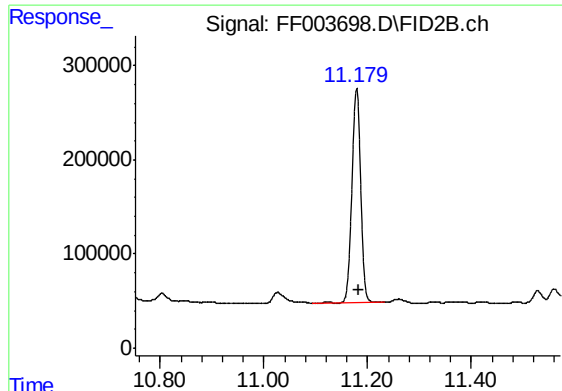


#6 N-OCTADECANE

R.T.: 11.179 min
Delta R.T.: -0.005 min
Response: 2665128
Conc: 16.18 ug/ml

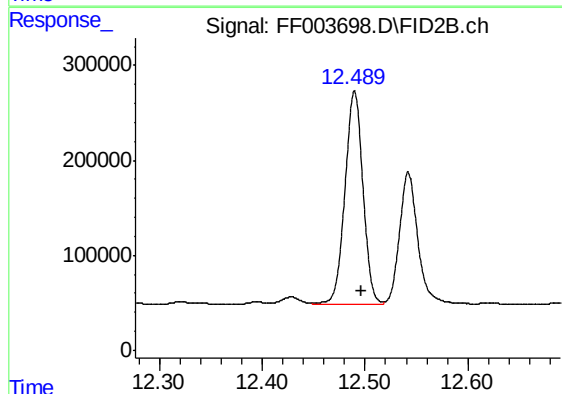


#7 N-EICOSANE

R.T.: 12.490 min
Delta R.T.: -0.007 min
Response: 2714384
Conc: 16.59 ug/ml

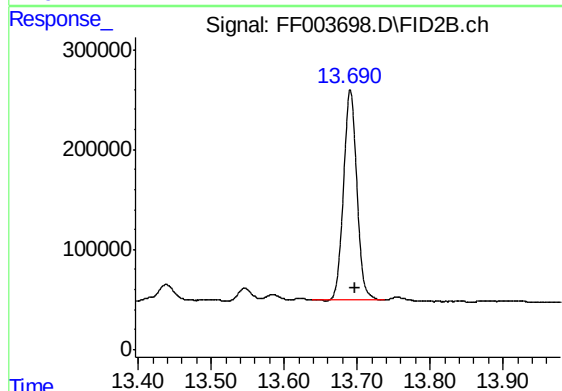


#8 N-DOCOSANE

R.T.: 13.691 min
Delta R.T.: -0.006 min
Response: 2667912
Conc: 16.53 ug/ml

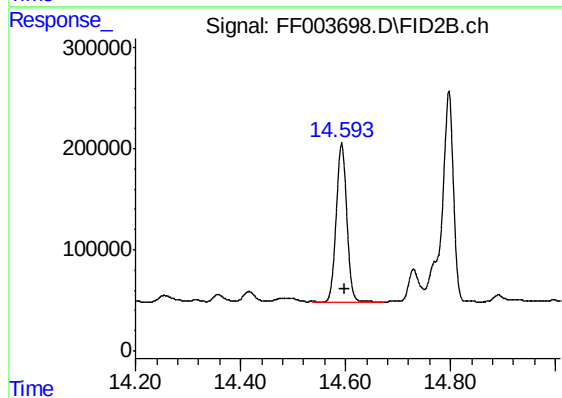


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.593 min
Delta R.T.: -0.006 min
Response: 2199219
Conc: 15.80 ug/ml

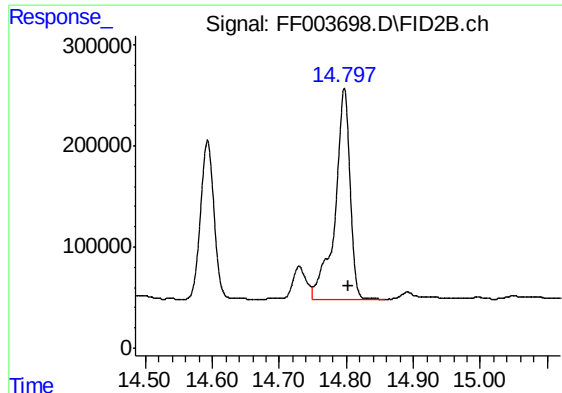


#10 N-TETRACOSANE

R.T.: 14.797 min
Delta R.T.: -0.005 min
Response: 3237163
Conc: 20.46 ug/ml

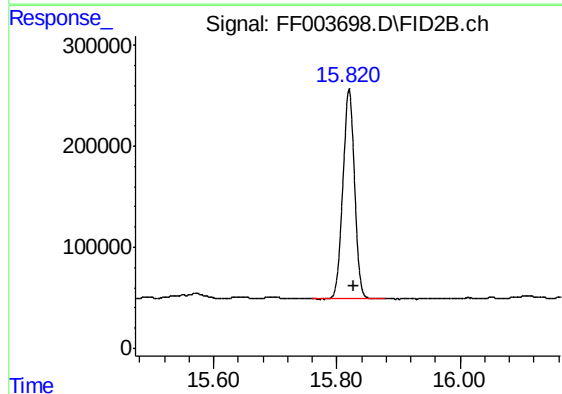

#11 N-HEXACOSANE

R.T.: 15.820 min
Delta R.T.: -0.007 min
Response: 2723160
Conc: 17.64 ug/ml

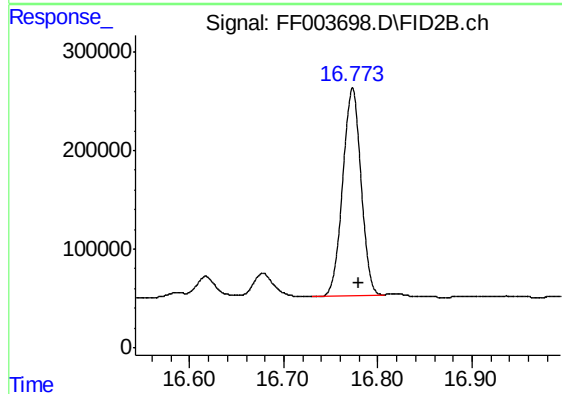

#12 N-OCTACOSANE

R.T.: 16.773 min
Delta R.T.: -0.006 min
Response: 2851751
Conc: 18.87 ug/ml