

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030519\
Data File : FF003722.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2019 09:59
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 06 00:01:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.515	261954	1.842 ug/ml
16) N-HEXATRIACONTANE	20.075	1227925	9.411 ug/ml
18) N-TETRACONTANE	21.686	1326444	10.662 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030519\
Data File : FF003722.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2019 09:59
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 06 00:01:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

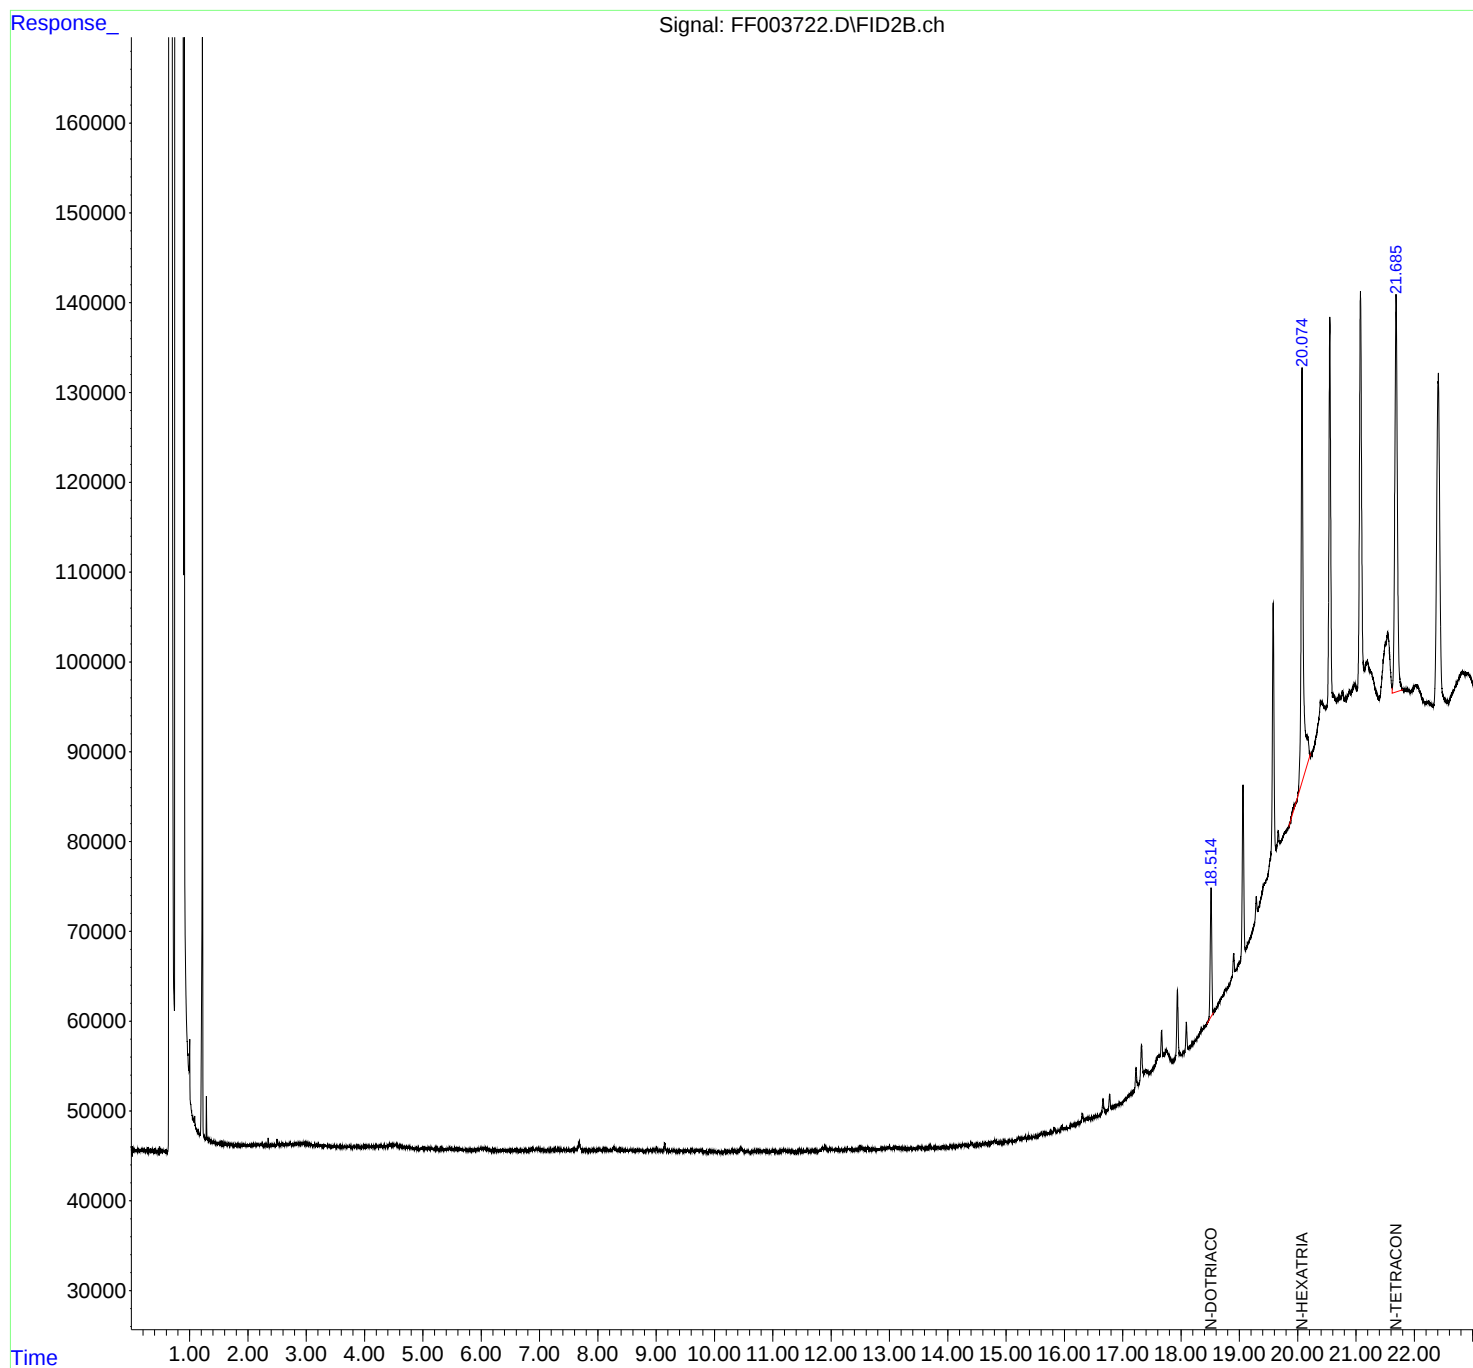


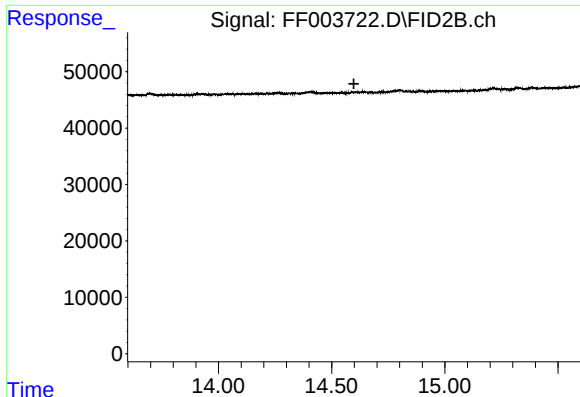

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.598 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

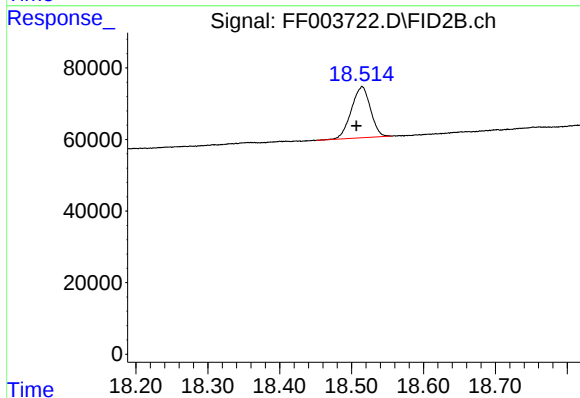


#14 N-DOTRIACONTANE

R.T.: 18.515 min
Delta R.T.: 0.008 min
Response: 261954
Conc: 1.84 ug/ml

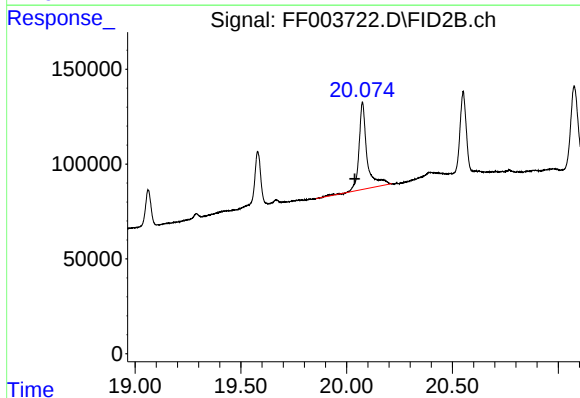

#16 N-HEXATRIACONTANE

R.T.: 20.075 min
Delta R.T.: 0.037 min
Response: 1227925
Conc: 9.41 ug/ml

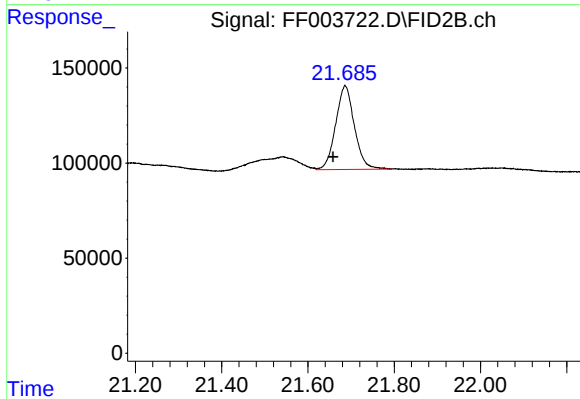

#18 N-TETRACONTANE

R.T.: 21.686 min
Delta R.T.: 0.027 min
Response: 1326444
Conc: 10.66 ug/ml