

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030519\
Data File : FF003723.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2019 12:48
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 06 00:01:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.593	2299452	16.516 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.667	93374	0.635 ug/ml
14) N-DOTRIACONTANE	18.514	280098	1.970 ug/ml
16) N-HEXATRIACONTANE	20.081	463743	3.554 ug/ml
18) N-TETRACONTANE	21.692	724945	5.827 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030519\
Data File : FF003723.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2019 12:48
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 06 00:01:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

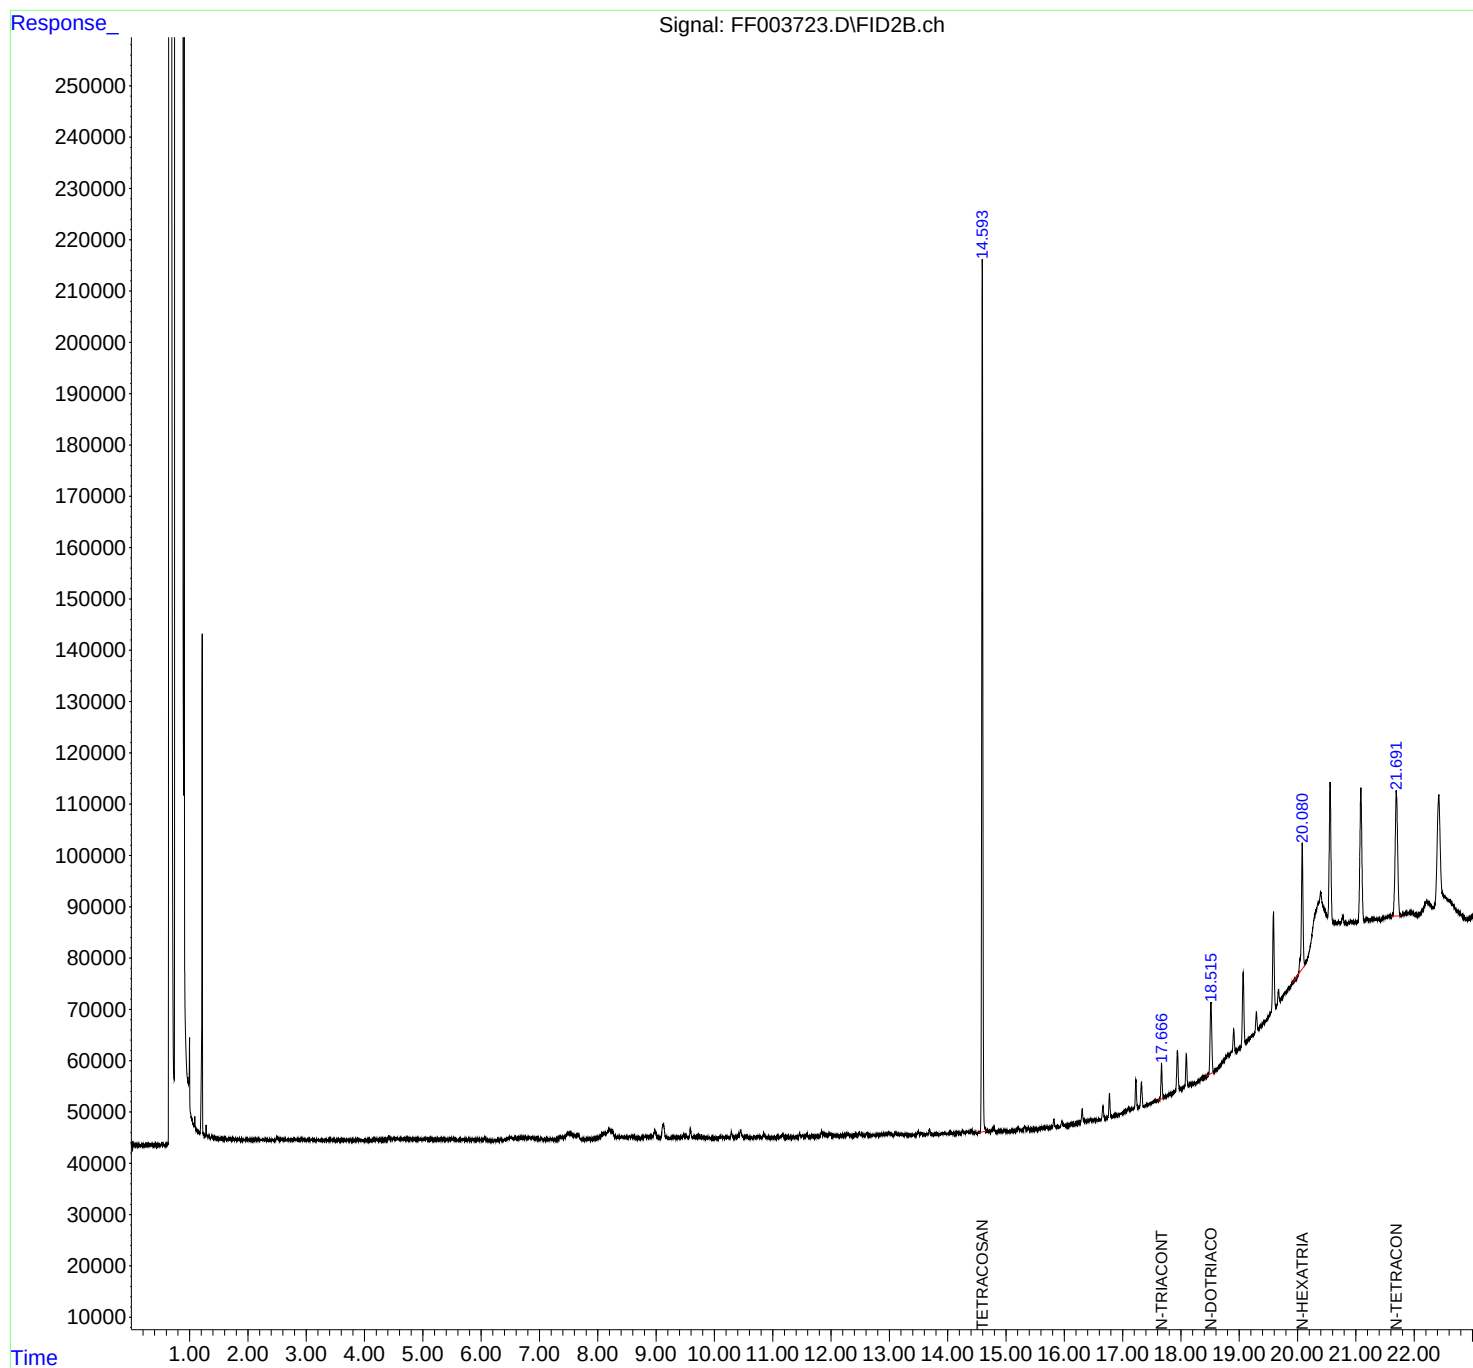


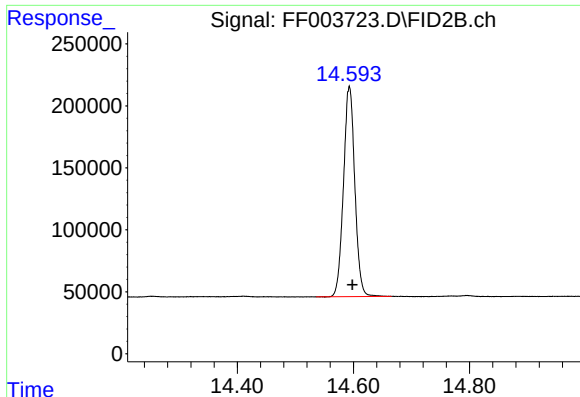

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.593 min
Delta R.T.: -0.005 min
Response: 2299452
Conc: 16.52 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

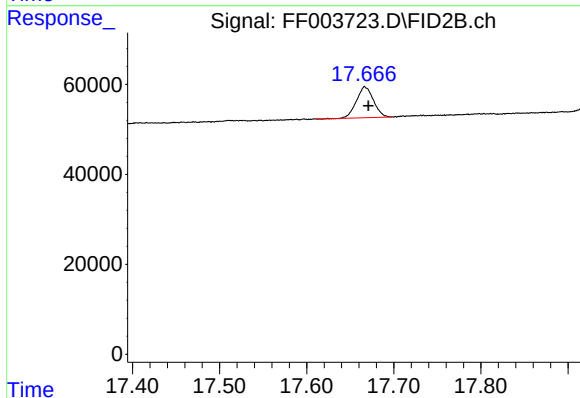


#13 N-TRIACONTANE

R.T.: 17.667 min
Delta R.T.: -0.004 min
Response: 93374
Conc: 0.63 ug/ml

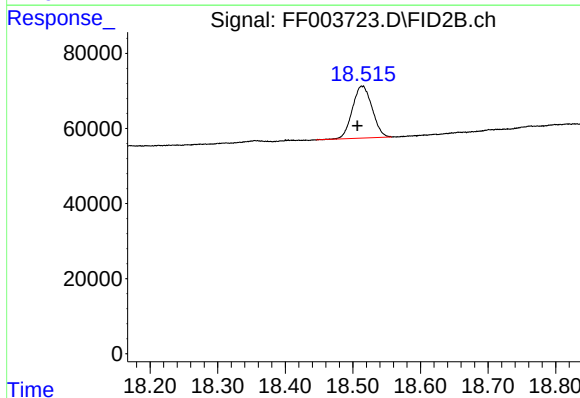


#14 N-DOTRIACONTANE

R.T.: 18.514 min
Delta R.T.: 0.007 min
Response: 280098
Conc: 1.97 ug/ml

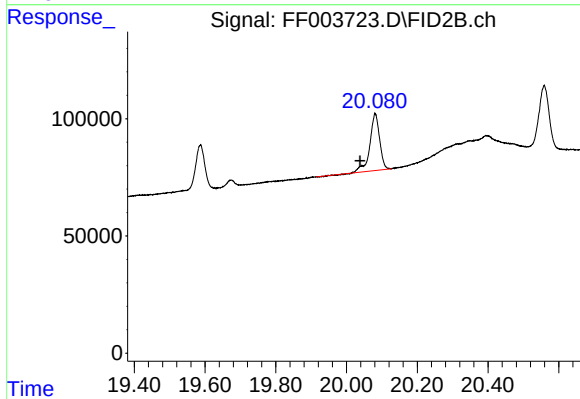

#16 N-HEXATRIACONTANE

R.T.: 20.081 min
Delta R.T.: 0.043 min
Response: 463743
Conc: 3.55 ug/ml

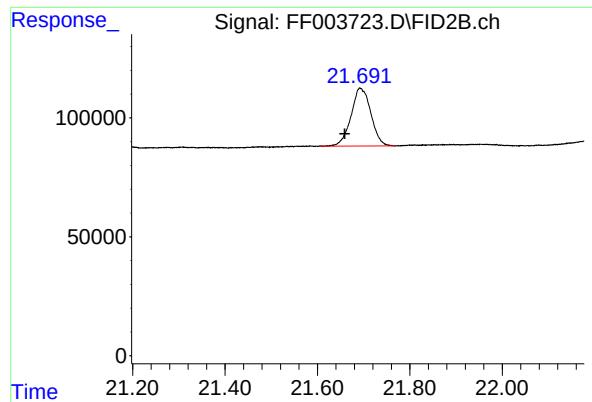

#18 N-TETRACONTANE

R.T.: 21.692 min
Delta R.T.: 0.034 min
Response: 724945
Conc: 5.83 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK