

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030519\
Data File : FF003725.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2019 13:48
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 06 00:01:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.344	3744857	23.996 ug/ml
12)	N-OCTACOSANE	16.777	3612655	23.907 ug/ml
13)	N-TRIACONTANE	17.665	644202	4.379 ug/ml
14)	N-DOTRIACONTANE	18.501	776571	5.461 ug/ml
15)	N-TETRATRIACONTANE	19.289	545167	4.072 ug/ml
16)	N-HEXATRIACONTANE	20.035	380132	2.913 ug/ml
17)	N-OCTATRIACONTANE	20.767	219374	1.900 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030519\
Data File : FF003725.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2019 13:48
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 06 00:01:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

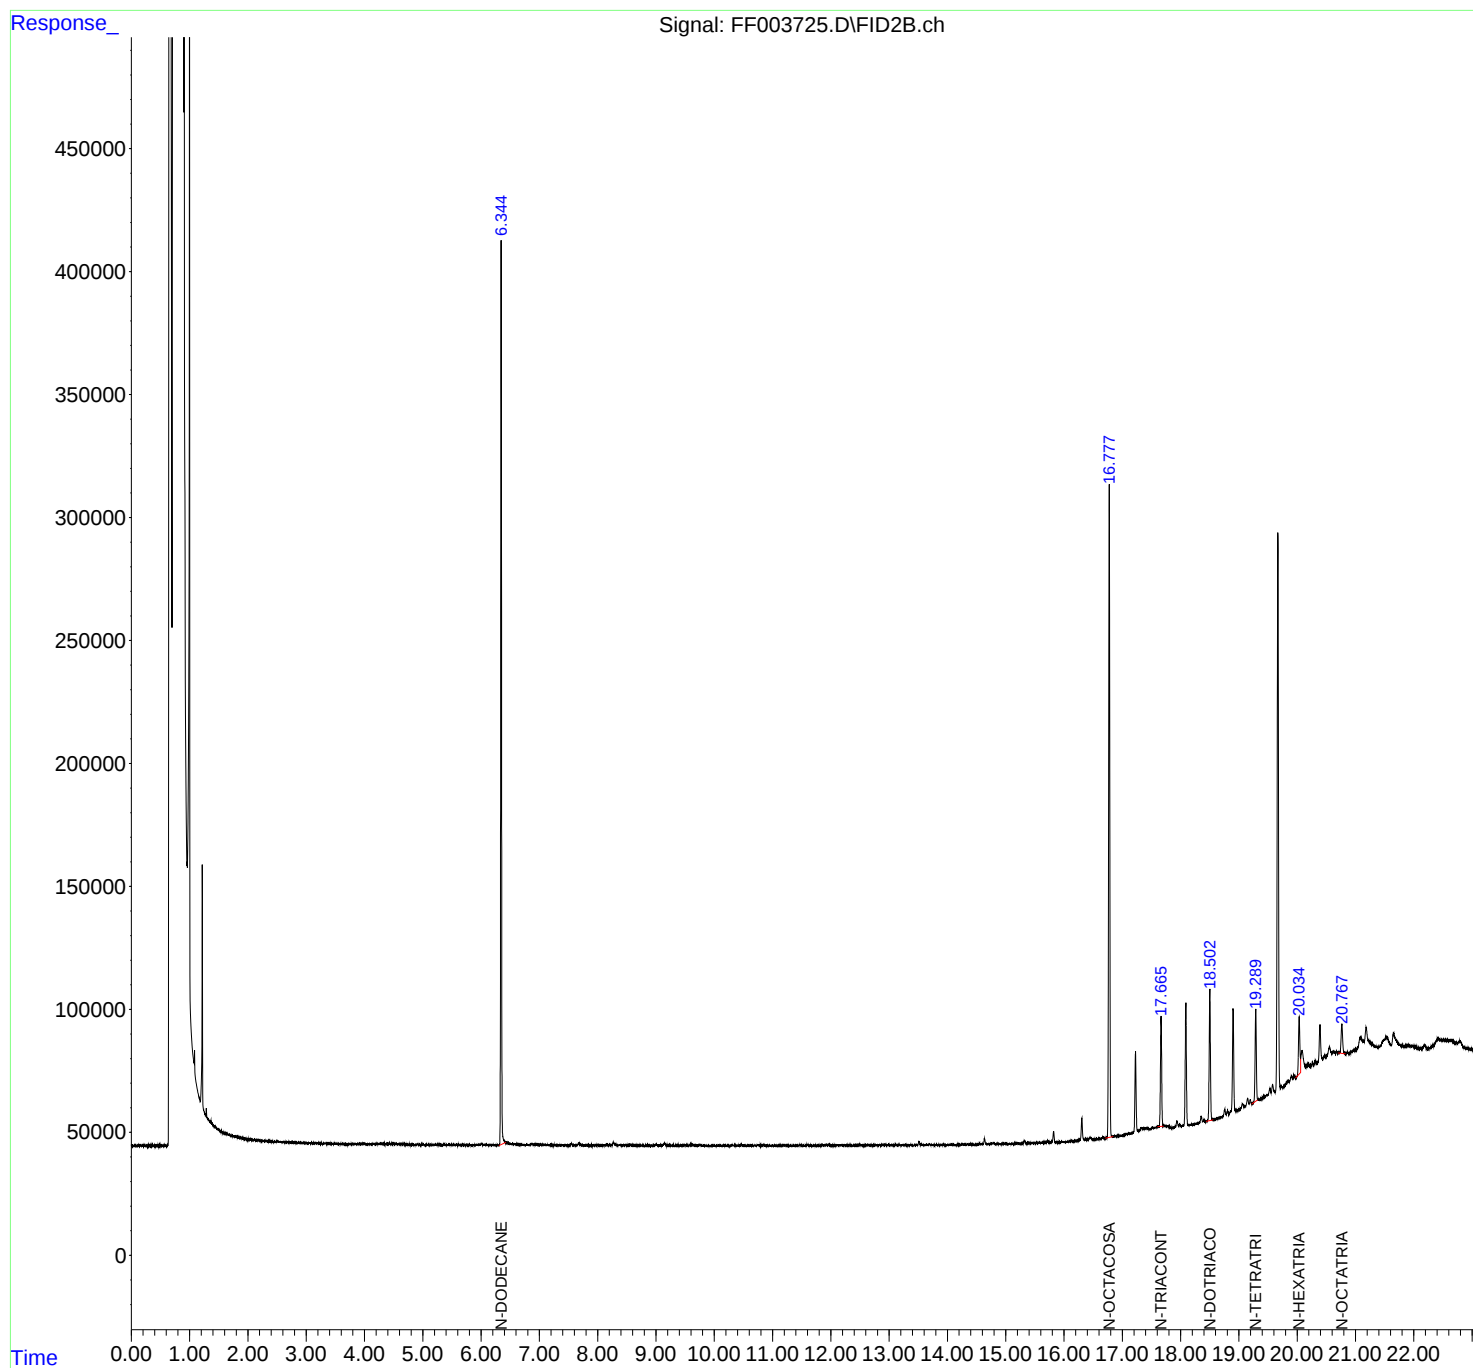


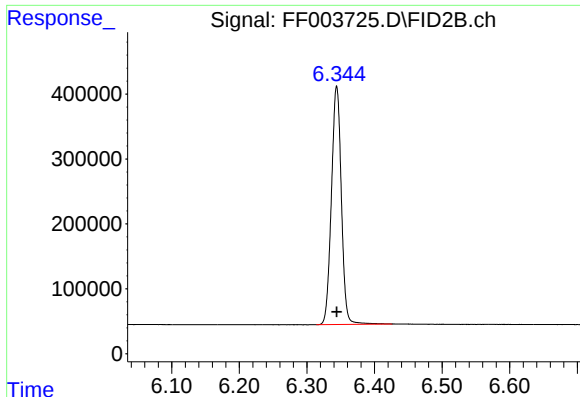

#3 N-DODECANE


R.T.: 6.344 min
Delta R.T.: 0.000 min
Response: 3744857
Conc: 24.00 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

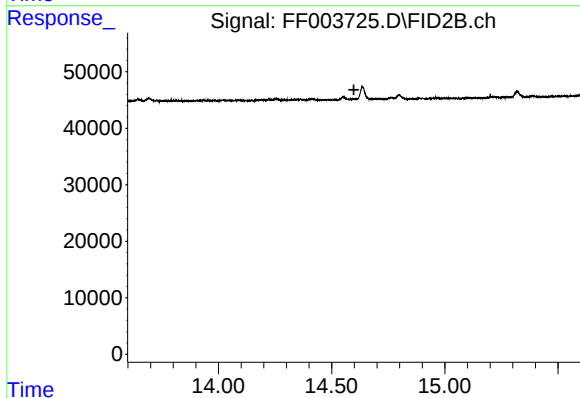


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.598 min
Response: 0
Conc: N.D.

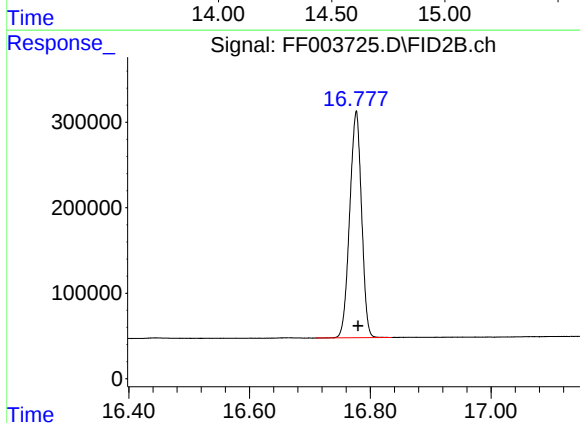


#12 N-OCTACOSANE

R.T.: 16.777 min
Delta R.T.: -0.003 min
Response: 3612655
Conc: 23.91 ug/ml

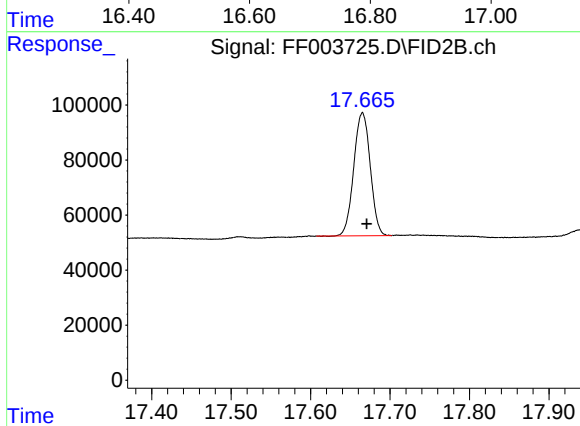

#13 N-TRIACONTANE


R.T.: 17.665 min
Delta R.T.: -0.006 min
Response: 644202
Conc: 4.38 ug/ml

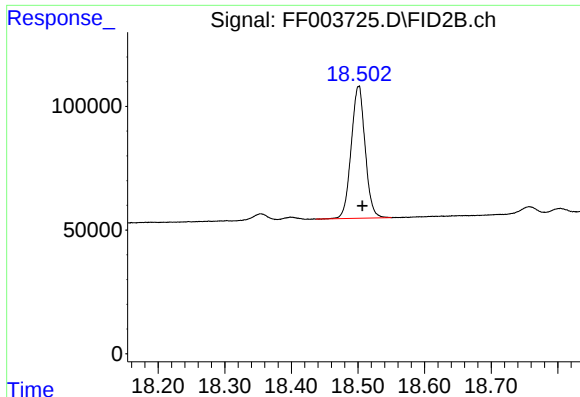

#14 N-DOTRIACONTANE


R.T.: 18.501 min
Delta R.T.: -0.006 min
Response: 776571
Conc: 5.46 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

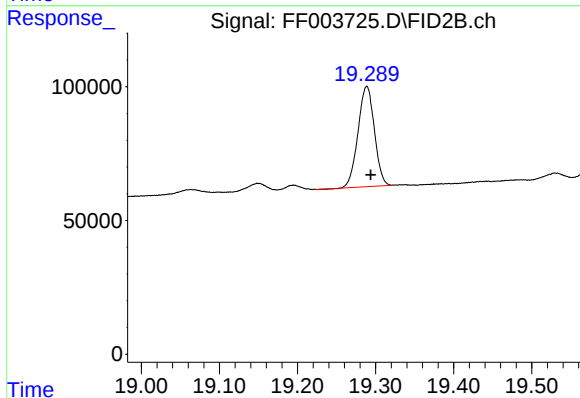


#15 N-TETRATRIACONTANE

R.T.: 19.289 min
Delta R.T.: -0.005 min
Response: 545167
Conc: 4.07 ug/ml

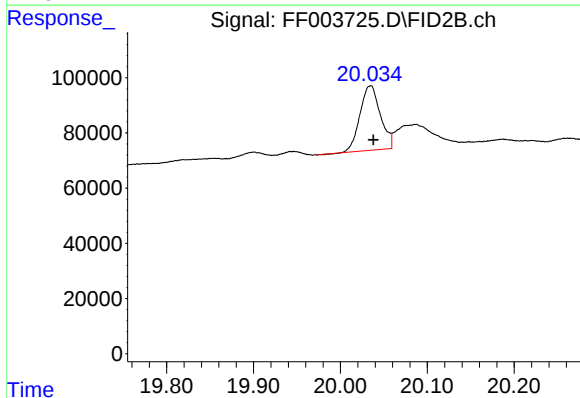

#16 N-HEXATRIACONTANE

R.T.: 20.035 min
Delta R.T.: -0.003 min
Response: 380132
Conc: 2.91 ug/ml

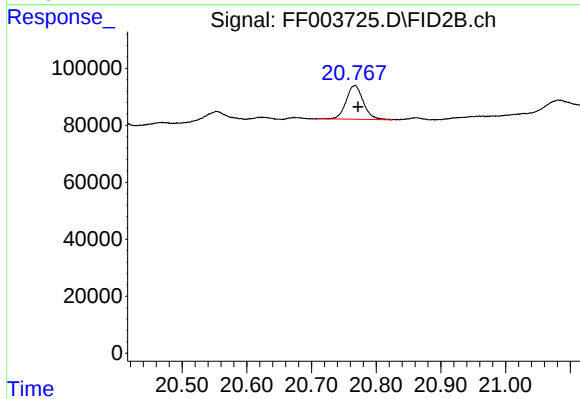

#17 N-OCTATRIACONTANE

R.T.: 20.767 min
Delta R.T.: -0.005 min
Response: 219374
Conc: 1.90 ug/ml