

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030519\
 Data File : FF003731.D
 Signal(s) : FID2B.ch
 Acq On : 05 Mar 2019 16:51
 Operator : AJ\SJ
 Sample : K1715-06 5X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 TP-4-B-D2

Integration File: autoint1.e
 Quant Time: Mar 06 00:03:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.597	322580	2.317 ug/ml
Target Compounds			
11) N-HEXACOSANE	15.827	208334	1.350 ug/ml
12) N-OCTACOSANE	16.782	784278	5.190 ug/ml
13) N-TRIACONTANE	17.670	812233	5.522 ug/ml
14) N-DOTRIACONTANE	18.514	1388387	9.763 ug/ml
15) N-TETRATRIACONTANE	19.302	443810	3.315 ug/ml
16) N-HEXATRIACONTANE	20.047	805955	6.177 ug/ml
17) N-OCTATRIACONTANE	20.782	836062	7.241 ug/ml
18) N-TETRACONTANE	21.674	537410	4.320 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030519\
Data File : FF003731.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2019 16:51
Operator : AJ\SJ
Sample : K1715-06 5X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
TP-4-B-D2

Integration File: autoint1.e
Quant Time: Mar 06 00:03:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

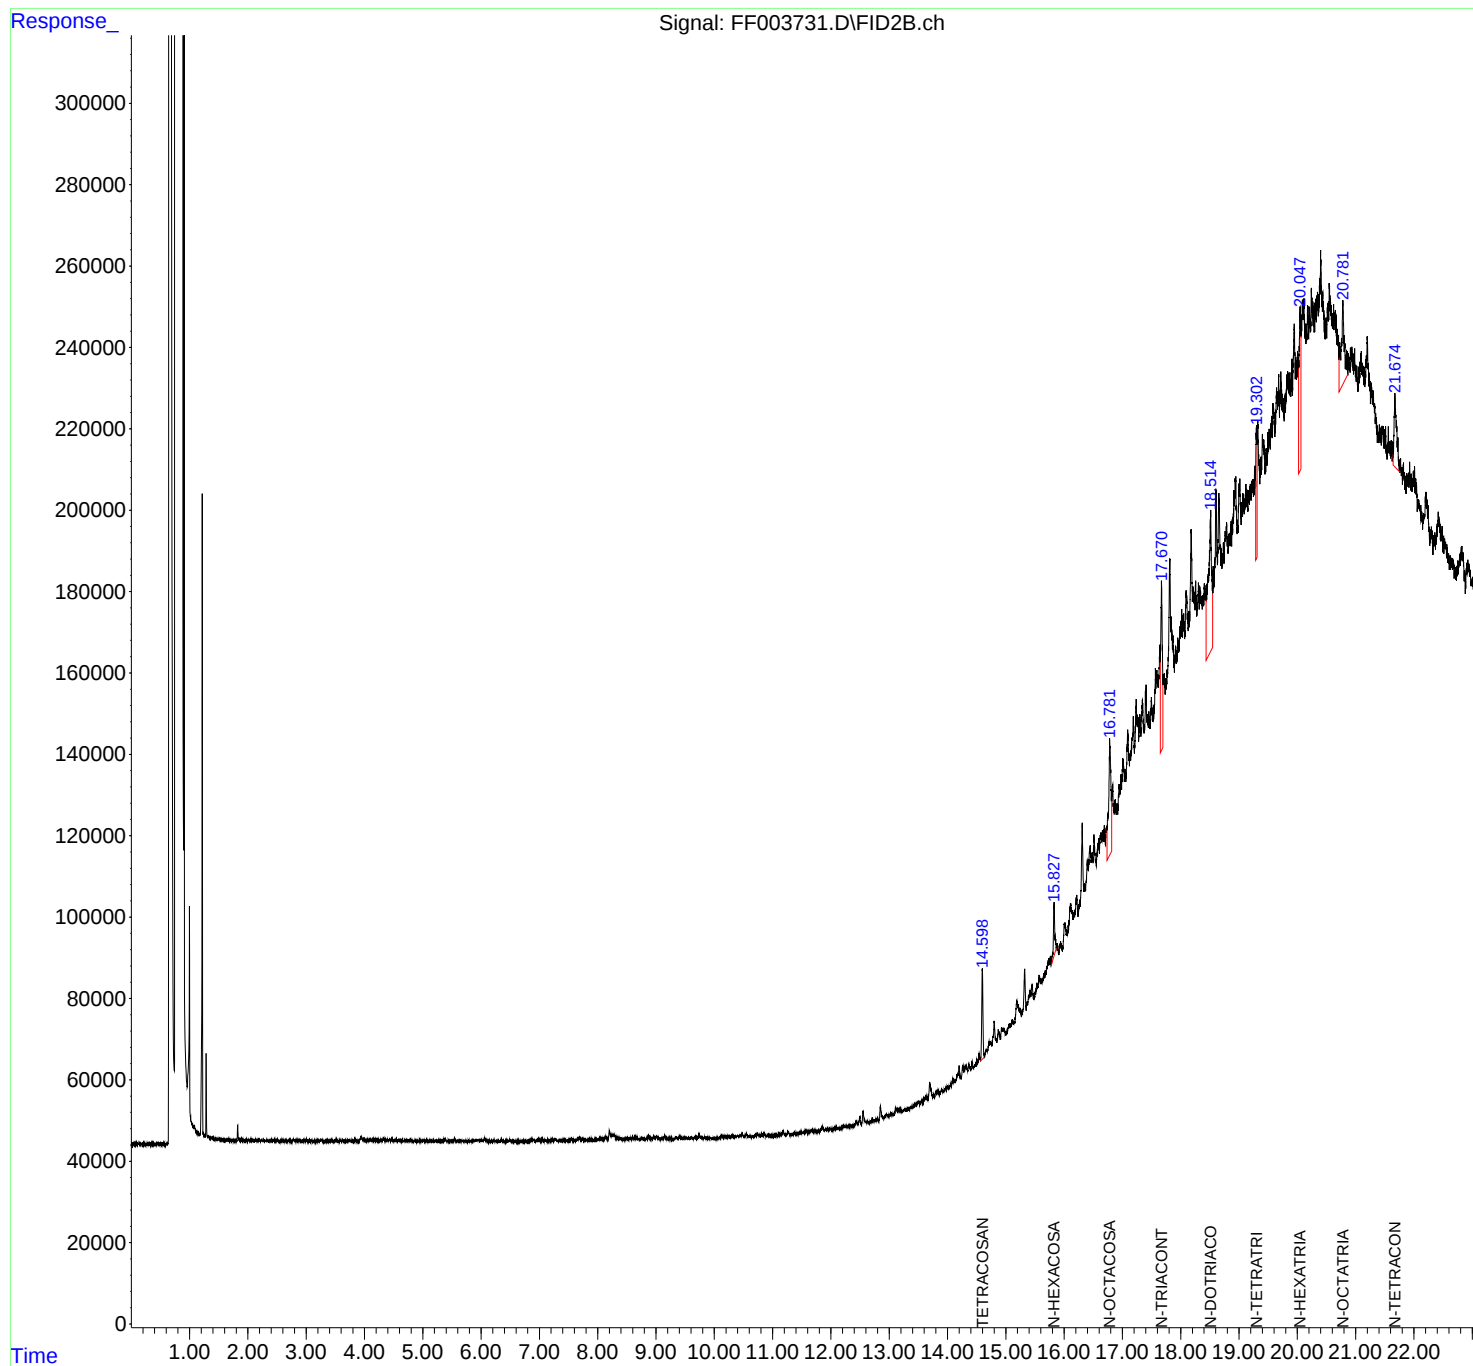


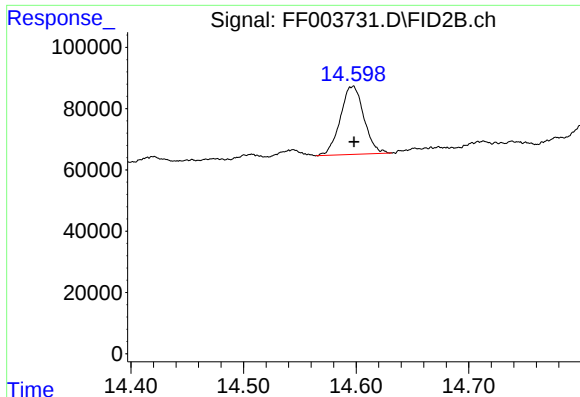

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.597 min
Delta R.T.: -0.001 min
Response: 322580
Conc: 2.32 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-4-B-D2

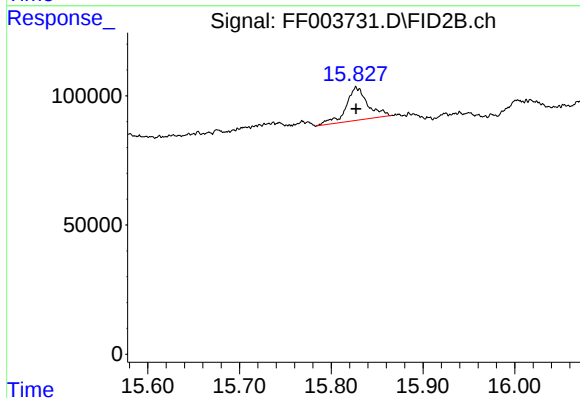


#11 N-HEXACOSANE

R.T.: 15.827 min
Delta R.T.: 0.000 min
Response: 208334
Conc: 1.35 ug/ml

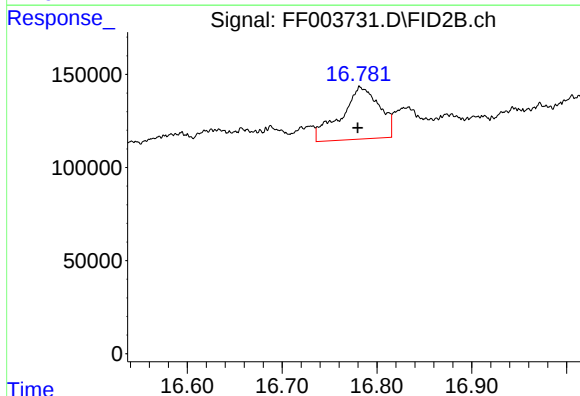


#12 N-OCTACOSANE

R.T.: 16.782 min
Delta R.T.: 0.003 min
Response: 784278
Conc: 5.19 ug/ml

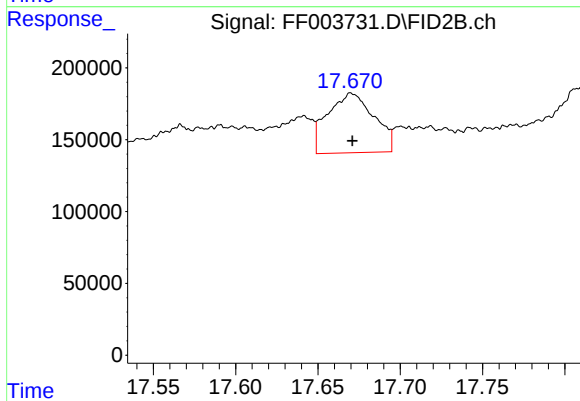

#13 N-TRIACONTANE


R.T.: 17.670 min
Delta R.T.: 0.000 min
Response: 812233
Conc: 5.52 ug/ml

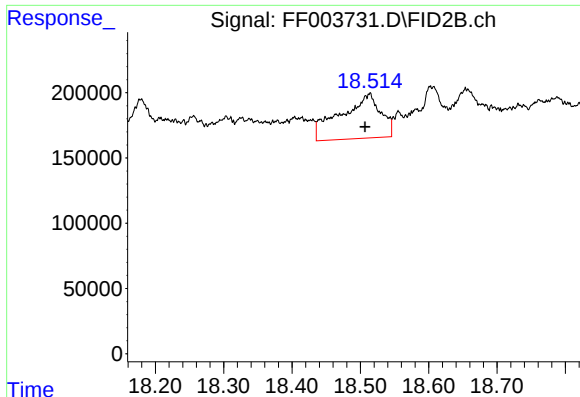

#14 N-DOTRIACONTANE


R.T.: 18.514 min
Delta R.T.: 0.007 min
Response: 1388387
Conc: 9.76 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-4-B-D2

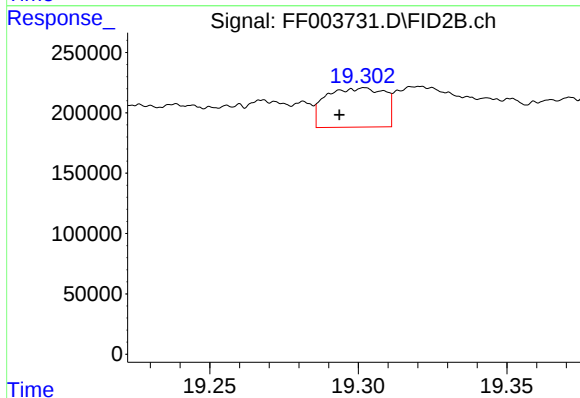


#15 N-TETRATRIACONTANE

R.T.: 19.302 min
Delta R.T.: 0.008 min
Response: 443810
Conc: 3.31 ug/ml

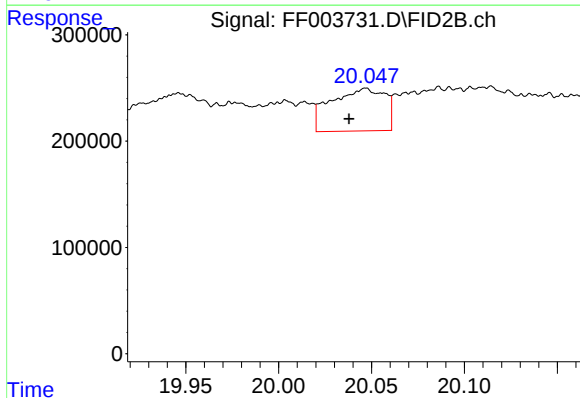


#16 N-HEXATRIACONTANE

R.T.: 20.047 min
Delta R.T.: 0.009 min
Response: 805955
Conc: 6.18 ug/ml

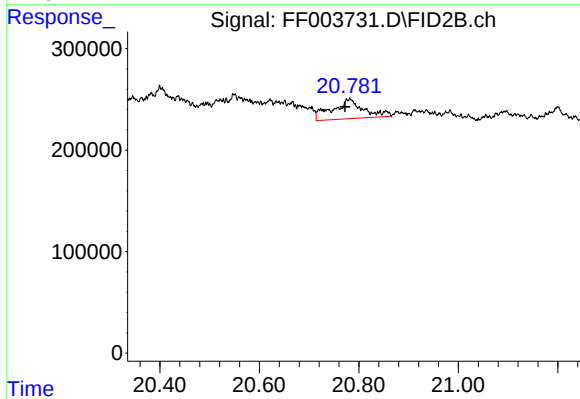

#17 N-OCTATRIACONTANE

R.T.: 20.782 min
Delta R.T.: 0.010 min
Response: 836062
Conc: 7.24 ug/ml

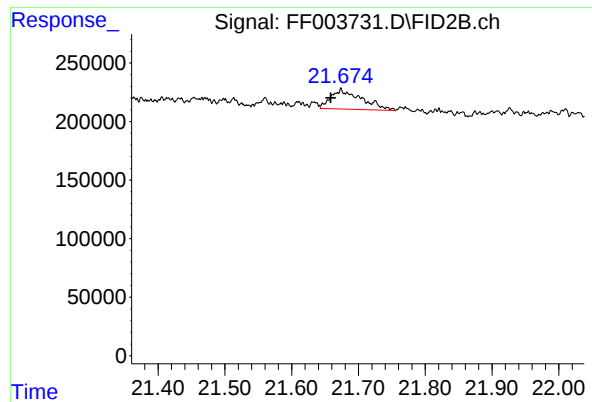

#18 N-TETRACONTANE

R.T.: 21.674 min
Delta R.T.: 0.015 min
Response: 537410
Conc: 4.32 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-4-B-D2