

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030519\
 Data File : FF003732.D
 Signal(s) : FID2B.ch
 Acq On : 05 Mar 2019 17:21
 Operator : AJ\SJ
 Sample : PB117622BL
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB117622BL

Integration File: autoint1.e
 Quant Time: Mar 06 00:04:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.598	1986796	14.270 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.669	73994	0.503 ug/ml
14) N-DOTRIACONTANE	18.515	171825	1.208 ug/ml
16) N-HEXATRIACONTANE	20.042	346018	2.652 ug/ml
17) N-OCTATRIACONTANE	20.770	484487	4.196 ug/ml
18) N-TETRACONTANE	21.691	353663	2.843 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030519\
Data File : FF003732.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2019 17:21
Operator : AJ\SJ
Sample : PB117622BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB117622BL

Integration File: autoint1.e
Quant Time: Mar 06 00:04:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

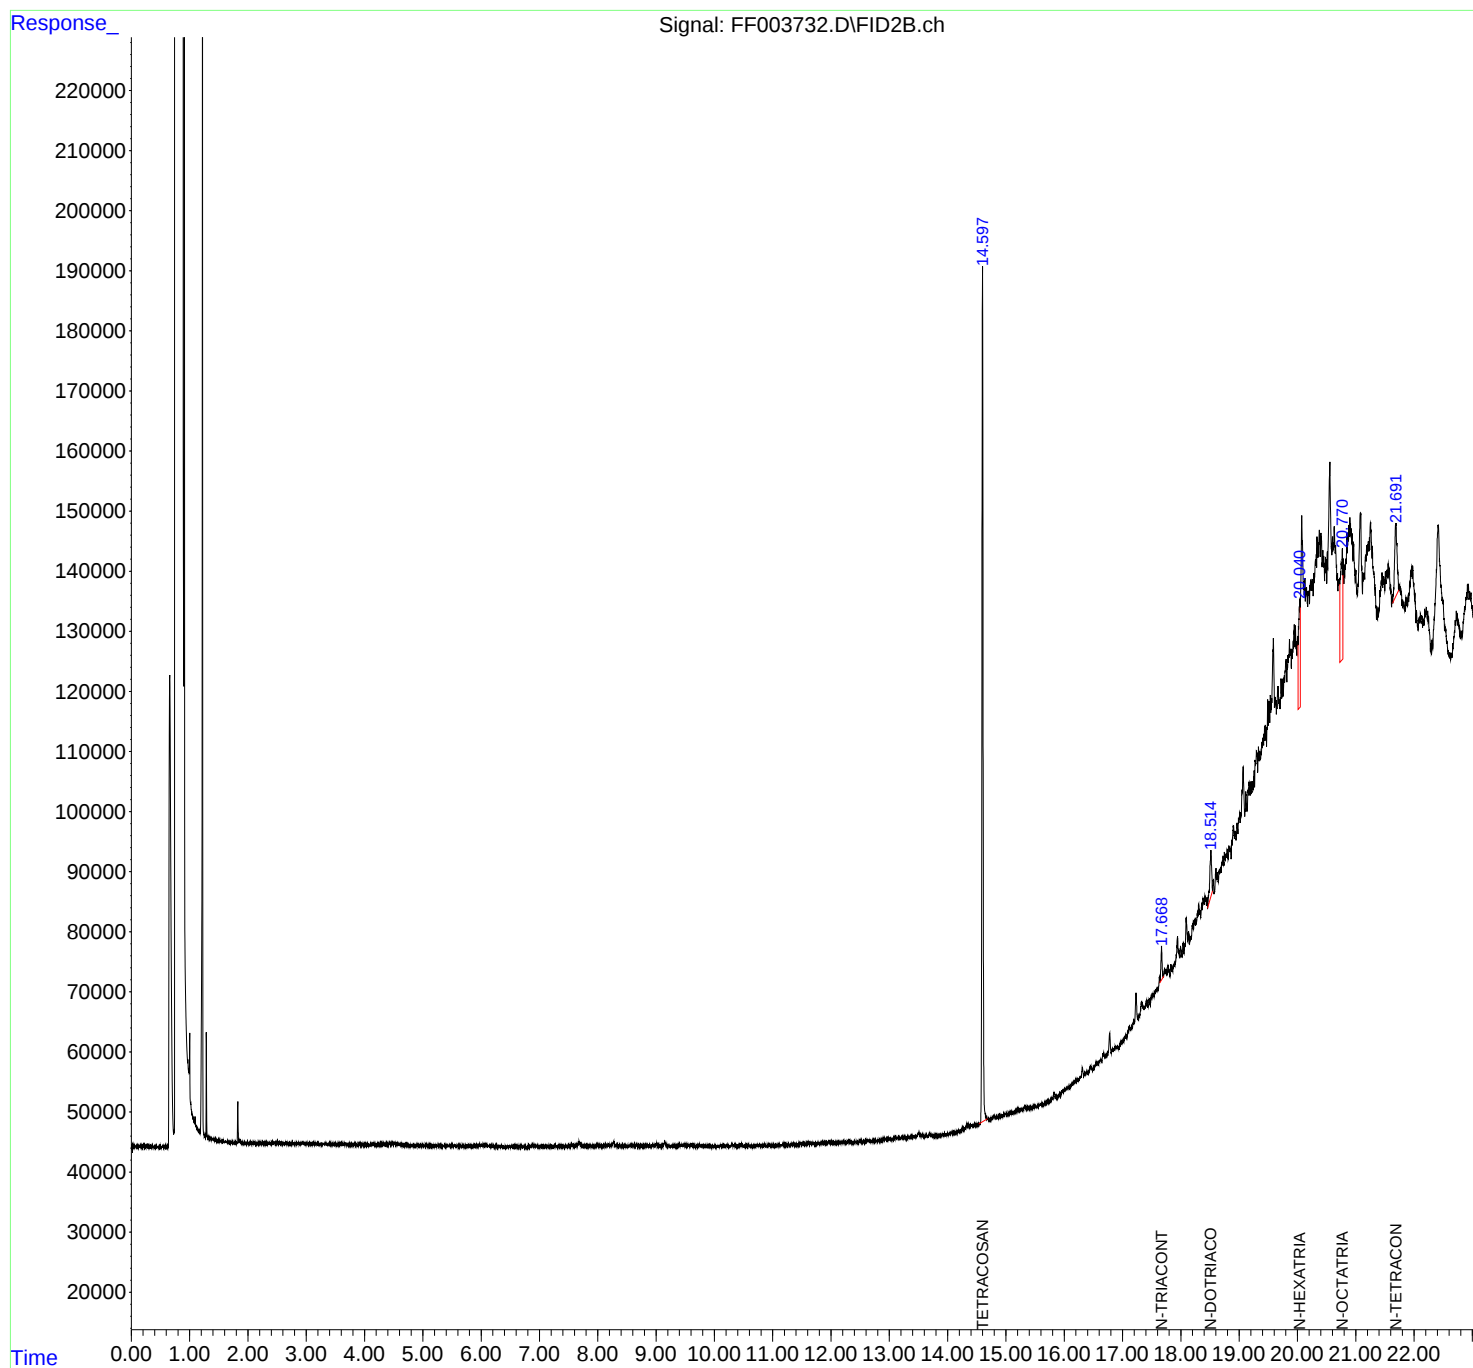


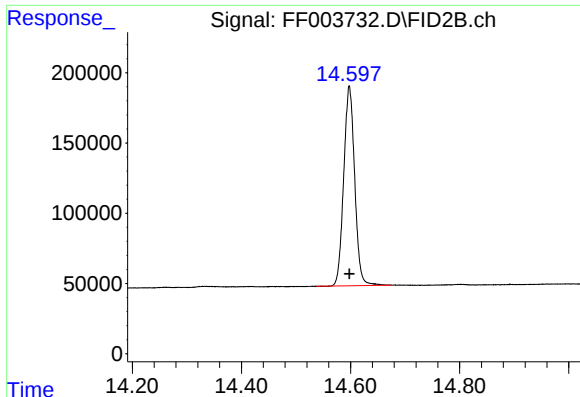

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.598 min
Delta R.T.: 0.000 min
Response: 1986796
Conc: 14.27 ug/ml

Instrument :
FID_F
ClientSampleId :
PB117622BL

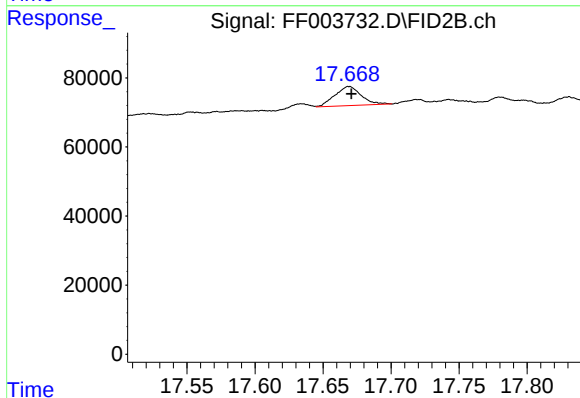


#13 N-TRIACONTANE

R.T.: 17.669 min
Delta R.T.: -0.002 min
Response: 73994
Conc: 0.50 ug/ml

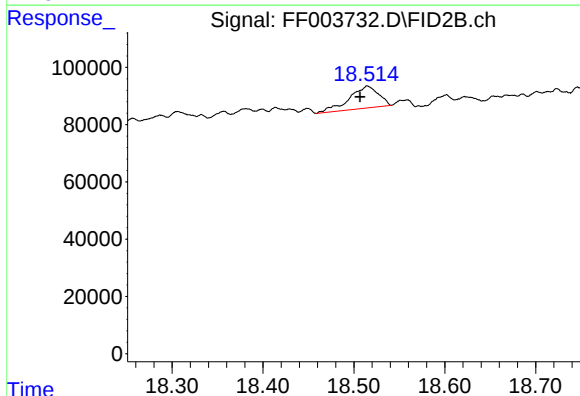


#14 N-DOTRIACONTANE

R.T.: 18.515 min
Delta R.T.: 0.008 min
Response: 171825
Conc: 1.21 ug/ml

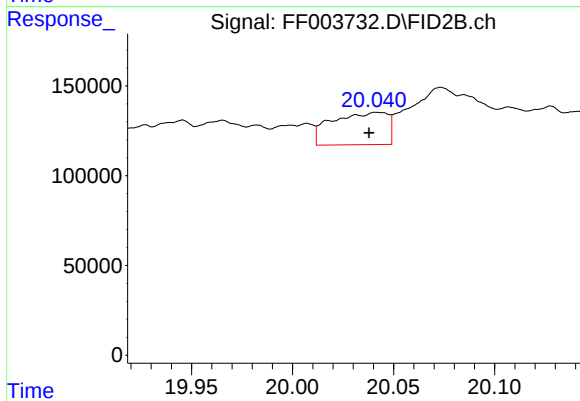

#16 N-HEXATRIACONTANE


R.T.: 20.042 min
Delta R.T.: 0.004 min
Response: 346018
Conc: 2.65 ug/ml

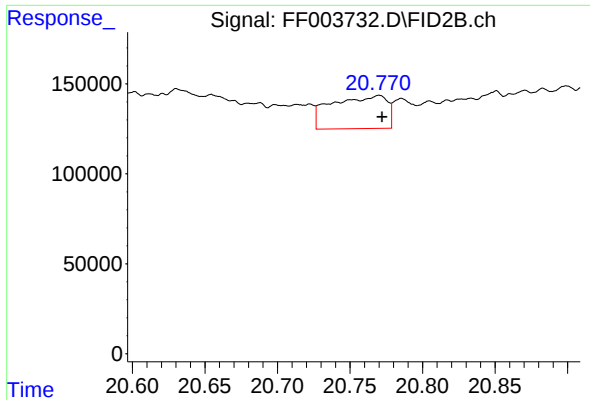

#17 N-OCTATRIACONTANE

R.T.: 20.770 min
Delta R.T.: -0.002 min
Response: 484487
Conc: 4.20 ug/ml

Instrument :
FID_F
ClientSampleId :
PB117622BL

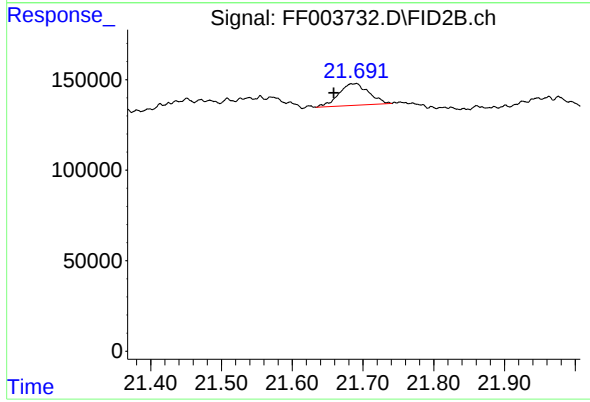

#18 N-TETRACONTANE

R.T.: 21.691 min
Delta R.T.: 0.032 min
Response: 353663
Conc: 2.84 ug/ml