

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030519\
 Data File : FF003735.D
 Signal(s) : FID2B.ch
 Acq On : 05 Mar 2019 18:53
 Operator : AJ\SJ
 Sample : K1726-01
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 DSN001

Integration File: autoint1.e
 Quant Time: Mar 06 00:04:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

| Compound | R.T. | Response | Conc Units |
|-------------------------------|--------|----------|--------------|
| ----- | | | |
| System Monitoring Compounds | | | |
| 9) S TETRACOSANE-d50 (SURR... | 14.597 | 1646394 | 11.825 ug/ml |
| Target Compounds | | | |
| 12) N-OCTACOSANE | 16.778 | 109095 | 0.722 ug/ml |
| 13) N-TRIACONTANE | 17.668 | 139351 | 0.947 ug/ml |
| 14) N-DOTRIACONTANE | 18.505 | 157921 | 1.110 ug/ml |
| 15) N-TETRATRIACONTANE | 19.291 | 21284 | 0.159 ug/ml |
| 16) N-HEXATRIACONTANE | 20.083 | 250740 | 1.922 ug/ml |
| ----- | | | |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030519\
Data File : FF003735.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2019 18:53
Operator : AJ\SJ
Sample : K1726-01
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
DSN001

Integration File: autoint1.e
Quant Time: Mar 06 00:04:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

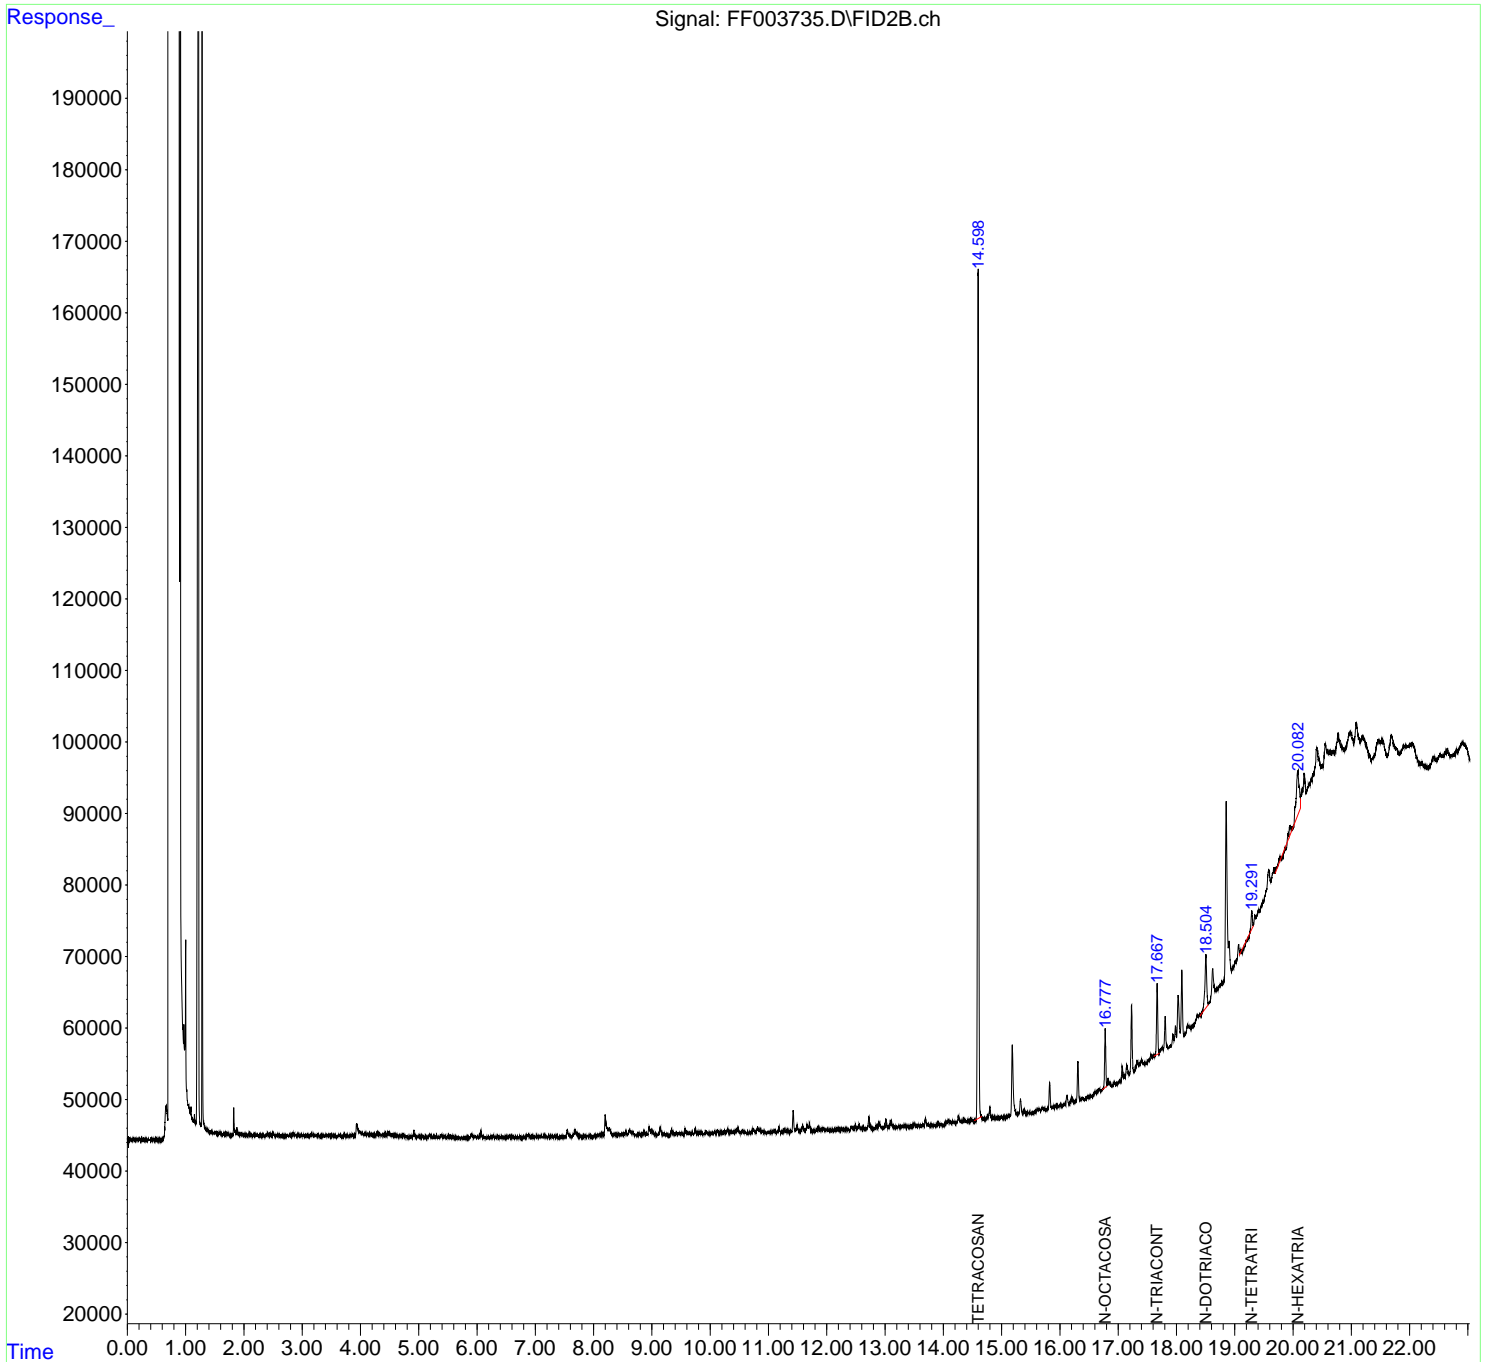


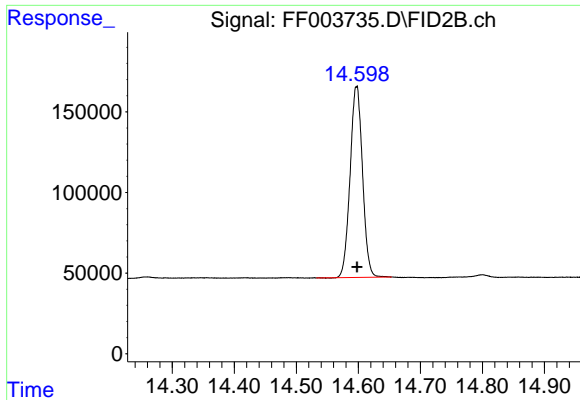

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.597 min
 Delta R.T.: 0.000 min
 Response: 1646394
 Conc: 11.83 ug/ml

Instrument :
 FID_F
 ClientSampled :
 DSN001

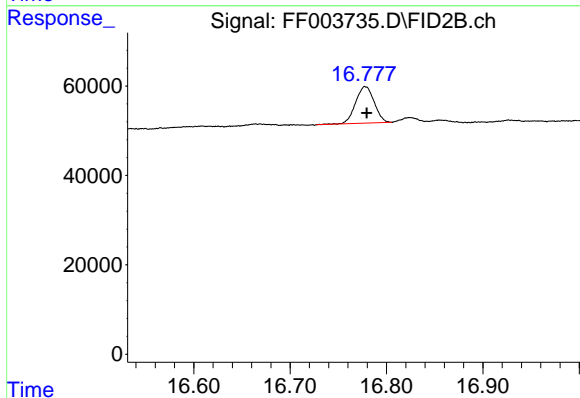


#12 N-OCTACOSANE

R.T.: 16.778 min
 Delta R.T.: -0.002 min
 Response: 109095
 Conc: 0.72 ug/ml

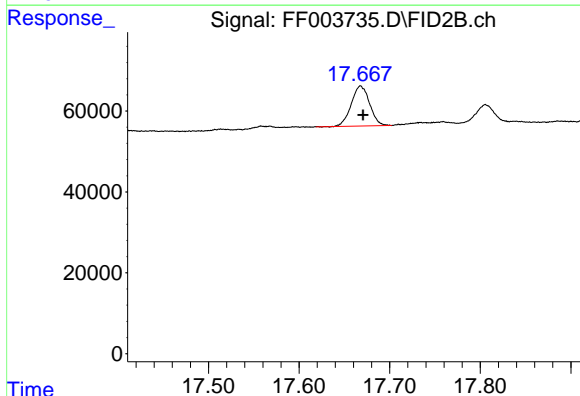


#13 N-TRIACONTANE

R.T.: 17.668 min
 Delta R.T.: -0.003 min
 Response: 139351
 Conc: 0.95 ug/ml

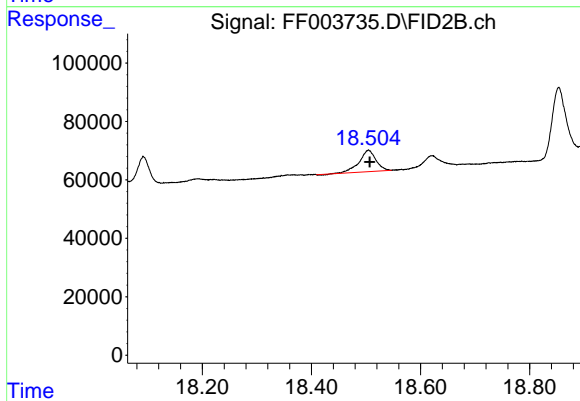

#14 N-DOTRIACONTANE


R.T.: 18.505 min
 Delta R.T.: -0.002 min
 Response: 157921
 Conc: 1.11 ug/ml

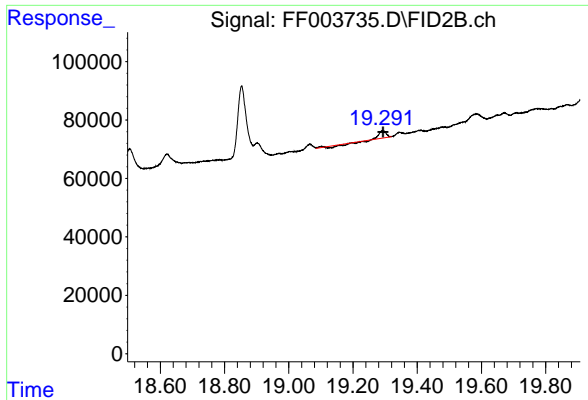

#15 N-TETRATRIACONTANE

R.T.: 19.291 min
Delta R.T.: -0.002 min
Response: 21284
Conc: 0.16 ug/ml

Instrument :
FID_F
ClientSampleId :
DSN001

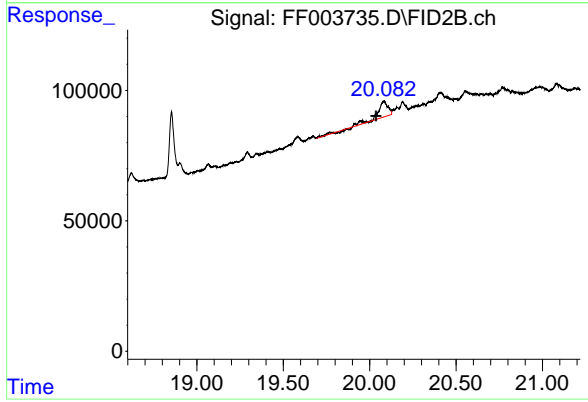

#16 N-HEXATRIACONTANE

R.T.: 20.083 min
Delta R.T.: 0.045 min
Response: 250740
Conc: 1.92 ug/ml