

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030519\
Data File : FF003737.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2019 19:53
Operator : AJ\SJ
Sample : K1727-07
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 06 00:05:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.597	2042833	14.673 ug/ml
Target Compounds				
16)	N-HEXATRIACONTANE	20.076	182247	1.397 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030519\
Data File : FF003737.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2019 19:53
Operator : AJ\SJ
Sample : K1727-07
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 06 00:05:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

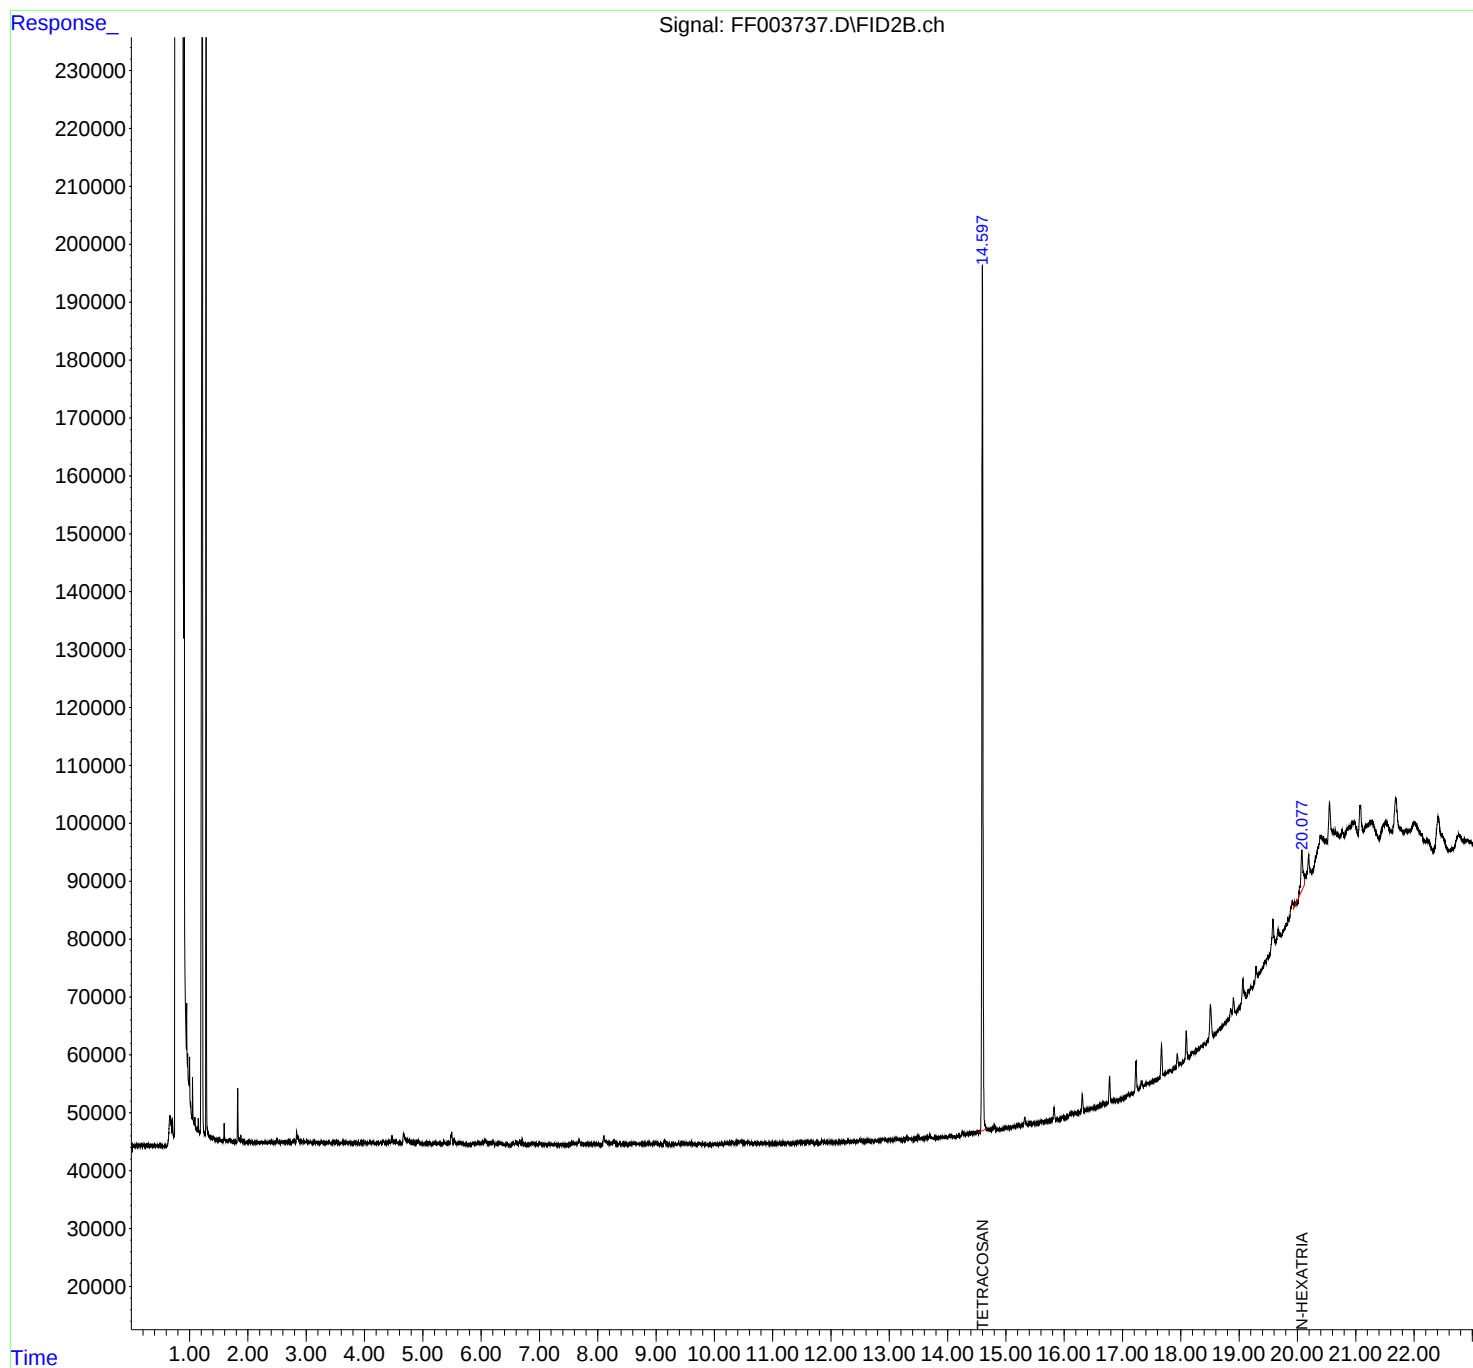


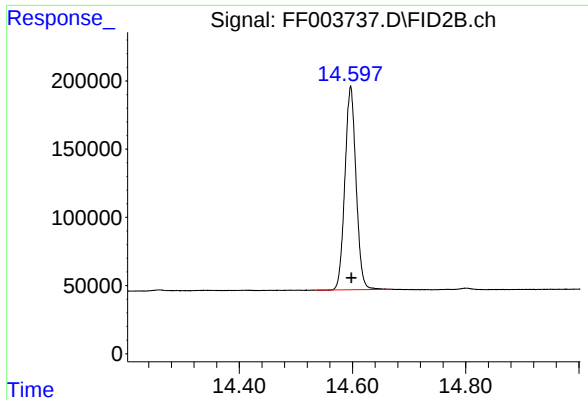

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.597 min
Delta R.T.: -0.001 min
Response: 2042833
Conc: 14.67 ug/ml

Instrument :
FID_F
ClientSampleId :

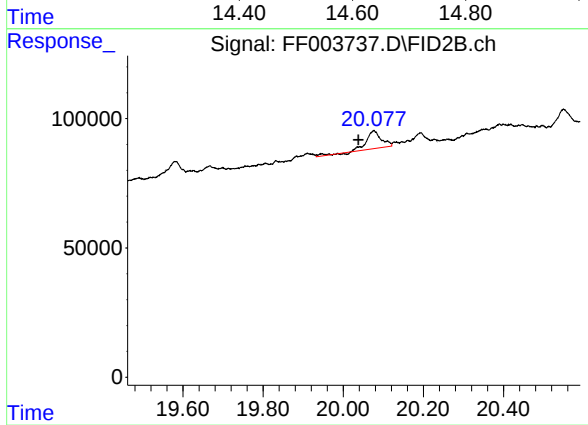

#16 N-HEXATRIACONTANE

R.T.: 20.076 min
Delta R.T.: 0.038 min
Response: 182247
Conc: 1.40 ug/ml