

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030519\
Data File : FF003726.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2019 14:19
Operator : AJ\SJ
Sample : K1688-01 20X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
JC-03-030119-A

Integration File: autoint1.e
Quant Time: Mar 06 00:01:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.594	129453	0.930 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030519\
Data File : FF003726.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2019 14:19
Operator : AJ\SJ
Sample : K1688-01 20X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
JC-03-030119-A

Integration File: autoint1.e
Quant Time: Mar 06 00:01:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

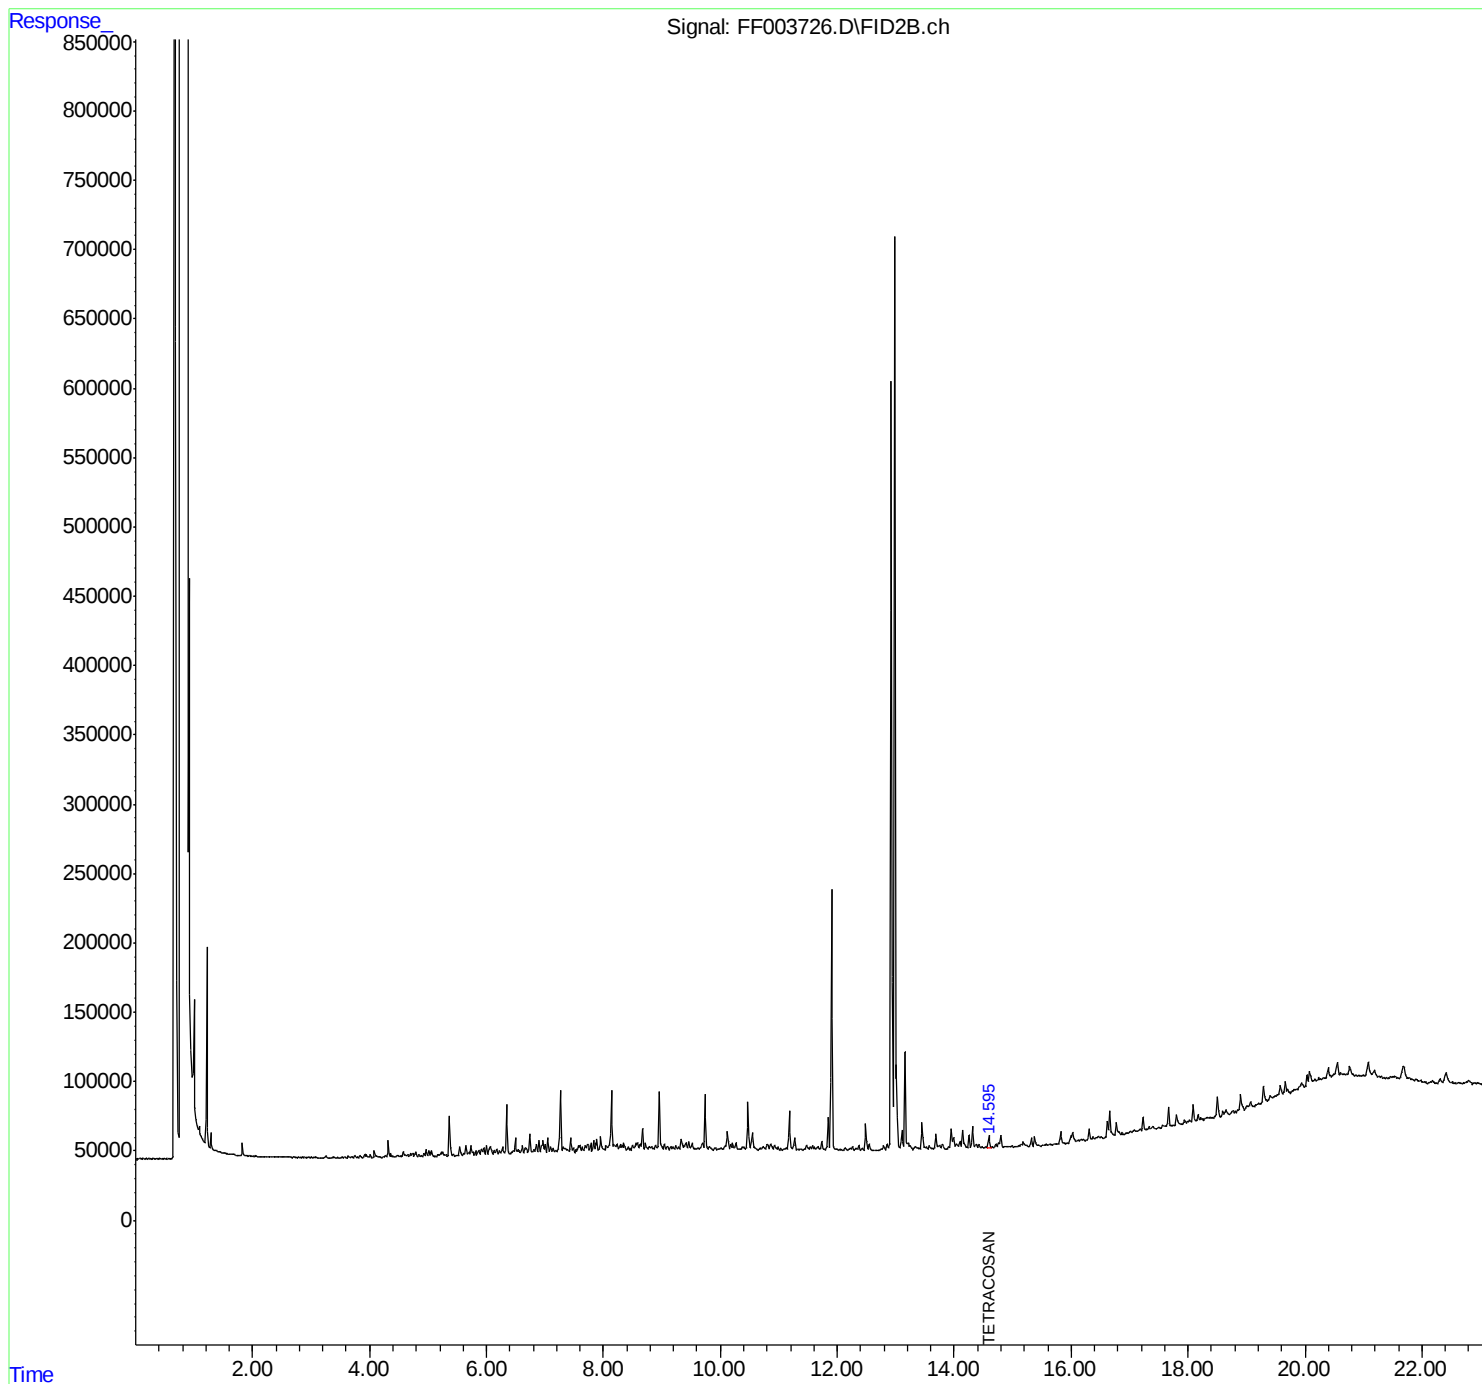

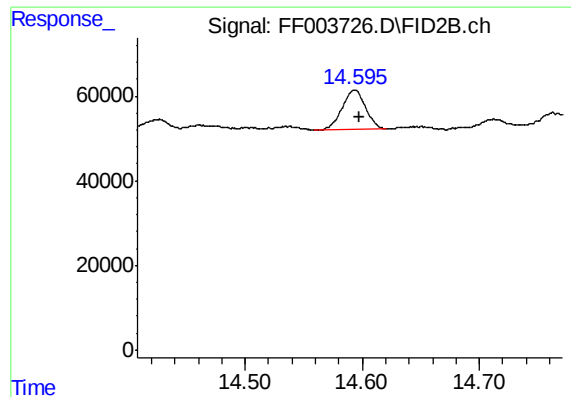

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.594 min
Delta R.T.: -0.004 min
Response: 129453
Conc: 0.93 ug/ml

Instrument :
FID_F
ClientSampleId :
JC-03-030119-A