

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030521\
 Data File : FF008164.D
 Signal(s) : FID2B.ch
 Acq On : 05 Mar 2021 10:23
 Operator : DD\AJ
 Sample : PB134910BL
 Misc : BL WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 05 22:01:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030421.M
 Quant Title :
 QLast Update : Fri Mar 05 09:17:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.668	3185215	22.555 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.584	200924	1.357 ug/ml
16) N-HEXATRIACONTANE	20.139	836377	6.489 ug/ml
18) N-TETRACONTANE	21.799f	1438617	11.704 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030521\
Data File : FF008164.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2021 10:23
Operator : DD\AJ
Sample : PB134910BL
Misc : BL WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 05 22:01:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030421.M
Quant Title :
QLast Update : Fri Mar 05 09:17:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

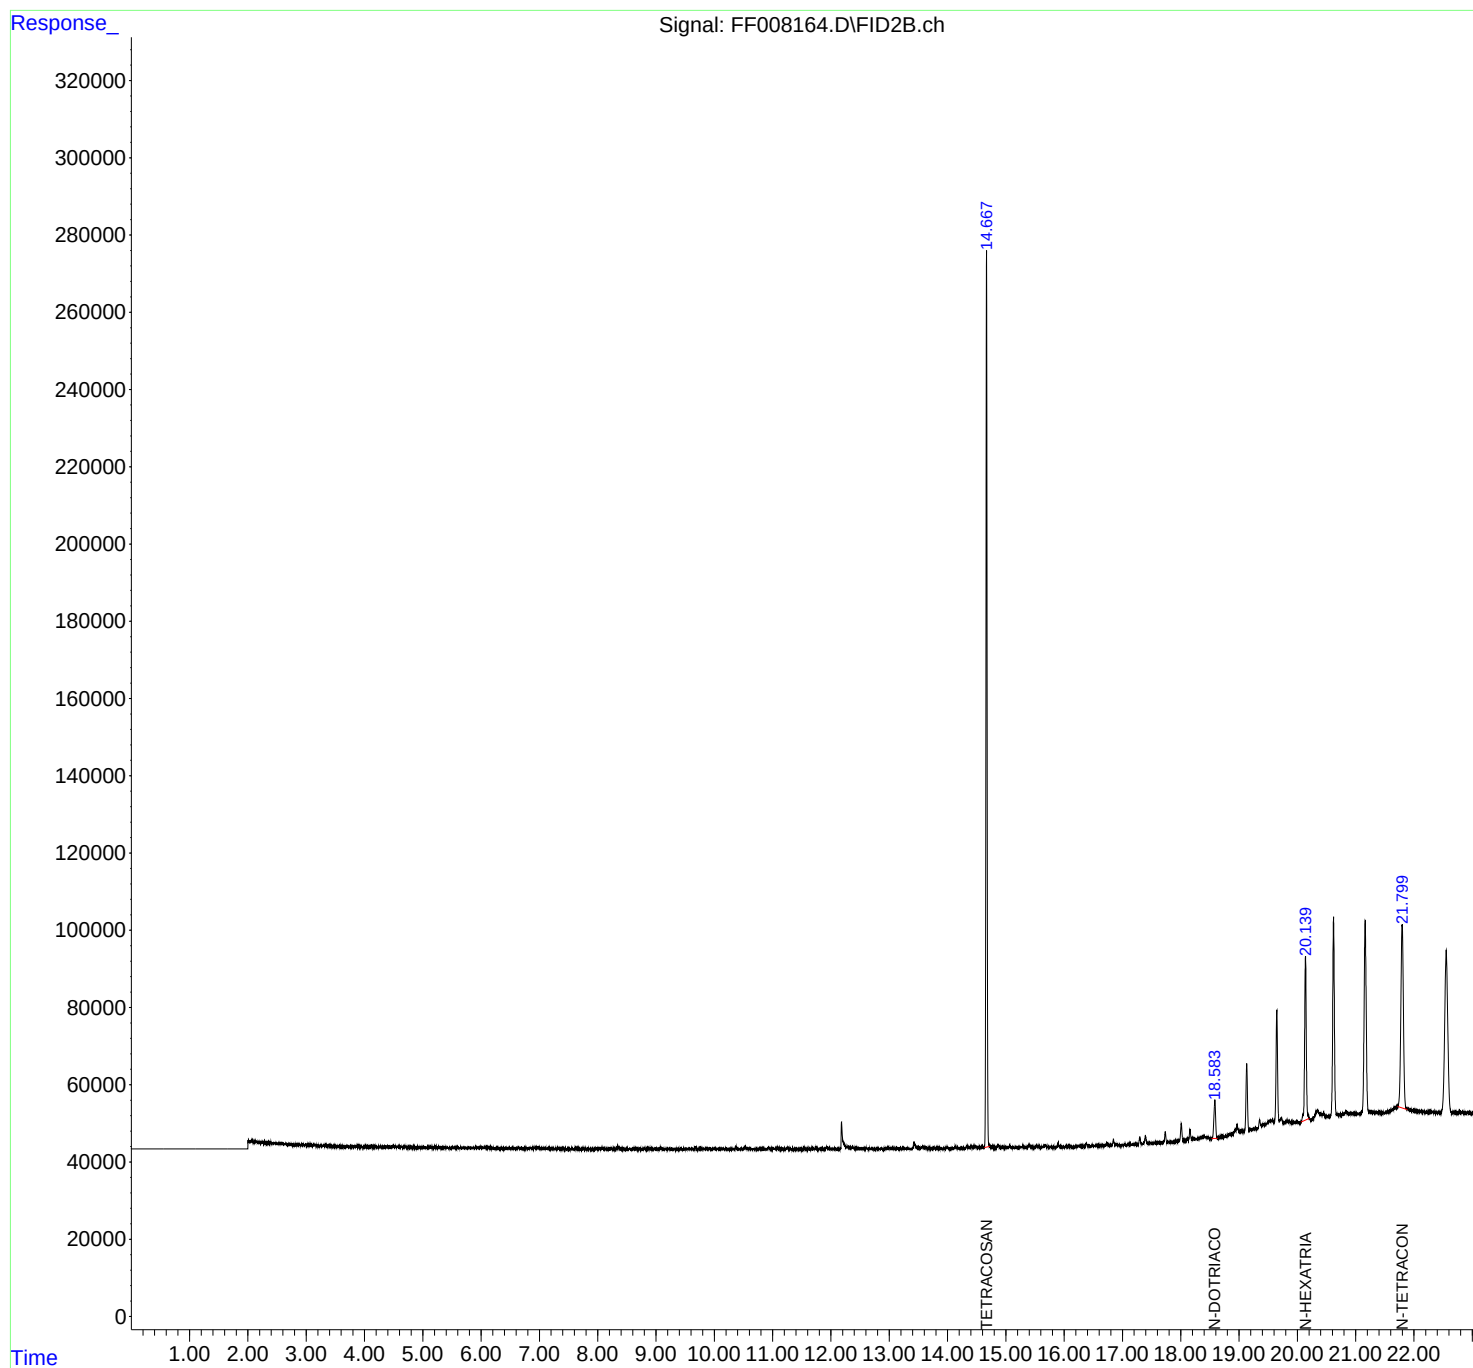


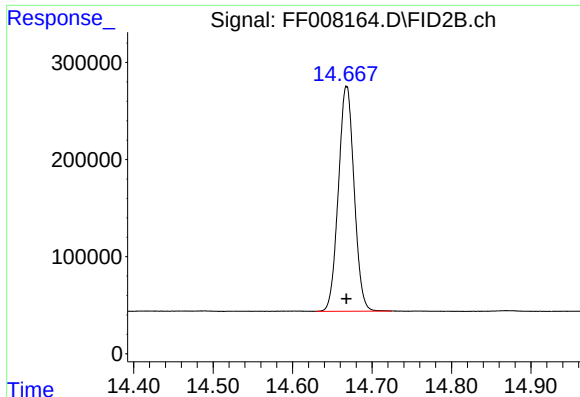

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.668 min
Delta R.T.: 0.000 min
Response: 3185215
Conc: 22.56 ug/ml

Instrument :
FID_F
ClientSampleId :

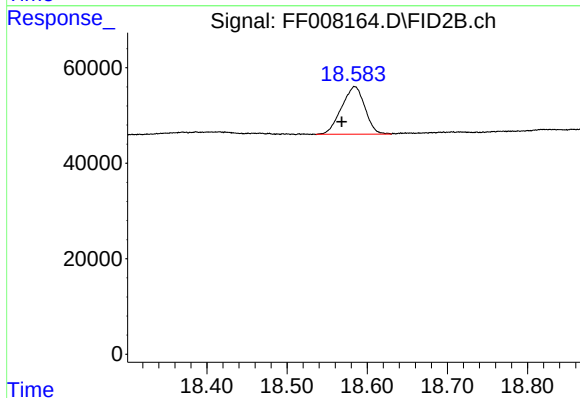


#14 N-DOTRIACONTANE

R.T.: 18.584 min
Delta R.T.: 0.015 min
Response: 200924
Conc: 1.36 ug/ml

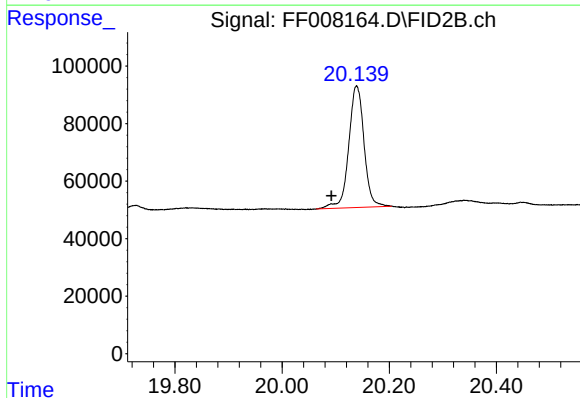

#16 N-HEXATRIACONTANE

R.T.: 20.139 min
Delta R.T.: 0.047 min
Response: 836377
Conc: 6.49 ug/ml

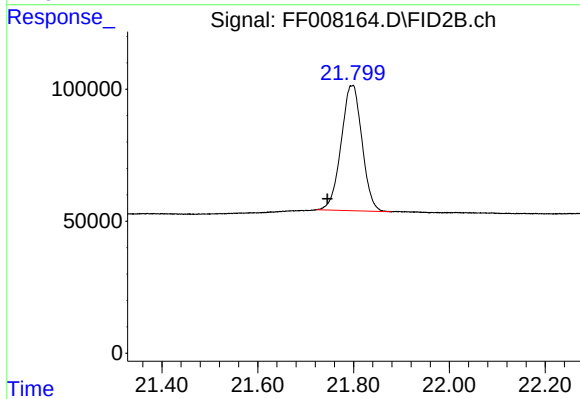

#18 N-TETRACONTANE

R.T.: 21.799 min
Delta R.T.: 0.054 min
Response: 1438617
Conc: 11.70 ug/ml