

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030521\
Data File : FF008173.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2021 15:06
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 05 22:03:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030421.M
Quant Title :
QLast Update : Fri Mar 05 09:17:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.668	2556644	18.104 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.140	102949	0.799 ug/ml
18) N-TETRACONTANE	21.799f	369923	3.009 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030521\
Data File : FF008173.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2021 15:06
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 05 22:03:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030421.M
Quant Title :
QLast Update : Fri Mar 05 09:17:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

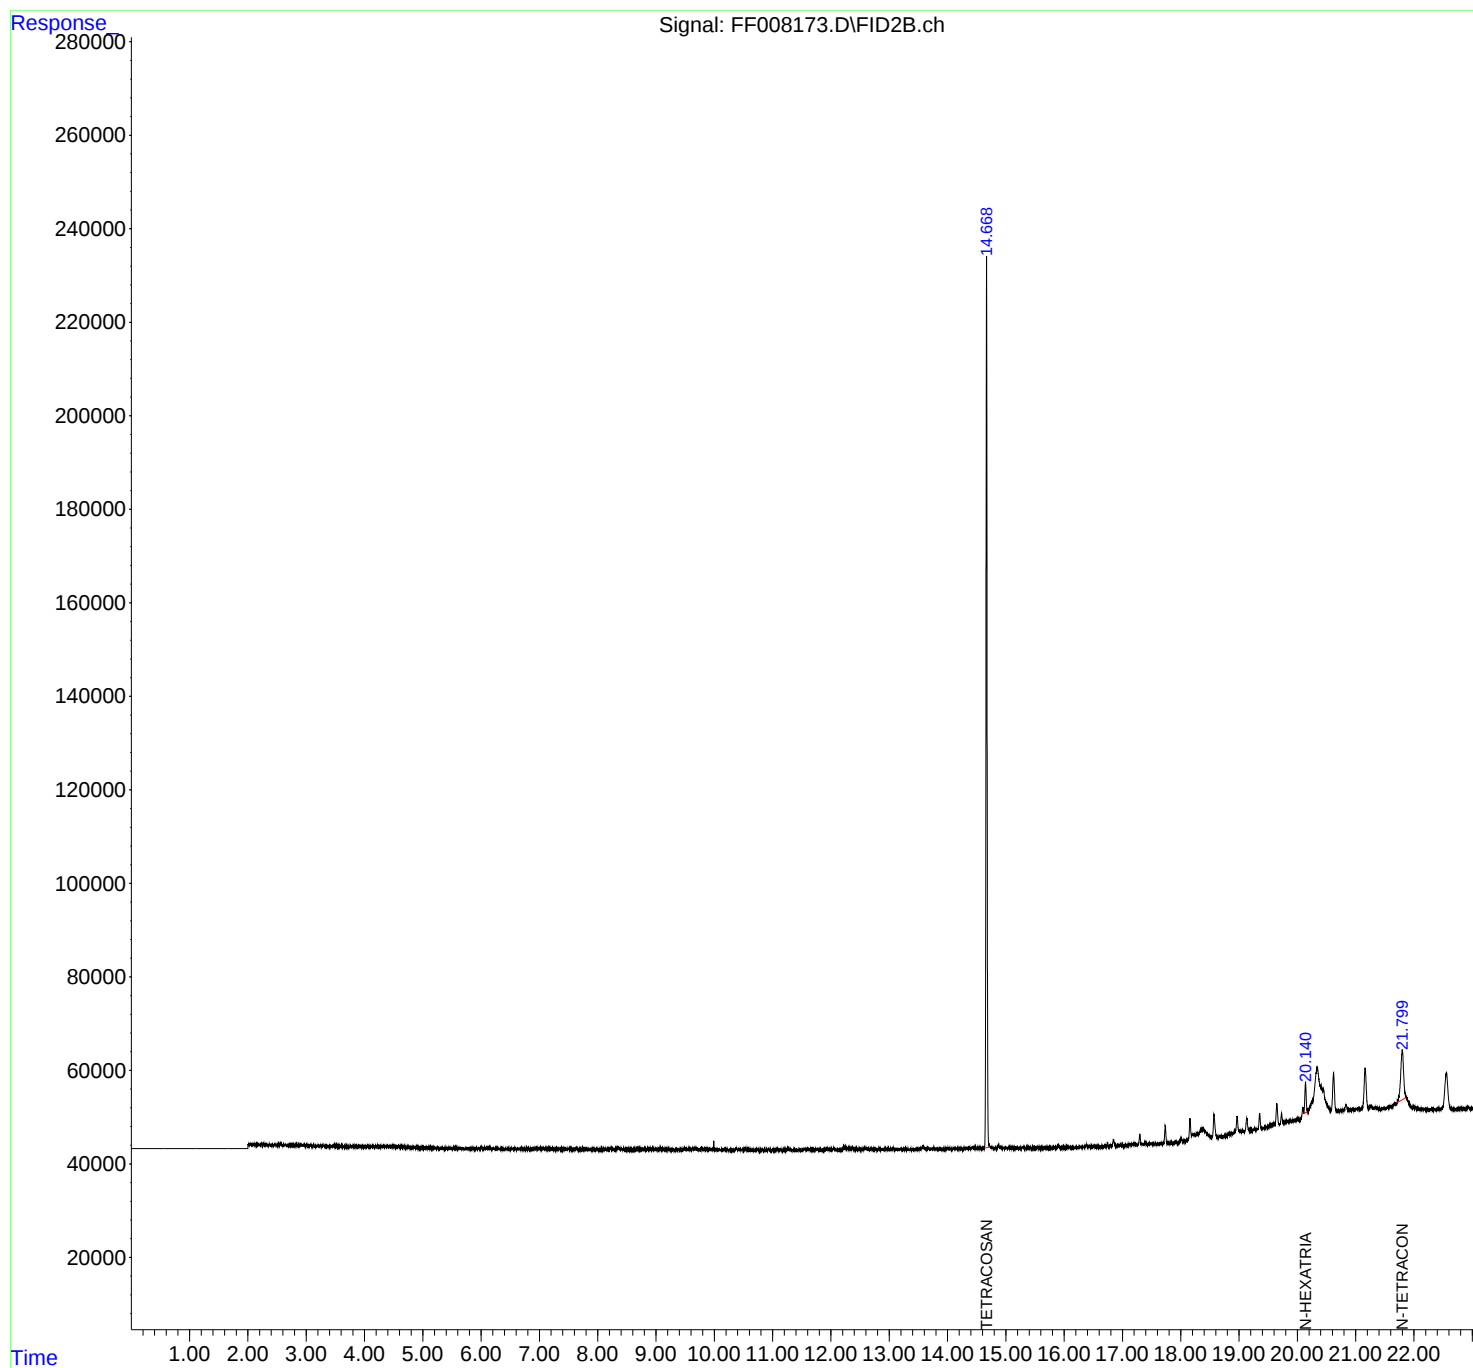


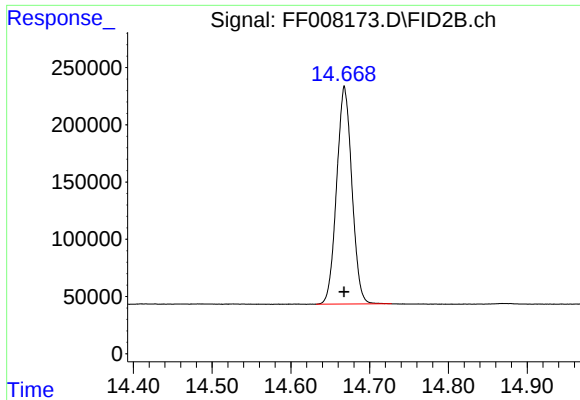

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.668 min
Delta R.T.: 0.000 min
Response: 2556644
Conc: 18.10 ug/ml

Instrument :
FID_F
ClientSampleId :

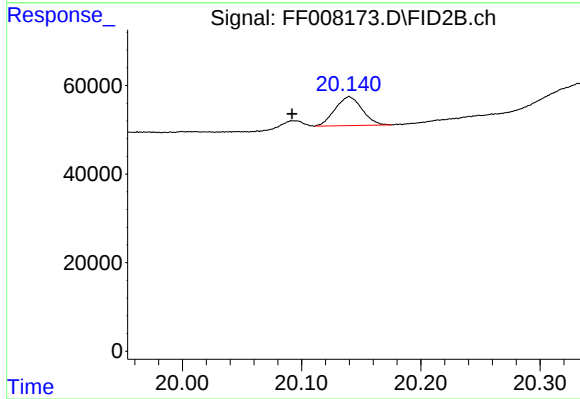

#16 N-HEXATRIACONTANE

R.T.: 20.140 min
Delta R.T.: 0.048 min
Response: 102949
Conc: 0.80 ug/ml

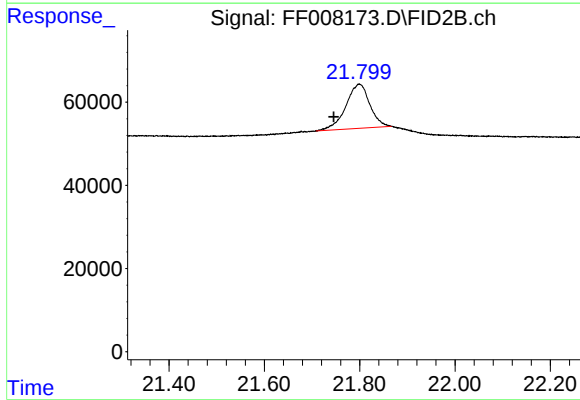

#18 N-TETRACONTANE

R.T.: 21.799 min
Delta R.T.: 0.054 min
Response: 369923
Conc: 3.01 ug/ml