

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030521\
 Data File : FF008178.D
 Signal(s) : FID2B.ch
 Acq On : 05 Mar 2021 18:49
 Operator : DD\AJ
 Sample : M1575-01
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 05 22:04:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030421.M
 Quant Title :
 QLast Update : Fri Mar 05 09:17:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.668	2830095	20.041 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.844	120023	0.764 ug/ml
13) N-TRIACONTANE	17.733	149360	0.970 ug/ml
14) N-DOTRIACONTANE	18.566	116304	0.786 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030521\
Data File : FF008178.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2021 18:49
Operator : DD\AJ
Sample : M1575-01
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 05 22:04:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030421.M
Quant Title :
QLast Update : Fri Mar 05 09:17:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

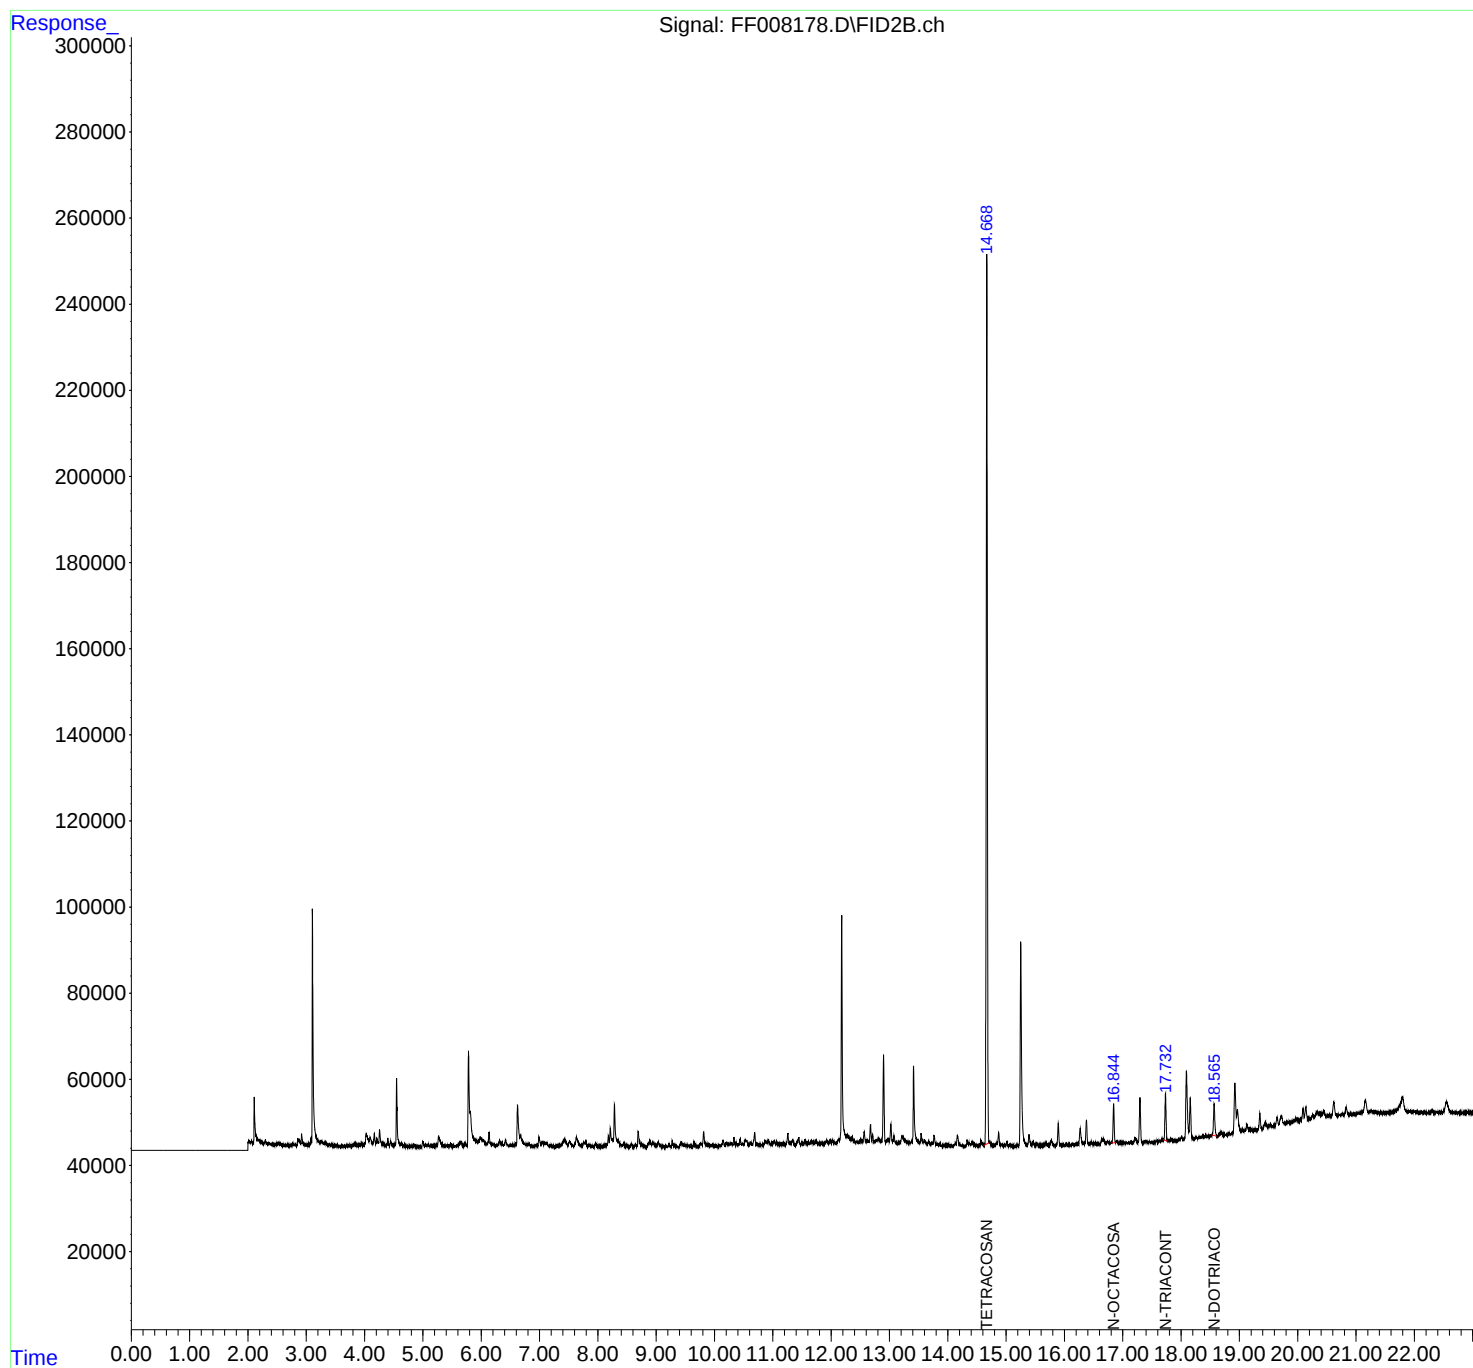


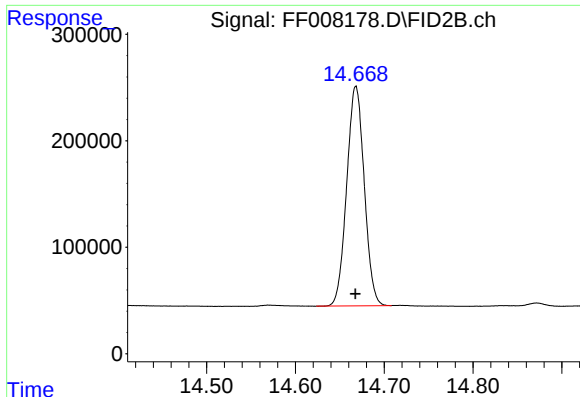

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.668 min
Delta R.T.: 0.000 min
Response: 2830095
Conc: 20.04 ug/ml

Instrument :
FID_F
ClientSampleId :

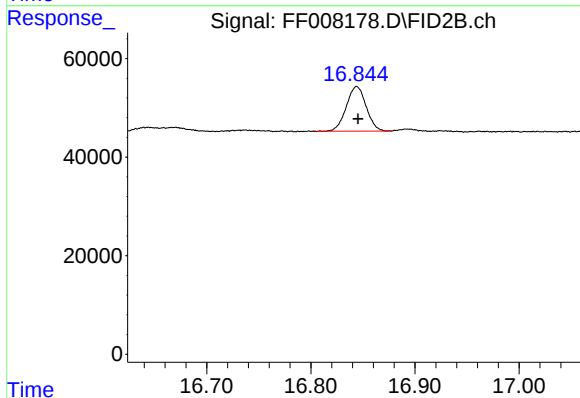


#12 N-OCTACOSANE

R.T.: 16.844 min
Delta R.T.: -0.001 min
Response: 120023
Conc: 0.76 ug/ml

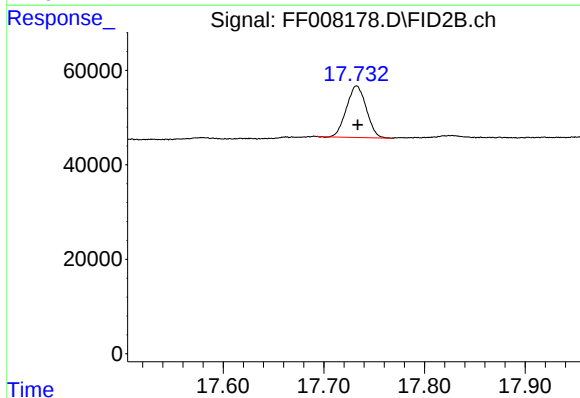

#13 N-TRIACONTANE

R.T.: 17.733 min
Delta R.T.: -0.001 min
Response: 149360
Conc: 0.97 ug/ml

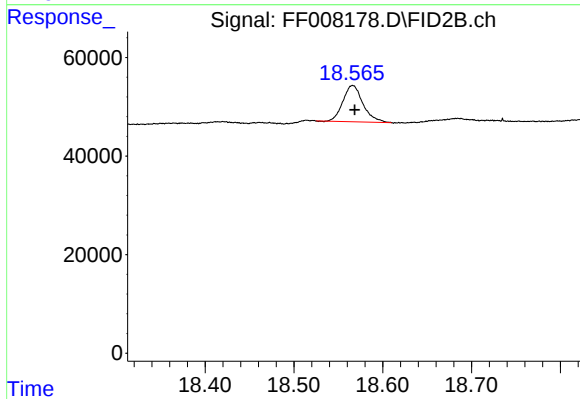

#14 N-DOTRIACONTANE

R.T.: 18.566 min
Delta R.T.: -0.002 min
Response: 116304
Conc: 0.79 ug/ml