

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030521\
Data File : FF008180.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2021 19:51
Operator : DD\AJ
Sample : M1575-03
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 05 22:05:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030421.M
Quant Title :
QLast Update : Fri Mar 05 09:17:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.668	2415979	17.108 ug/ml
Target Compounds			
4) N-TETRADECANE	8.185	2469115	16.786 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030521\
Data File : FF008180.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2021 19:51
Operator : DD\AJ
Sample : M1575-03
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 05 22:05:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030421.M
Quant Title :
QLast Update : Fri Mar 05 09:17:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

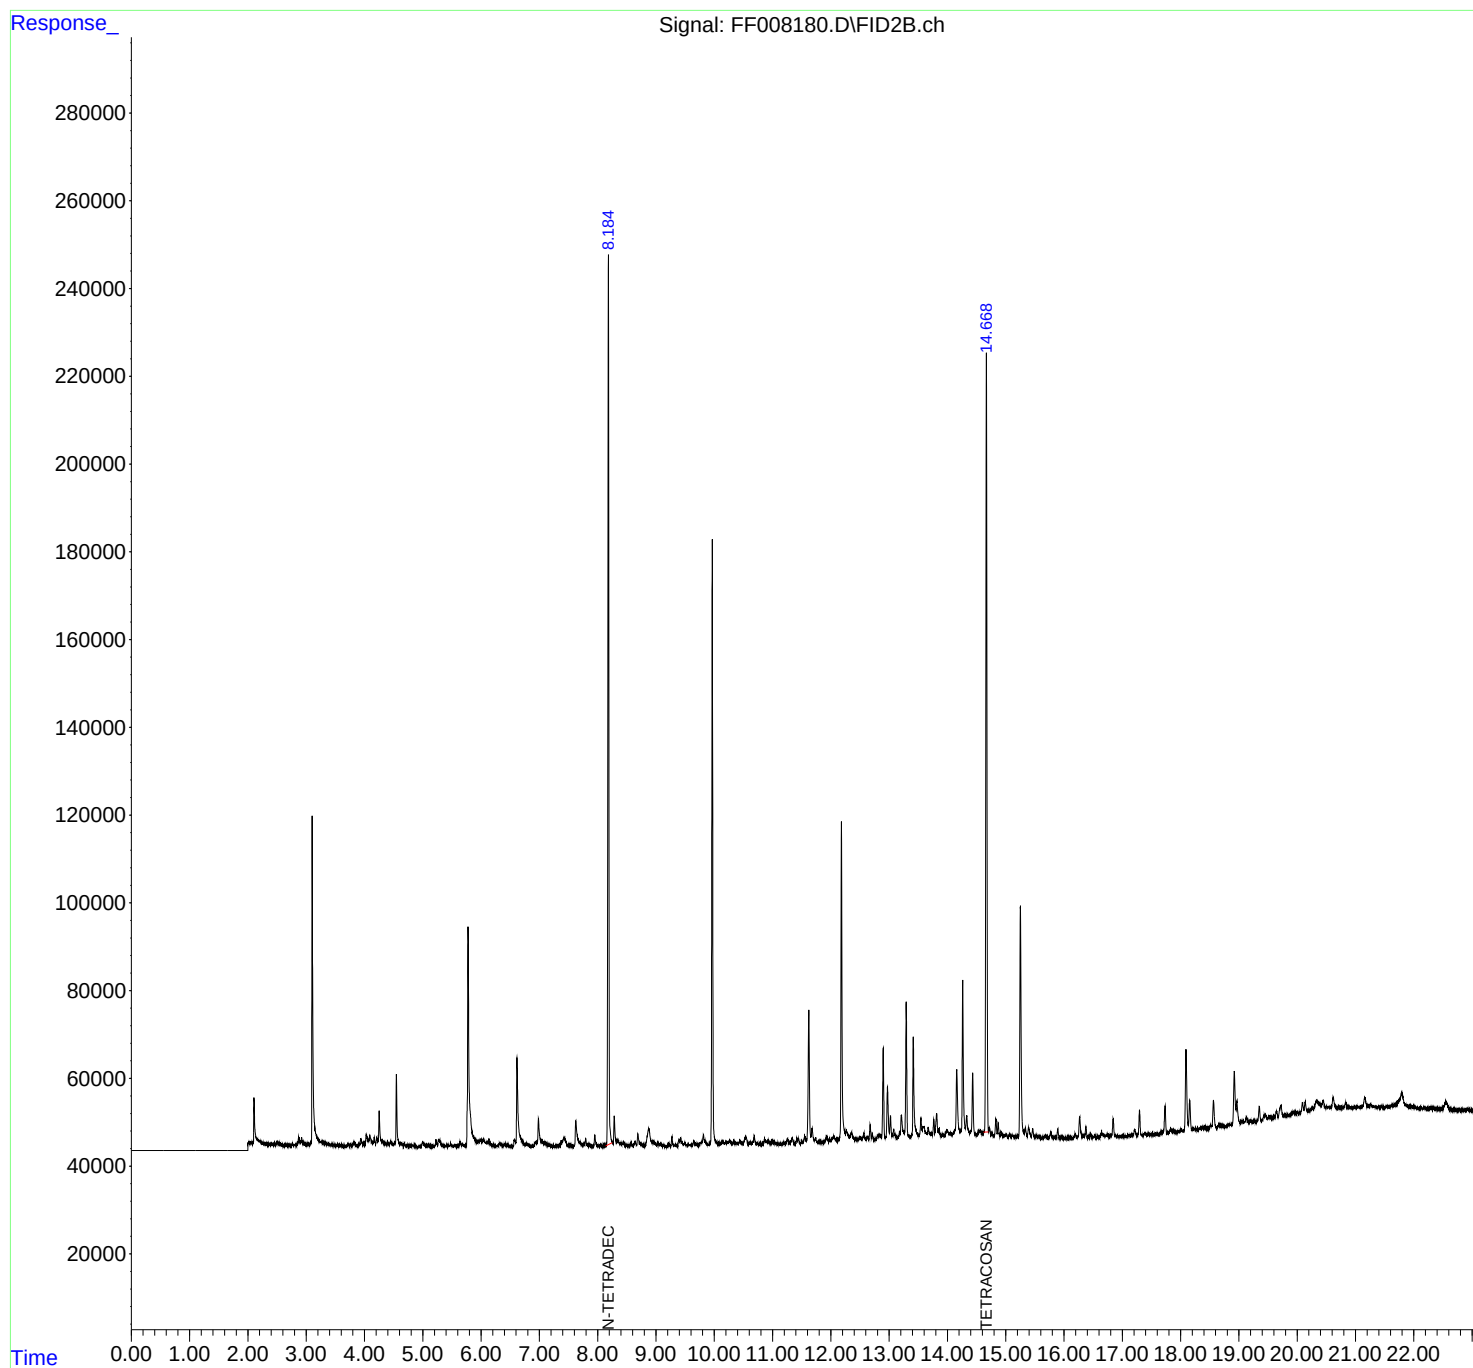


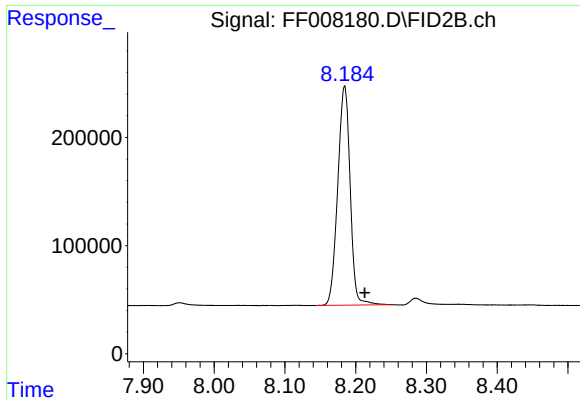

#4 N-TETRADECANE

R.T.: 8.185 min
Delta R.T.: -0.028 min
Response: 2469115
Conc: 16.79 ug/ml

Instrument :
FID_F
ClientSampleId :

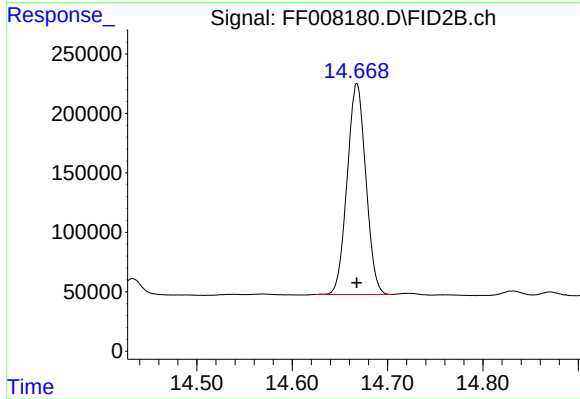

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.668 min
Delta R.T.: 0.000 min
Response: 2415979
Conc: 17.11 ug/ml