

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030521\
Data File : FF008164.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2021 10:23
Operator : DD\AJ
Sample : PB134910BL
Misc : BL WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB134910BL

Integration File: autoint1.e
Quant Time: Mar 05 22:01:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030421.M
Quant Title :
QLast Update : Fri Mar 05 09:17:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.668	3185215	22.555 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030521\
Data File : FF008164.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2021 10:23
Operator : DD\AJ
Sample : PB134910BL
Misc : BL WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB134910BL

Integration File: autoint1.e
Quant Time: Mar 05 22:01:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030421.M
Quant Title :
QLast Update : Fri Mar 05 09:17:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

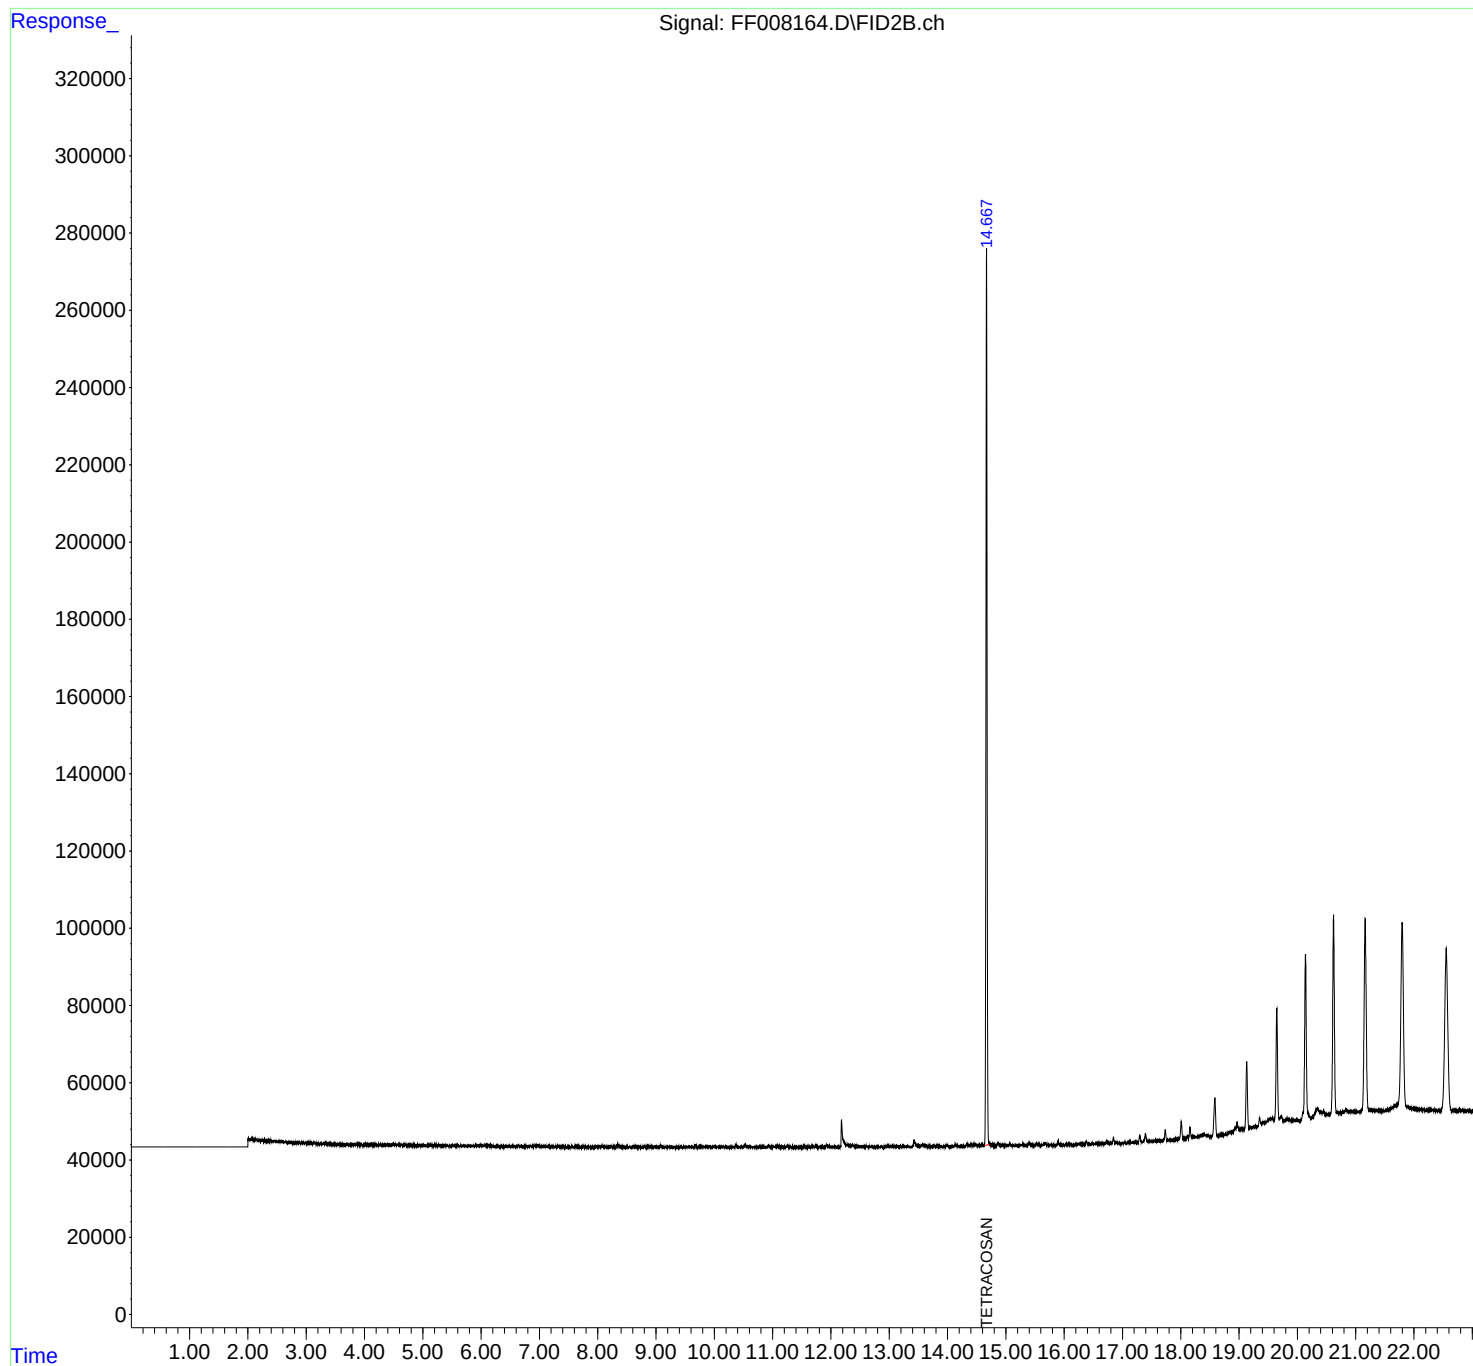

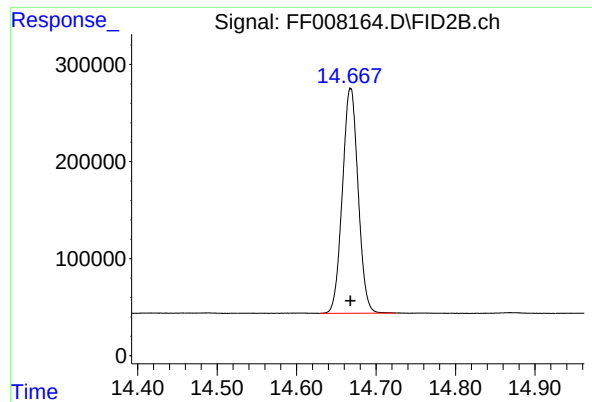

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.668 min
Delta R.T.: 0.000 min
Response: 3185215
Conc: 22.56 ug/ml

Instrument :
FID_F
ClientSampleId :
PB134910BL