

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030521\
 Data File : FF008177.D
 Signal(s) : FID2B.ch
 Acq On : 05 Mar 2021 18:18
 Operator : DD\AJ
 Sample : PB135026BSD
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB135026BSD

Integration File: autoint1.e
 Quant Time: Mar 05 22:04:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030421.M
 Quant Title :
 QLast Update : Fri Mar 05 09:17:37 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.668	2937885	20.804 ug/ml
Target Compounds			
2) N-DECANE	4.396	2517553	19.276 ug/ml
3) N-DODECANE	6.417	2708919	19.808 ug/ml
4) N-TETRADECANE	8.213	2910940	19.790 ug/ml
5) N-HEXADECANE	9.814	3039164	20.120 ug/ml
6) N-OCTADECANE	11.257	3172324	20.254 ug/ml
7) N-EICOSANE	12.568	3294275	20.800 ug/ml
8) N-DOCOSANE	13.767	3319792	20.844 ug/ml
10) N-TETRACOSANE	14.872	3301112	20.599 ug/ml
11) N-HEXACOSANE	15.895	3247903	20.528 ug/ml
12) N-OCTACOSANE	16.846	3193231	20.333 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030521\
Data File : FF008177.D
Signal(s) : FID2B.ch
Acq On : 05 Mar 2021 18:18
Operator : DD\AJ
Sample : PB135026BSD
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB135026BSD

Integration File: autoint1.e
Quant Time: Mar 05 22:04:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030421.M
Quant Title :
QLast Update : Fri Mar 05 09:17:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

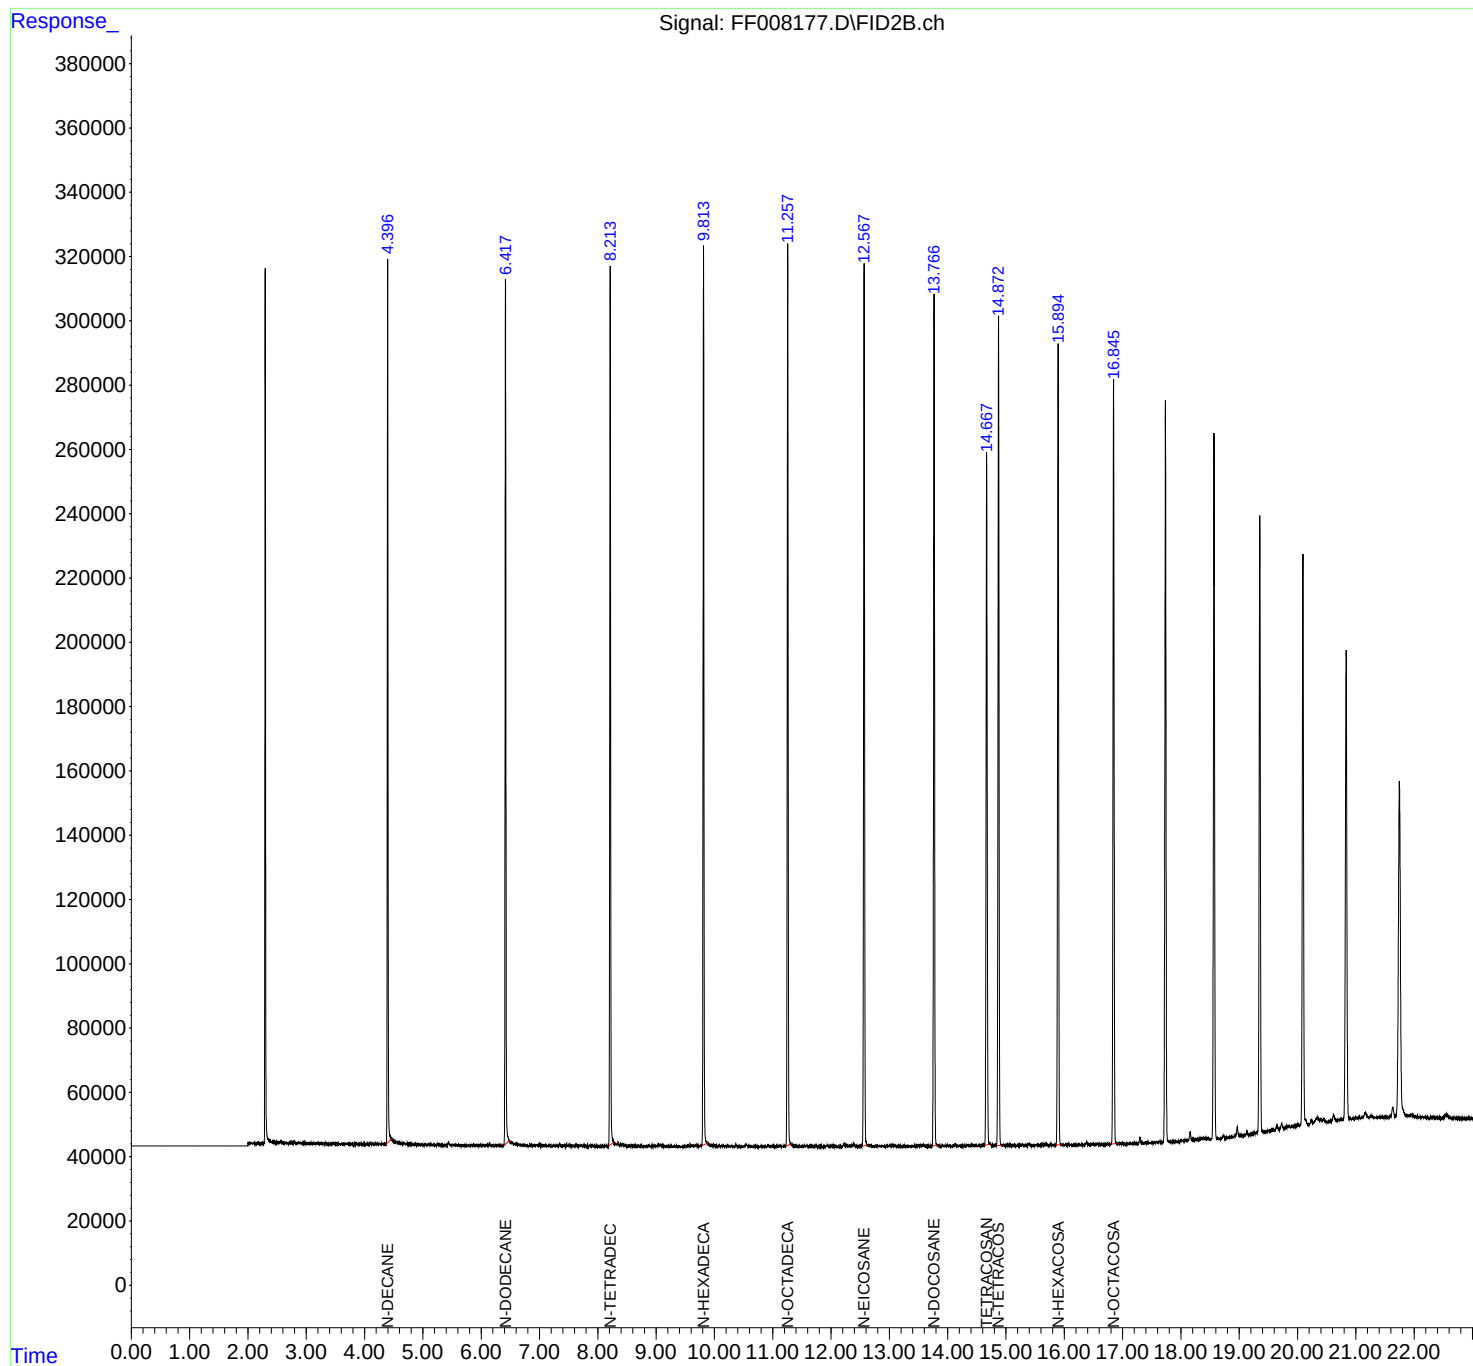


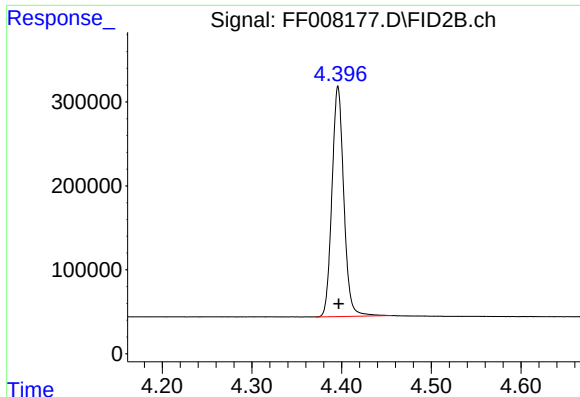

#2 N-DECANE


R.T.: 4.396 min
Delta R.T.: 0.000 min
Response: 2517553
Conc: 19.28 ug/ml

Instrument :
FID_F
ClientSampleId :
PB135026BSD

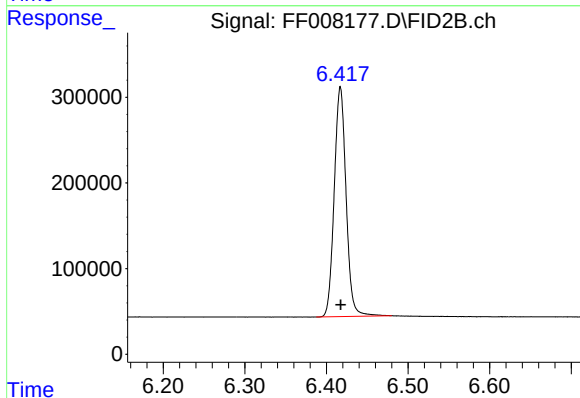


#3 N-DODECANE

R.T.: 6.417 min
Delta R.T.: 0.000 min
Response: 2708919
Conc: 19.81 ug/ml

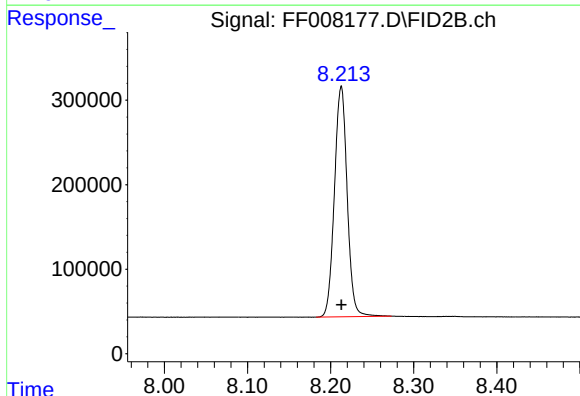


#4 N-TETRADECANE

R.T.: 8.213 min
Delta R.T.: 0.000 min
Response: 2910940
Conc: 19.79 ug/ml

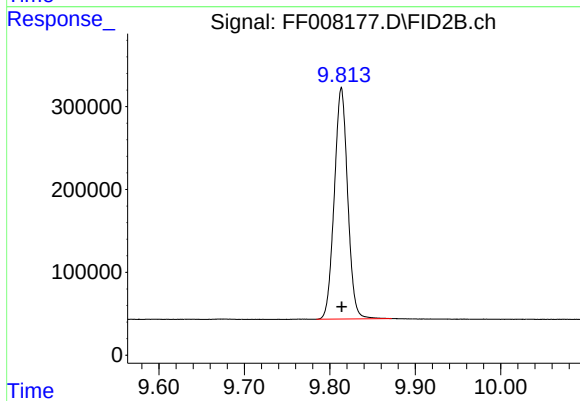

#5 N-HEXADECANE


R.T.: 9.814 min
Delta R.T.: 0.000 min
Response: 3039164
Conc: 20.12 ug/ml

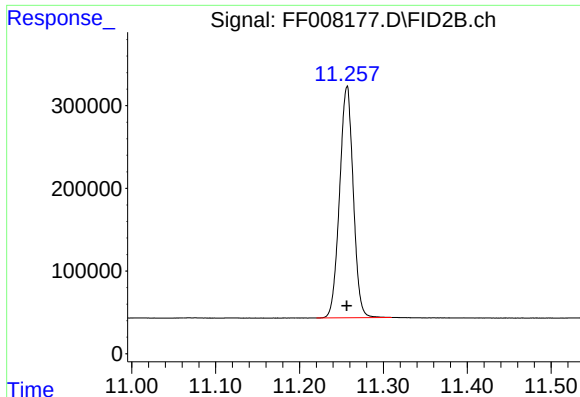

#6 N-OCTADECANE


R.T.: 11.257 min
Delta R.T.: 0.000 min
Response: 3172324
Conc: 20.25 ug/ml

Instrument :
FID_F
ClientSampleId :
PB135026BSD

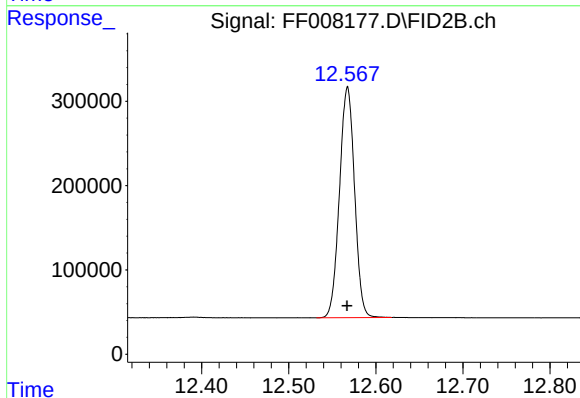


#7 N-EICOSANE

R.T.: 12.568 min
Delta R.T.: 0.000 min
Response: 3294275
Conc: 20.80 ug/ml

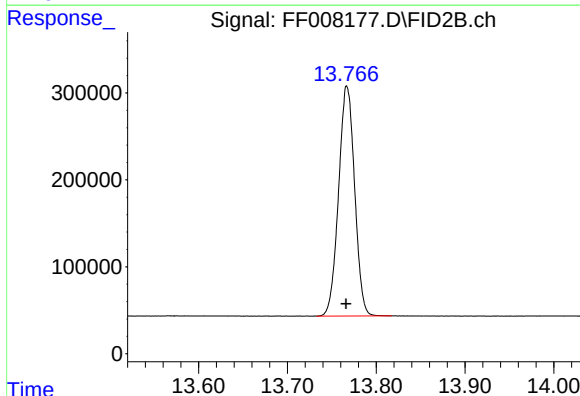


#8 N-DOCOSANE

R.T.: 13.767 min
Delta R.T.: 0.000 min
Response: 3319792
Conc: 20.84 ug/ml

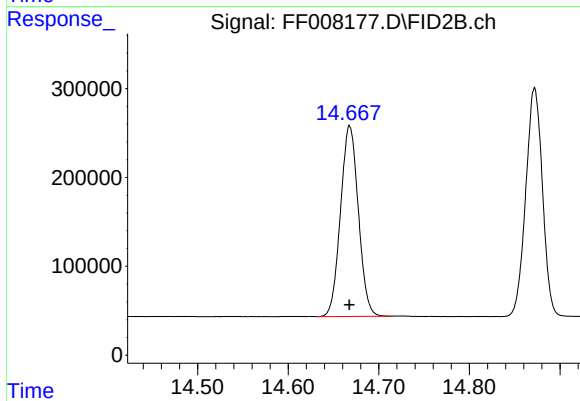

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.668 min
Delta R.T.: 0.000 min
Response: 2937885
Conc: 20.80 ug/ml

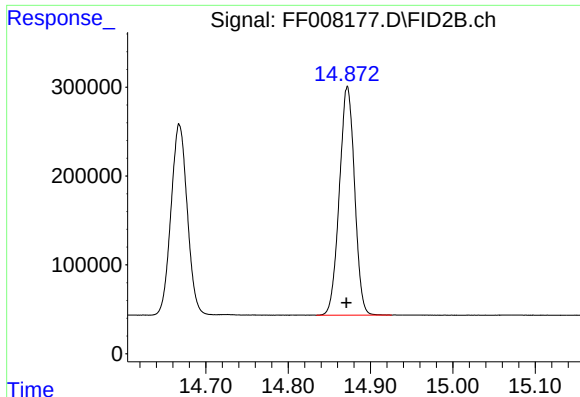

#10 N-TETRACOSANE


R.T.: 14.872 min
Delta R.T.: 0.001 min
Response: 3301112
Conc: 20.60 ug/ml

Instrument :
FID_F
ClientSampleId :
PB135026BSD

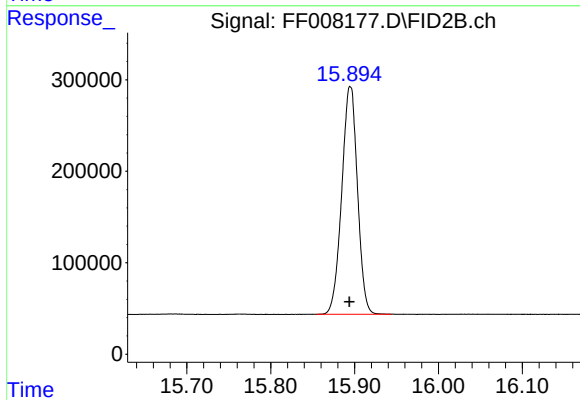

#11 N-HEXACOSANE

R.T.: 15.895 min
Delta R.T.: 0.001 min
Response: 3247903
Conc: 20.53 ug/ml

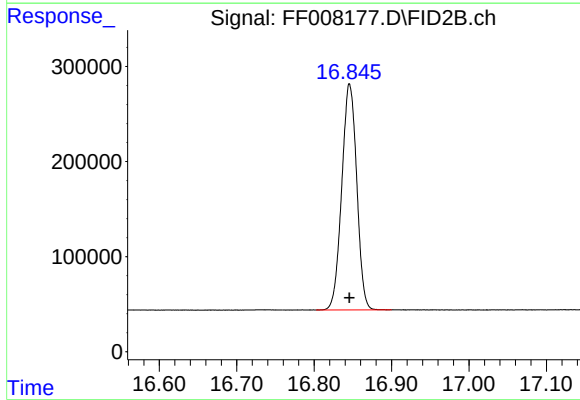

#12 N-OCTACOSANE

R.T.: 16.846 min
Delta R.T.: 0.000 min
Response: 3193231
Conc: 20.33 ug/ml