

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030619\
 Data File : FF003743.D
 Signal(s) : FID2B.ch
 Acq On : 06 Mar 2019 12:14
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Mar 07 00:20:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.342	3182436	20.392 ug/ml
12) N-OCTACOSANE	16.776	3097510	20.498 ug/ml
13) N-TRIACONTANE	17.665	645120	4.386 ug/ml
14) N-DOTRIACONTANE	18.501	789047	5.548 ug/ml
15) N-TETRATRIACONTANE	19.289	545948	4.077 ug/ml
16) N-HEXATRIACONTANE	20.034	253212	1.941 ug/ml
17) N-OCTATRIACONTANE	20.767	218972	1.896 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030619\
Data File : FF003743.D
Signal(s) : FID2B.ch
Acq On : 06 Mar 2019 12:14
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 07 00:20:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

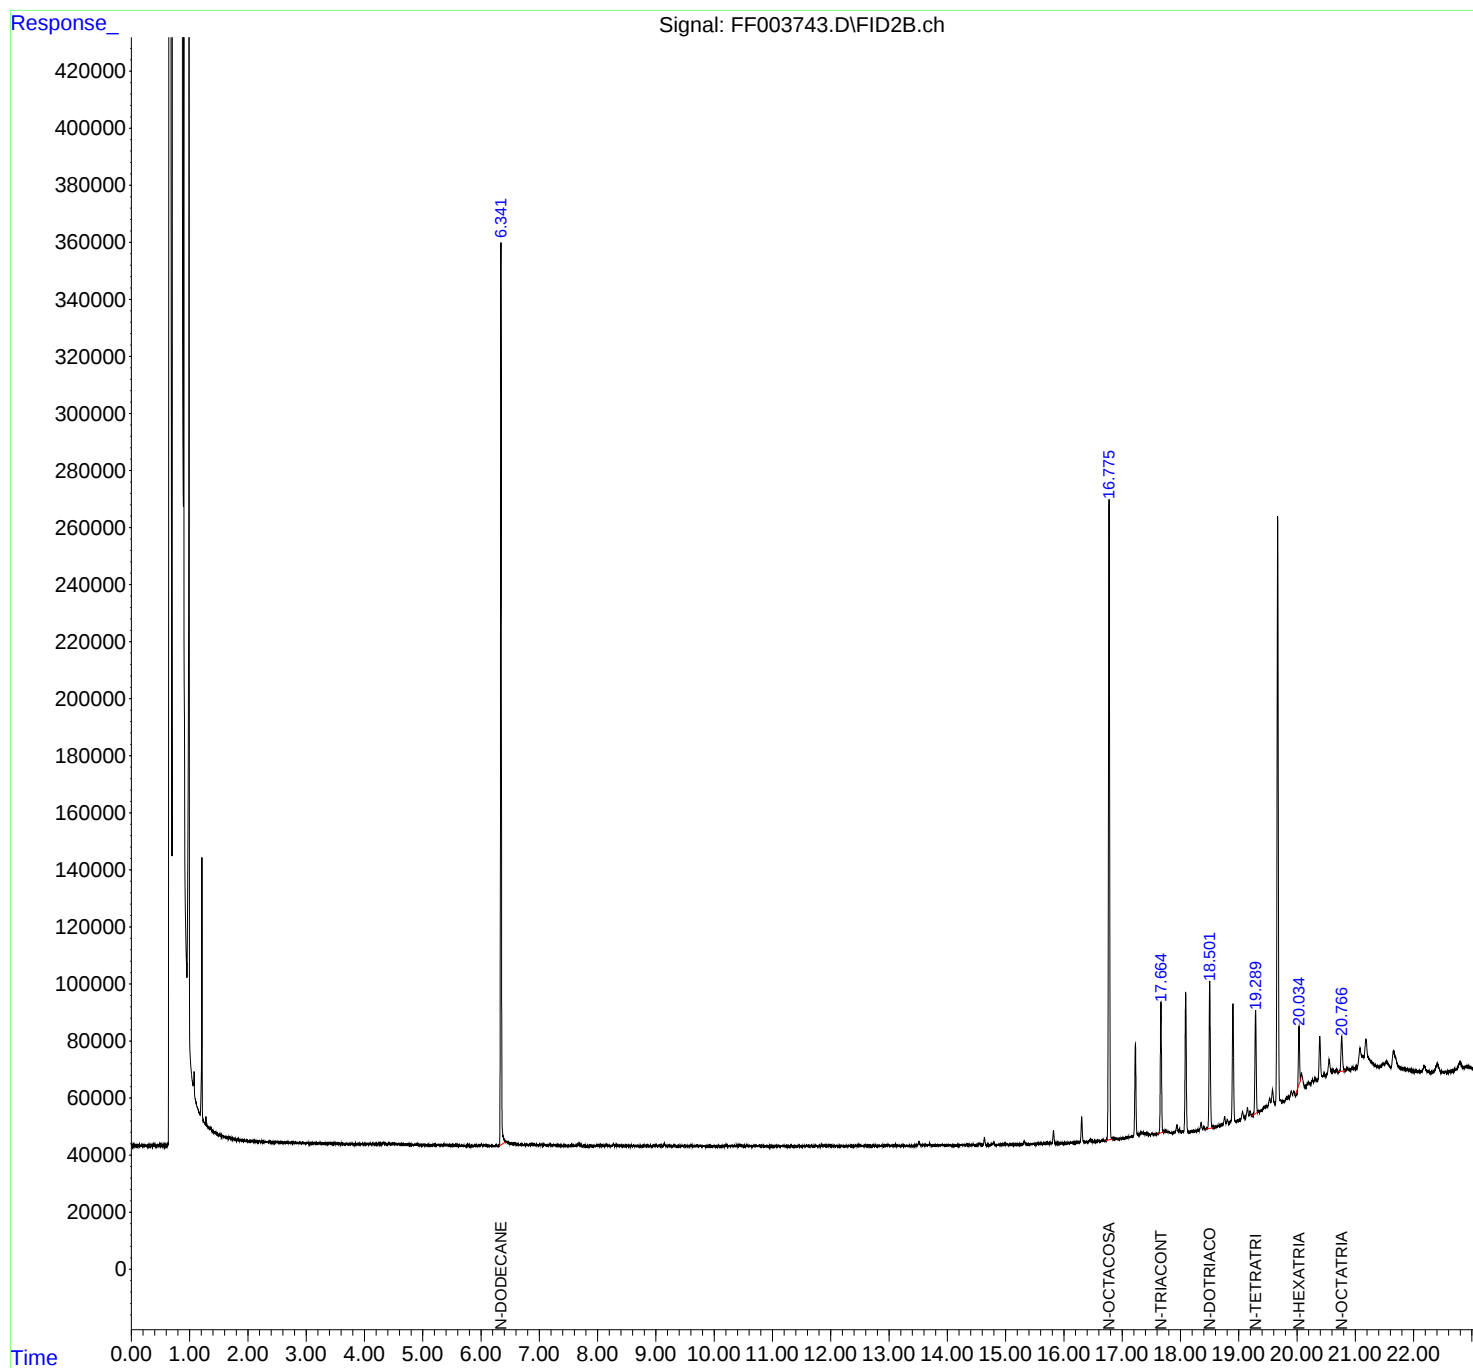


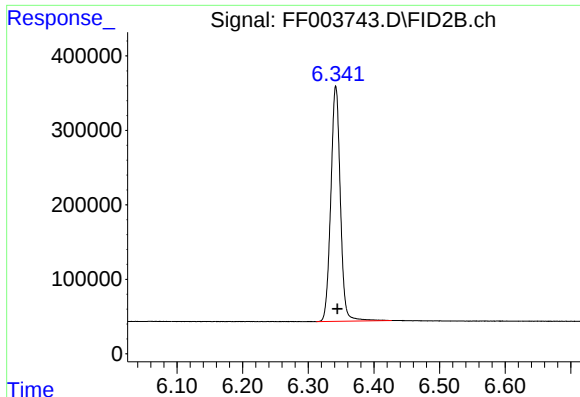

#3 N-DODECANE


R.T.: 6.342 min
Delta R.T.: -0.002 min
Response: 3182436
Conc: 20.39 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

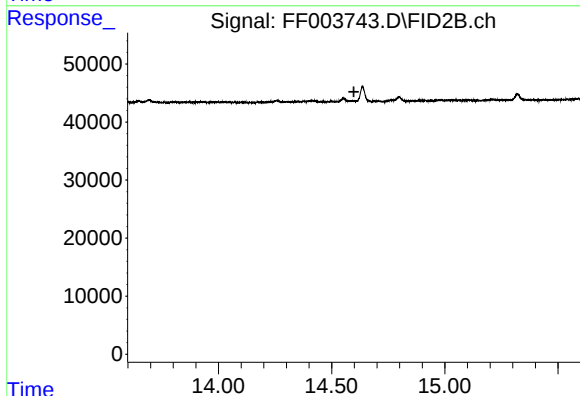


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.598 min
Response: 0
Conc: N.D.

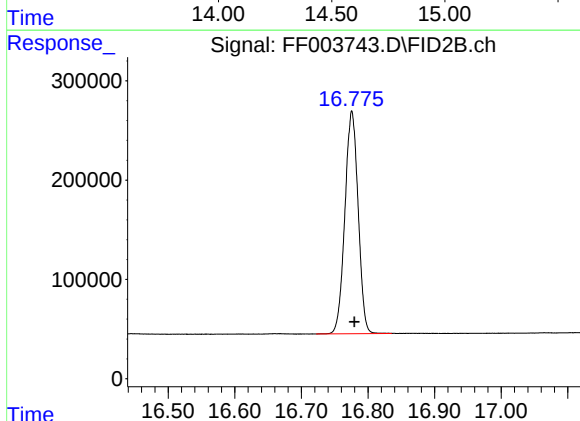


#12 N-OCTACOSANE

R.T.: 16.776 min
Delta R.T.: -0.004 min
Response: 3097510
Conc: 20.50 ug/ml

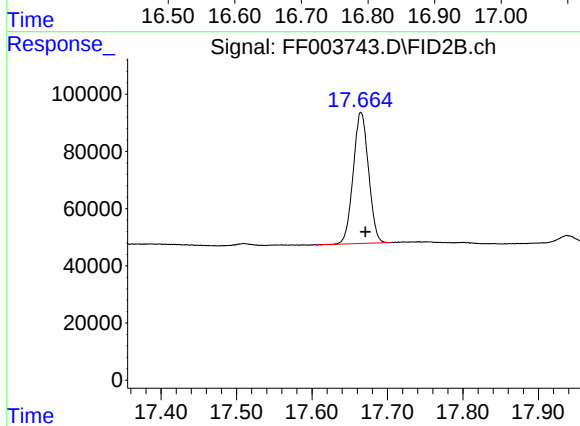

#13 N-TRIACONTANE


R.T.: 17.665 min
Delta R.T.: -0.006 min
Response: 645120
Conc: 4.39 ug/ml

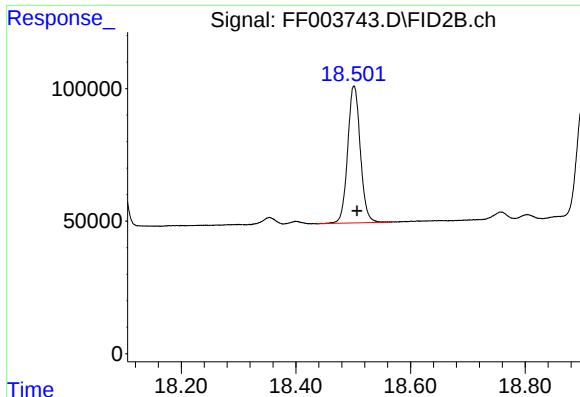

#14 N-DOTRIACONTANE


R.T.: 18.501 min
Delta R.T.: -0.005 min
Response: 789047
Conc: 5.55 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

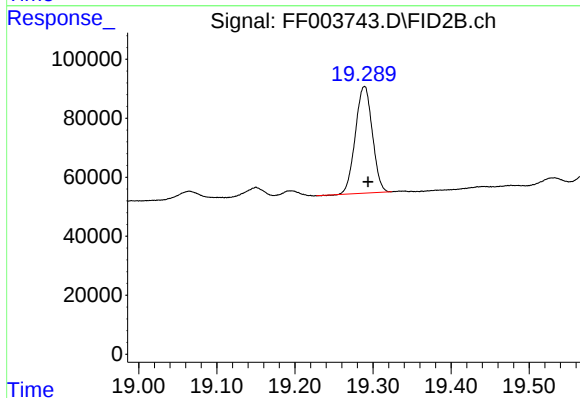


#15 N-TETRATRIACONTANE

R.T.: 19.289 min
Delta R.T.: -0.005 min
Response: 545948
Conc: 4.08 ug/ml

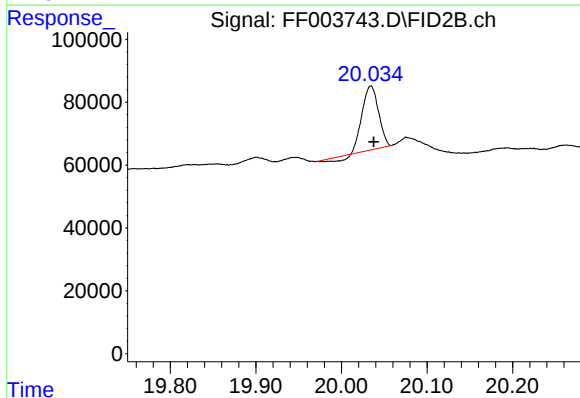

#16 N-HEXATRIACONTANE

R.T.: 20.034 min
Delta R.T.: -0.004 min
Response: 253212
Conc: 1.94 ug/ml

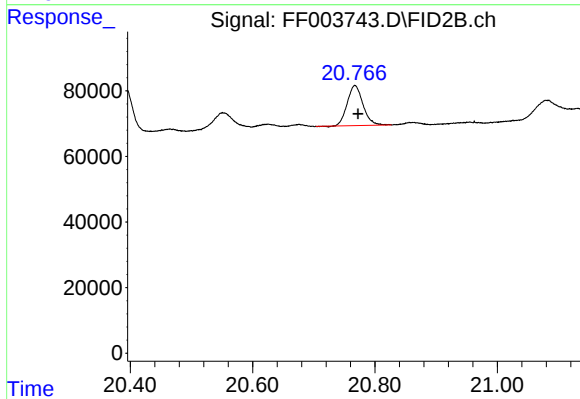

#17 N-OCTATRIACONTANE

R.T.: 20.767 min
Delta R.T.: -0.005 min
Response: 218972
Conc: 1.90 ug/ml