

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030619\
 Data File : FF003744.D
 Signal(s) : FID2B.ch
 Acq On : 06 Mar 2019 12:44
 Operator : AJ\SJ
 Sample : K1727-01 20X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 MW-11

Integration File: autoint1.e
 Quant Time: Mar 07 00:20:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.593	96454	0.693 ug/ml
Target Compounds			
2) N-DECANE	4.322	1138838	7.404 ug/ml
3) N-DODECANE	6.342	477422	3.059 ug/ml
4) N-TETRADECANE	8.135	349962	2.183 ug/ml
5) N-HEXADECANE	9.736	131569	0.808 ug/ml
6) N-OCTADECANE	11.177	72514	0.440 ug/ml
16) N-HEXATRIACONTANE	20.076	166696	1.278 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030619\
Data File : FF003744.D
Signal(s) : FID2B.ch
Acq On : 06 Mar 2019 12:44
Operator : AJ\SJ
Sample : K1727-01 20X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MW-11

Integration File: autoint1.e
Quant Time: Mar 07 00:20:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

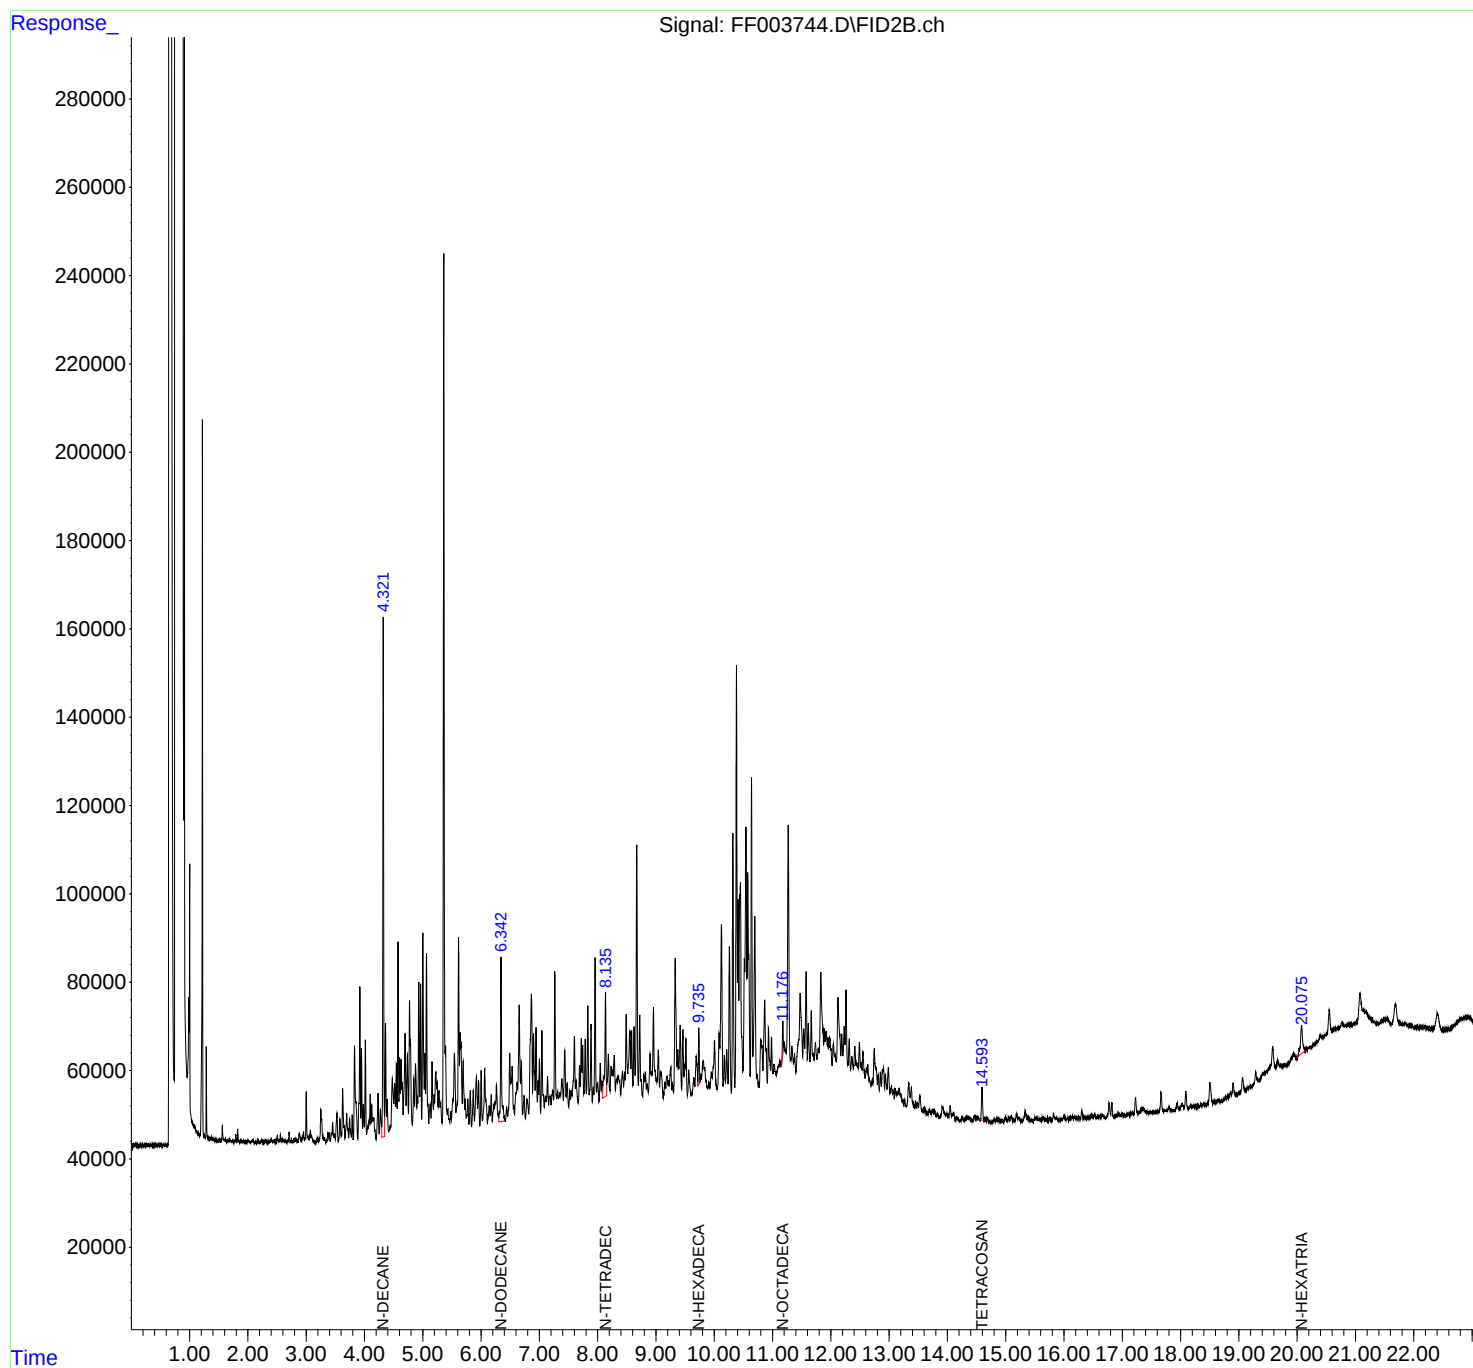


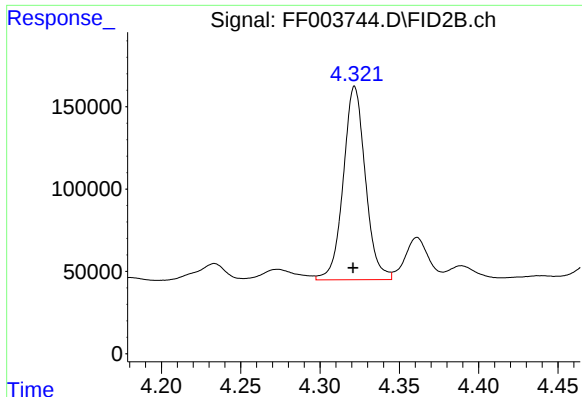

#2 N-DECANE


R.T.: 4.322 min
Delta R.T.: 0.001 min
Response: 1138838
Conc: 7.40 ug/ml

Instrument :
FID_F
ClientSampleId :
MW-11

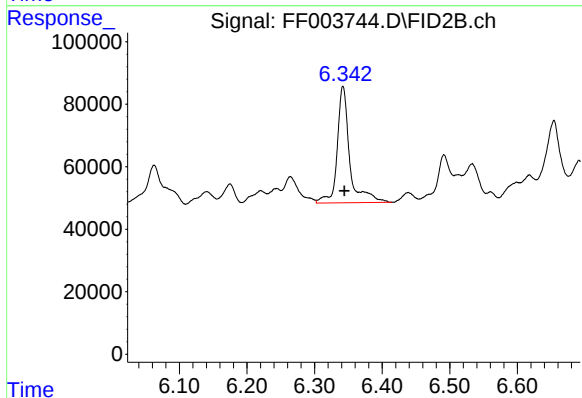


#3 N-DODECANE

R.T.: 6.342 min
Delta R.T.: -0.002 min
Response: 477422
Conc: 3.06 ug/ml

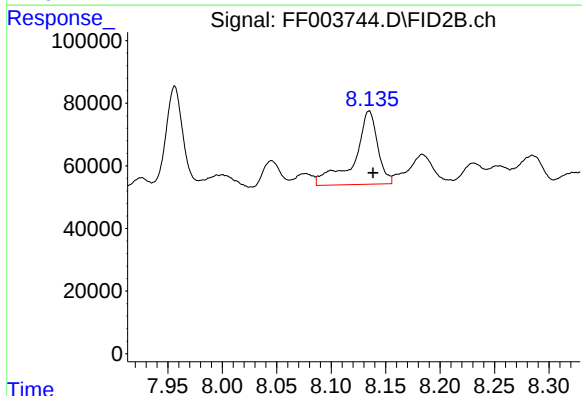


#4 N-TETRADECANE

R.T.: 8.135 min
Delta R.T.: -0.004 min
Response: 349962
Conc: 2.18 ug/ml

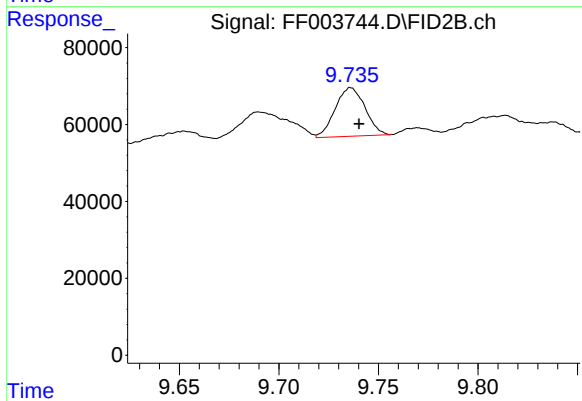

#5 N-HEXADECANE


R.T.: 9.736 min
Delta R.T.: -0.004 min
Response: 131569
Conc: 0.81 ug/ml

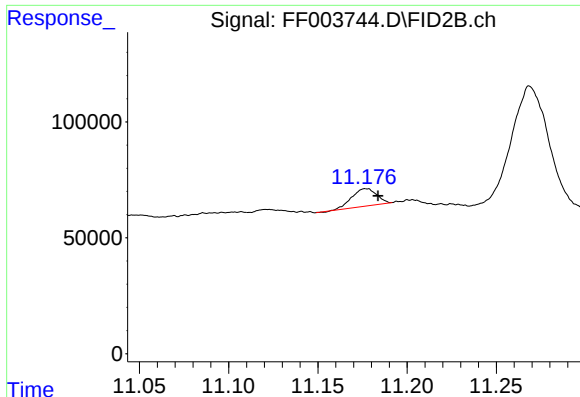

#6 N-OCTADECANE


R.T.: 11.177 min
Delta R.T.: -0.007 min
Response: 72514
Conc: 0.44 ug/ml

Instrument :
FID_F
ClientSampleId :
MW-11

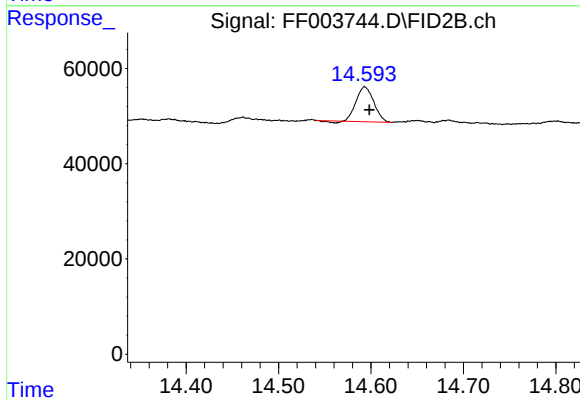

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.593 min
Delta R.T.: -0.005 min
Response: 96454
Conc: 0.69 ug/ml

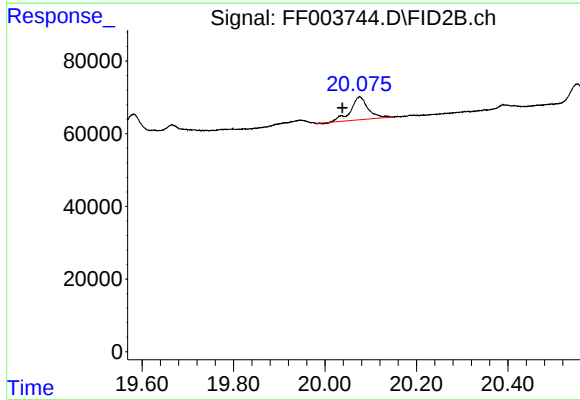

#16 N-HEXATRIACONTANE

R.T.: 20.076 min
Delta R.T.: 0.038 min
Response: 166696
Conc: 1.28 ug/ml