

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030619\
 Data File : FF003745.D
 Signal(s) : FID2B.ch
 Acq On : 06 Mar 2019 14:14
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Mar 07 00:20:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.593	2157190	15.494 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.774	100394	0.664 ug/ml
13) N-TRIACONTANE	17.665	151145	1.027 ug/ml
14) N-DOTRIACONTANE	18.515	465854	3.276 ug/ml
15) N-TETRATRIACONTANE	19.293	95905	0.716 ug/ml
16) N-HEXATRIACONTANE	20.080	940862	7.211 ug/ml
18) N-TETRACONTANE	21.692	872234	7.011 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030619\
Data File : FF003745.D
Signal(s) : FID2B.ch
Acq On : 06 Mar 2019 14:14
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 07 00:20:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

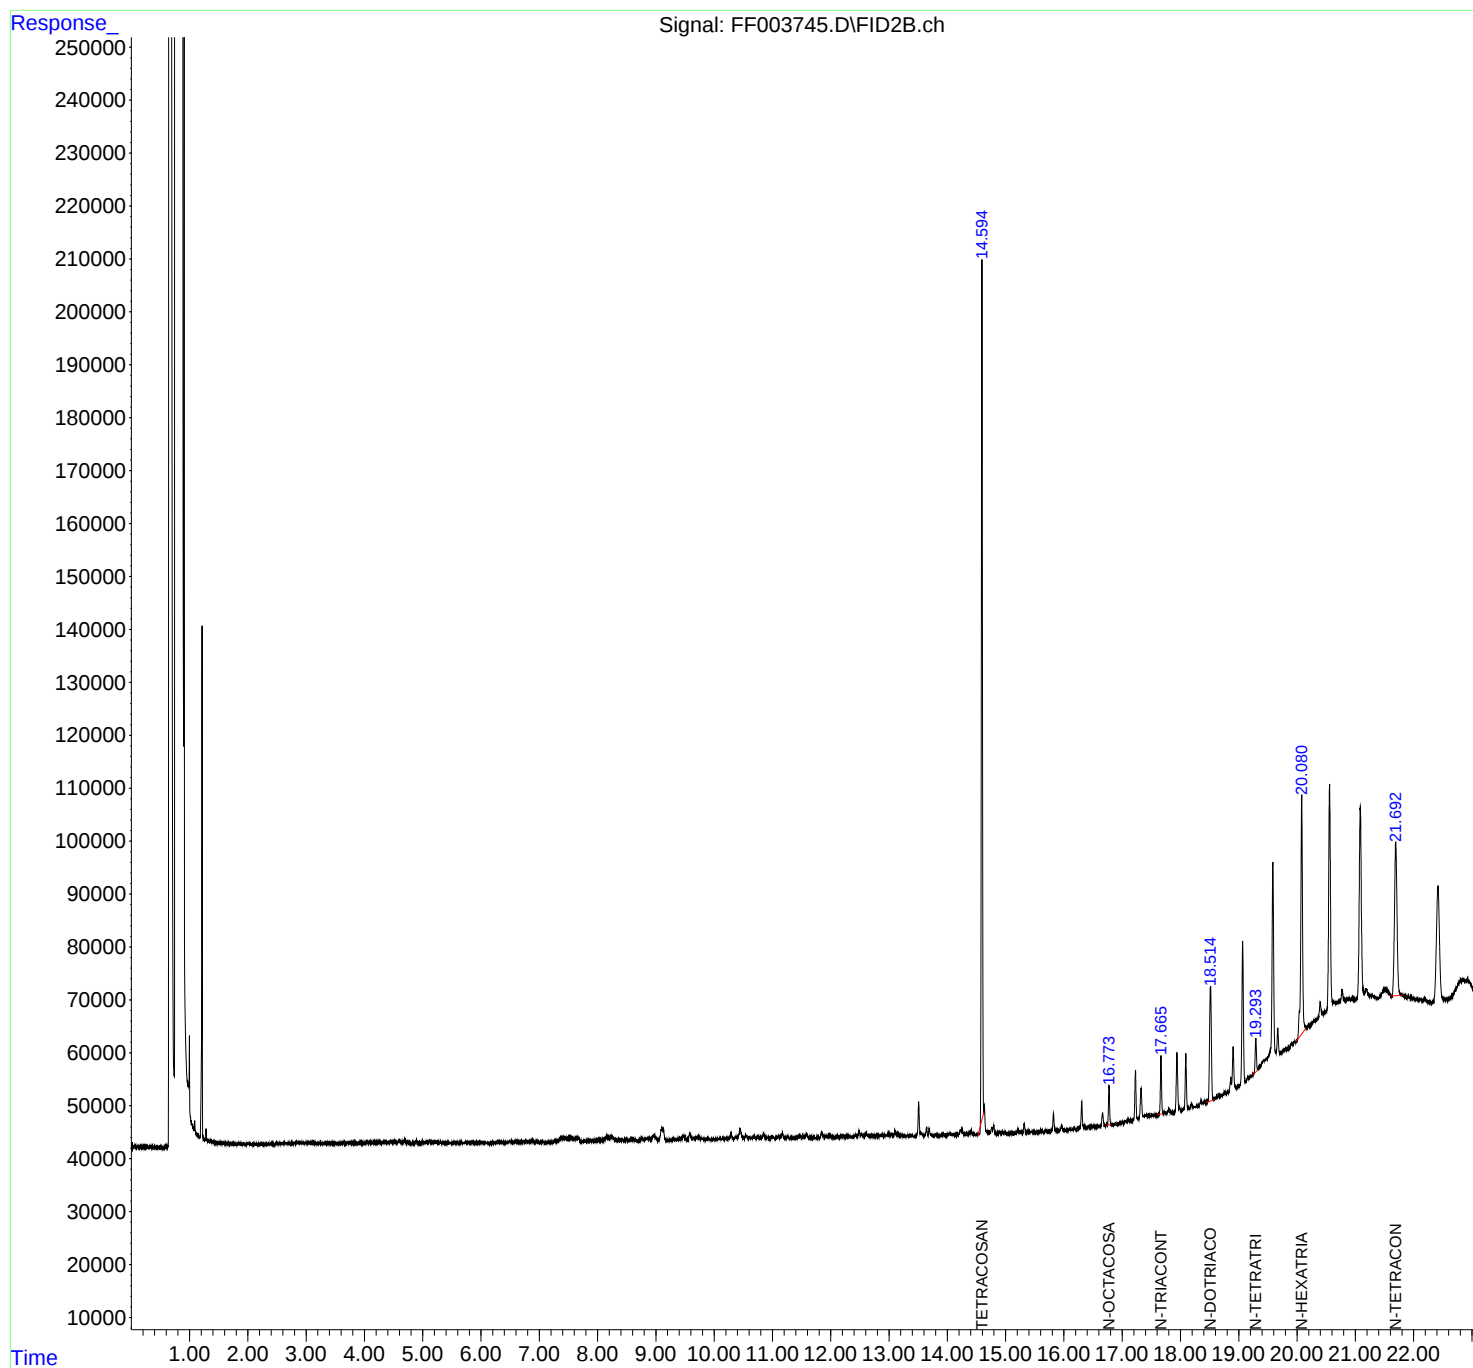


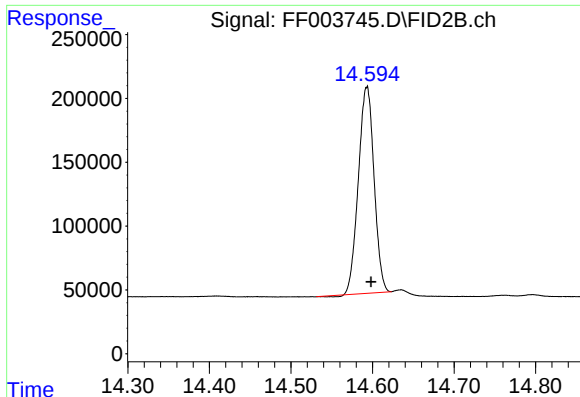

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.593 min
Delta R.T.: -0.005 min
Response: 2157190
Conc: 15.49 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

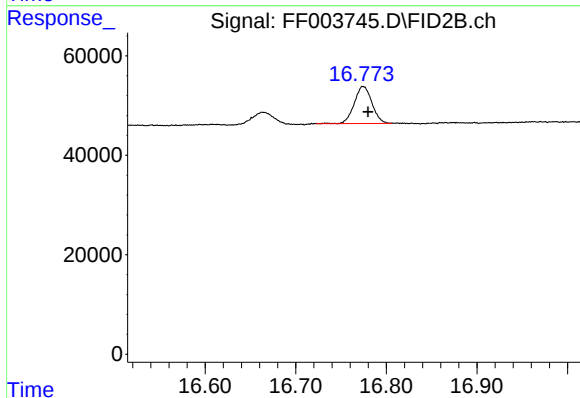


#12 N-OCTACOSANE

R.T.: 16.774 min
Delta R.T.: -0.005 min
Response: 100394
Conc: 0.66 ug/ml

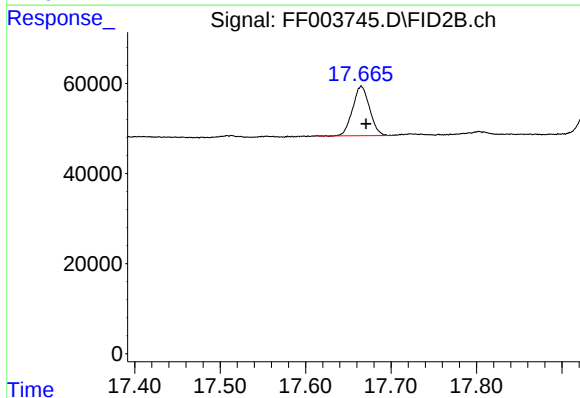


#13 N-TRIACONTANE

R.T.: 17.665 min
Delta R.T.: -0.006 min
Response: 151145
Conc: 1.03 ug/ml

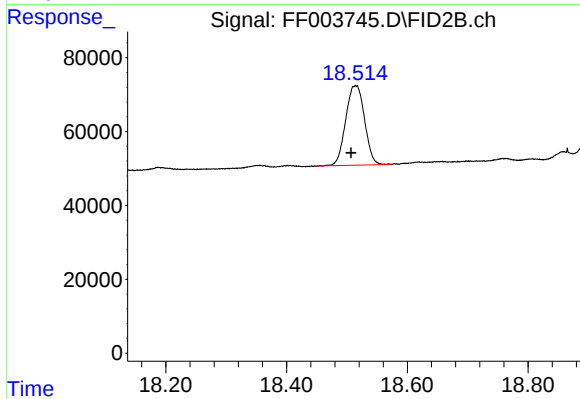

#14 N-DOTRIACONTANE


R.T.: 18.515 min
Delta R.T.: 0.008 min
Response: 465854
Conc: 3.28 ug/ml

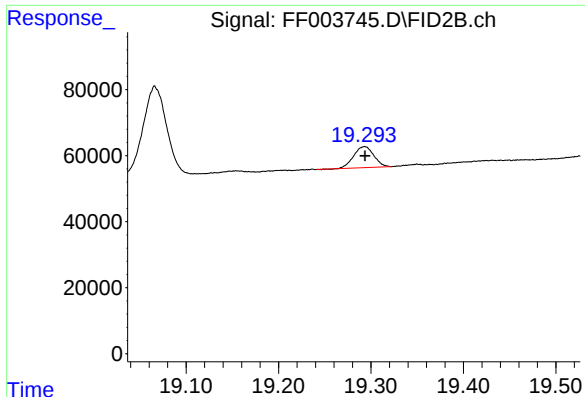

#15 N-TETRATRIACONTANE


R.T.: 19.293 min
Delta R.T.: 0.000 min
Response: 95905
Conc: 0.72 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

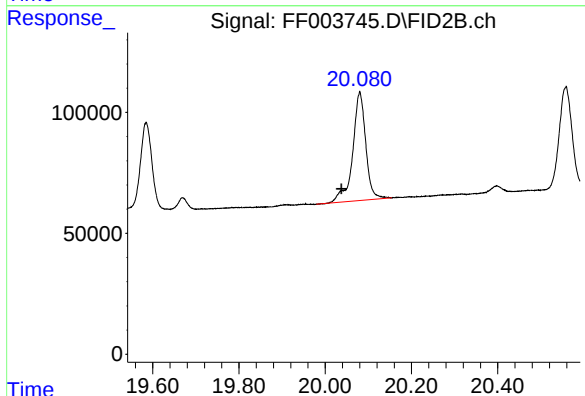

#16 N-HEXATRIACONTANE

R.T.: 20.080 min
Delta R.T.: 0.042 min
Response: 940862
Conc: 7.21 ug/ml

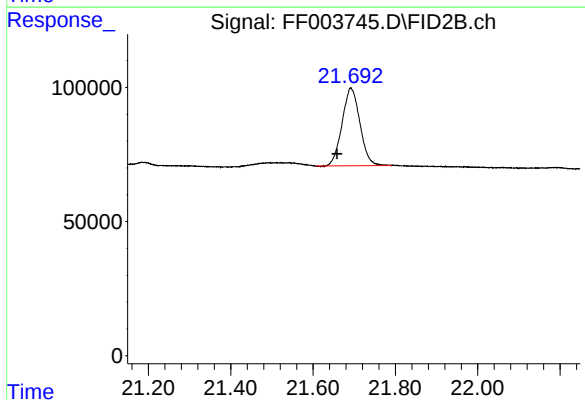

#18 N-TETRACONTANE

R.T.: 21.692 min
Delta R.T.: 0.033 min
Response: 872234
Conc: 7.01 ug/ml