

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030619\
Data File : FF003747.D
Signal(s) : FID2B.ch
Acq On : 06 Mar 2019 16:46
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Mar 07 00:21:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.514	165325	1.163 ug/ml
16) N-HEXATRIACONTANE	20.076	787958	6.039 ug/ml
18) N-TETRACONTANE	21.685	604722	4.861 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030619\
Data File : FF003747.D
Signal(s) : FID2B.ch
Acq On : 06 Mar 2019 16:46
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Mar 07 00:21:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

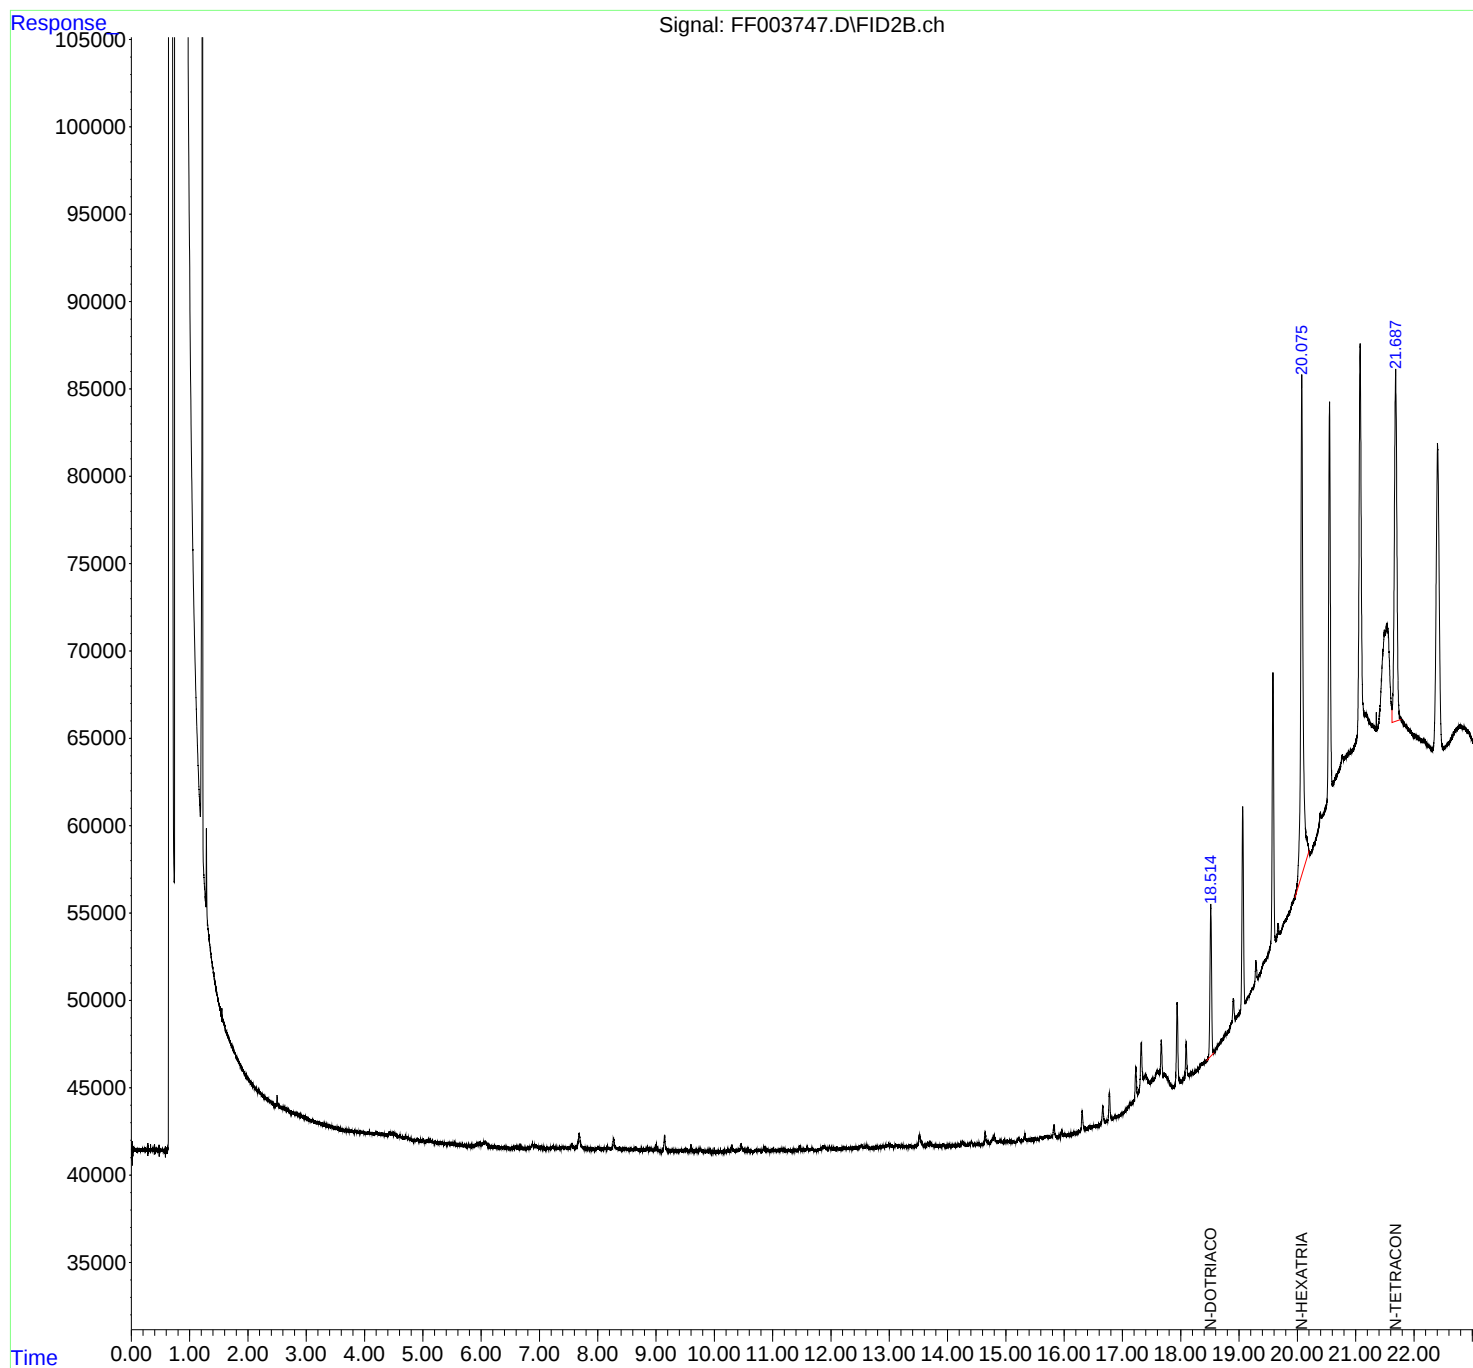


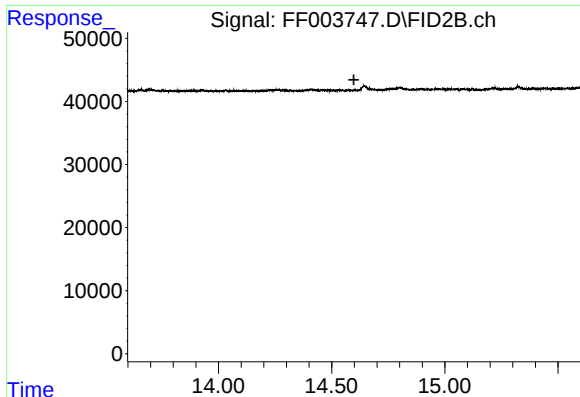

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.598 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :
MECL2

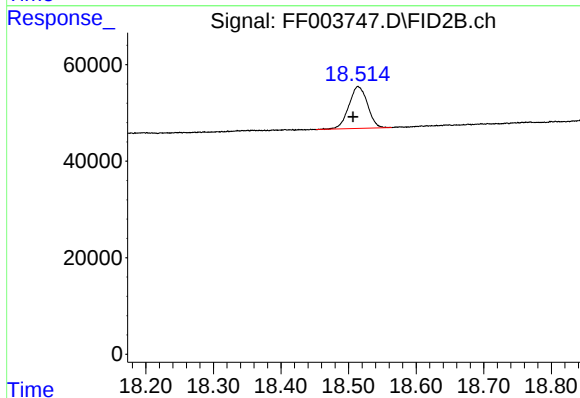


#14 N-DOTRIACONTANE

R.T.: 18.514 min
Delta R.T.: 0.007 min
Response: 165325
Conc: 1.16 ug/ml

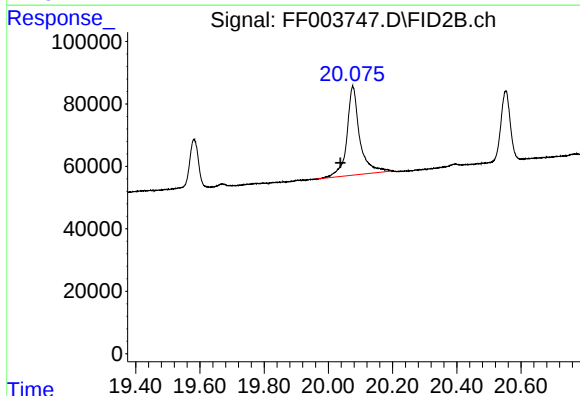

#16 N-HEXATRIACONTANE

R.T.: 20.076 min
Delta R.T.: 0.038 min
Response: 787958
Conc: 6.04 ug/ml

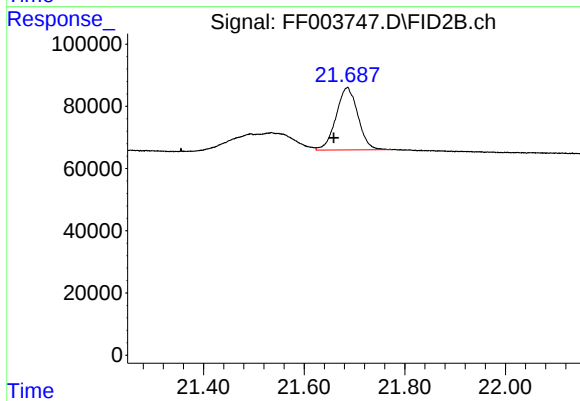

#18 N-TETRACONTANE

R.T.: 21.685 min
Delta R.T.: 0.027 min
Response: 604722
Conc: 4.86 ug/ml