

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030719\
 Data File : FF003750.D
 Signal(s) : FID2B.ch
 Acq On : 07 Mar 2019 11:31
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Mar 07 23:47:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.337	3183766	20.400 ug/ml
12) N-OCTACOSANE	16.772	3157744	20.896 ug/ml
13) N-TRIACONTANE	17.661	739578	5.028 ug/ml
14) N-DOTRIACONTANE	18.497	880006	6.188 ug/ml
15) N-TETRATRIACONTANE	19.285	633535	4.732 ug/ml
16) N-HEXATRIACONTANE	20.028	473974	3.633 ug/ml
17) N-OCTATRIACONTANE	20.759	245185	2.123 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030719\
Data File : FF003750.D
Signal(s) : FID2B.ch
Acq On : 07 Mar 2019 11:31
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 07 23:47:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

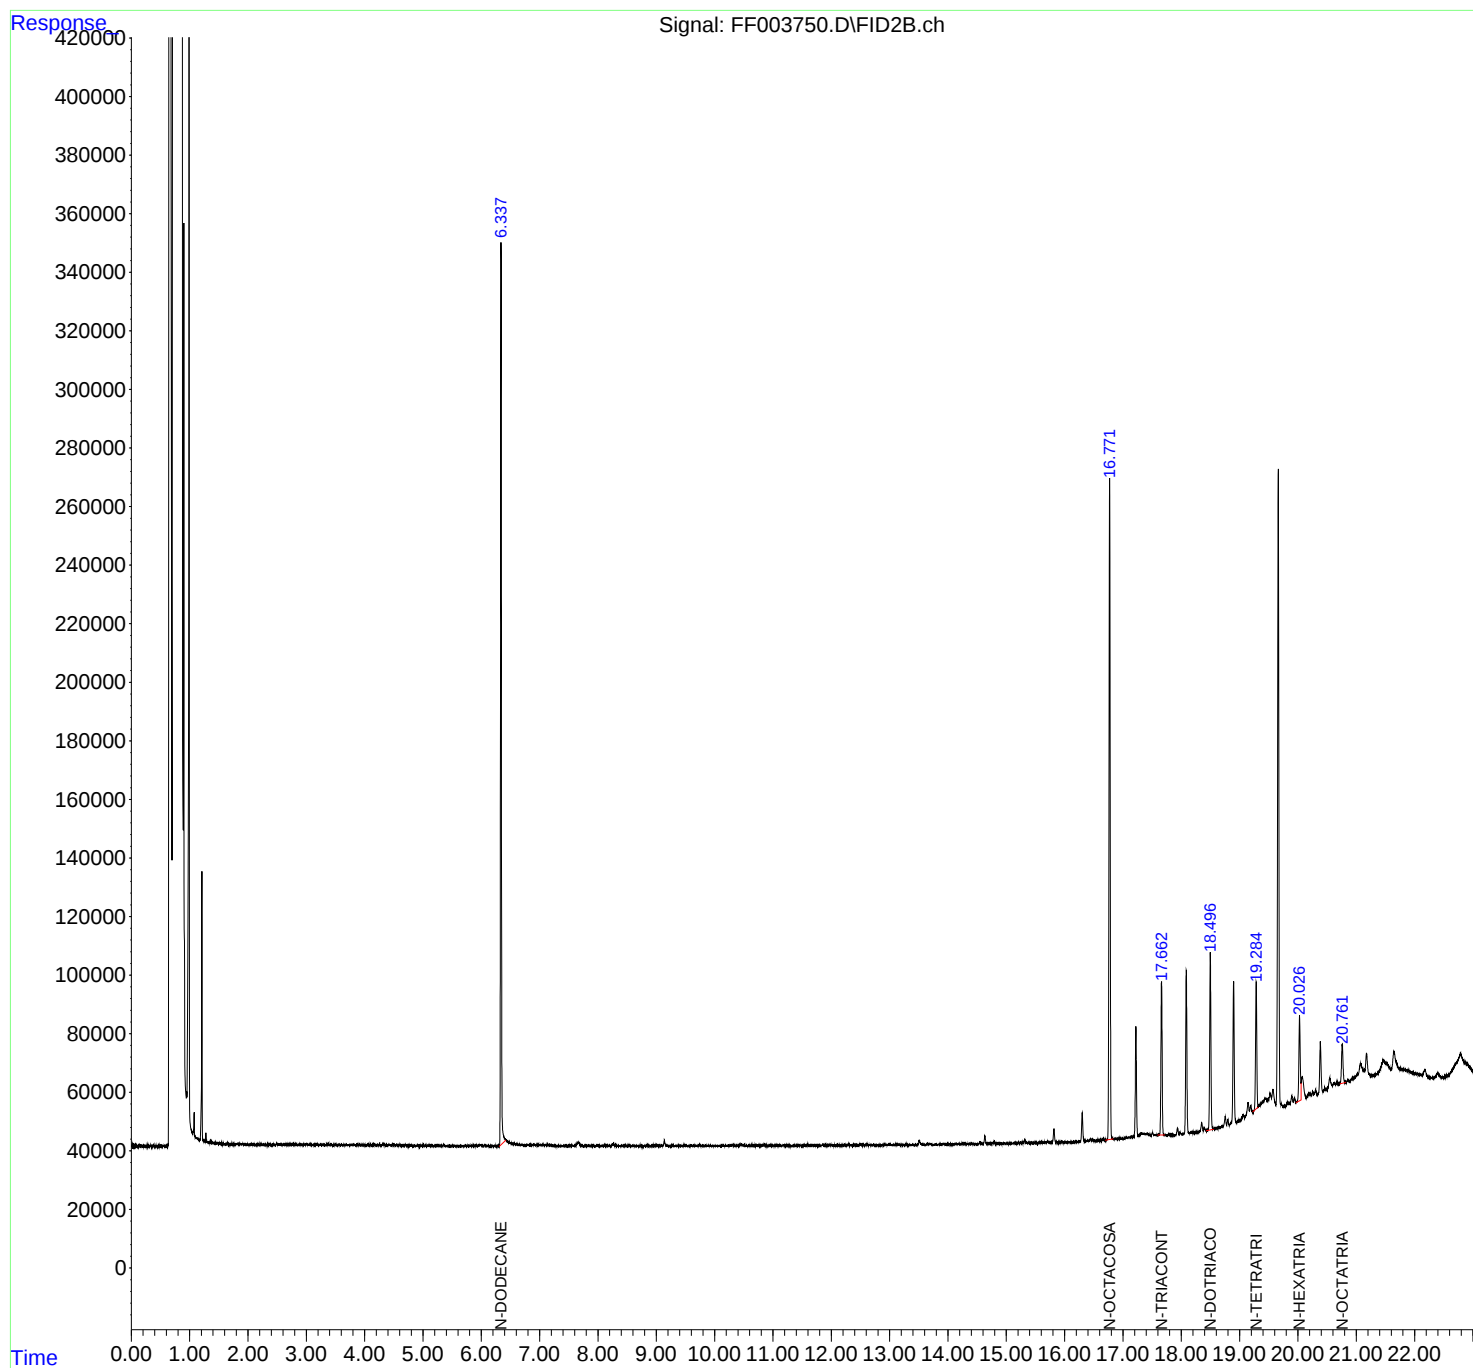


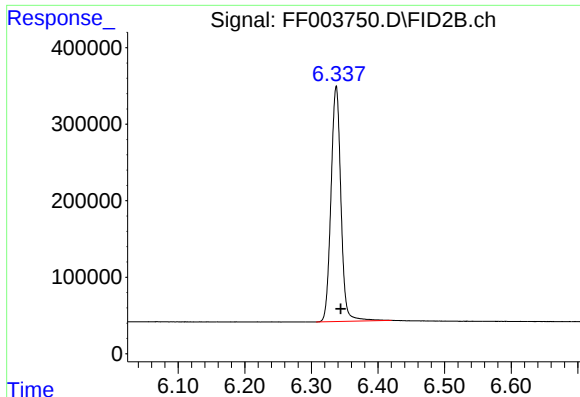

#3 N-DODECANE


R.T.: 6.337 min
Delta R.T.: -0.007 min
Response: 3183766
Conc: 20.40 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

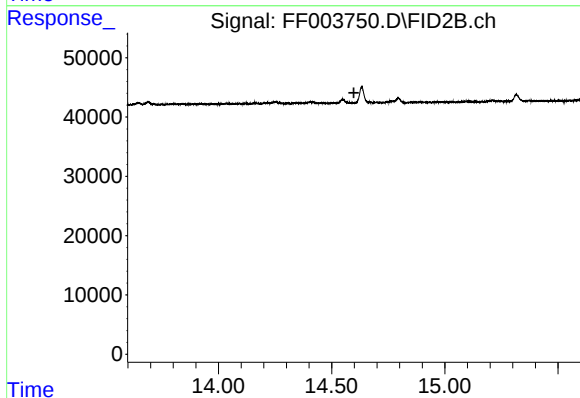


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.598 min
Response: 0
Conc: N.D.

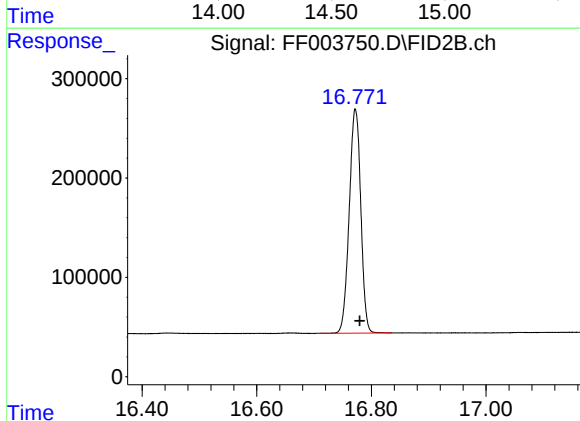


#12 N-OCTACOSANE

R.T.: 16.772 min
Delta R.T.: -0.008 min
Response: 3157744
Conc: 20.90 ug/ml

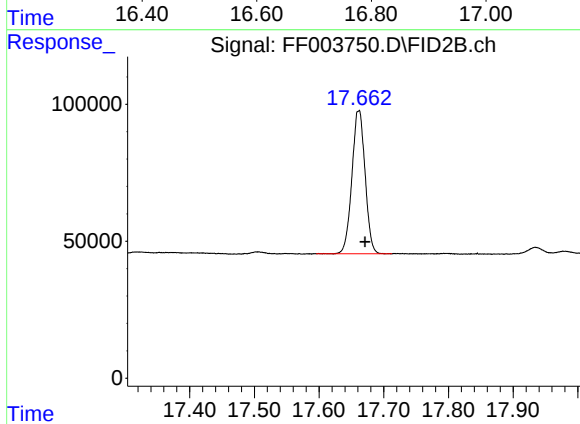

#13 N-TRIACONTANE


R.T.: 17.661 min
Delta R.T.: -0.009 min
Response: 739578
Conc: 5.03 ug/ml

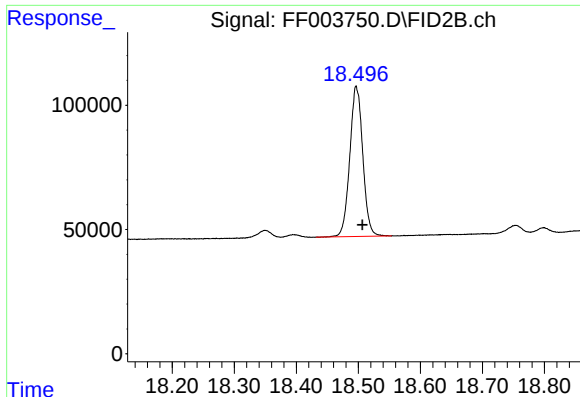

#14 N-DOTRIACONTANE


R.T.: 18.497 min
Delta R.T.: -0.010 min
Response: 880006
Conc: 6.19 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

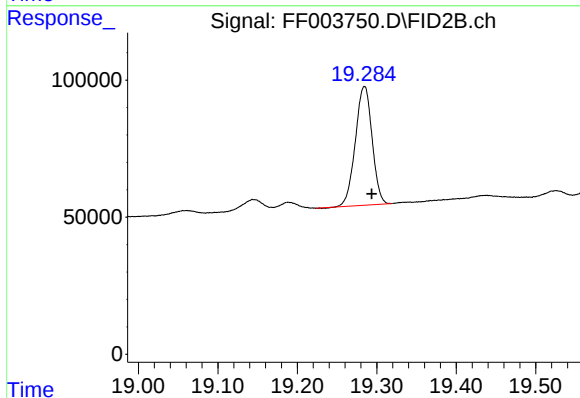


#15 N-TETRATRIACONTANE

R.T.: 19.285 min
Delta R.T.: -0.009 min
Response: 633535
Conc: 4.73 ug/ml

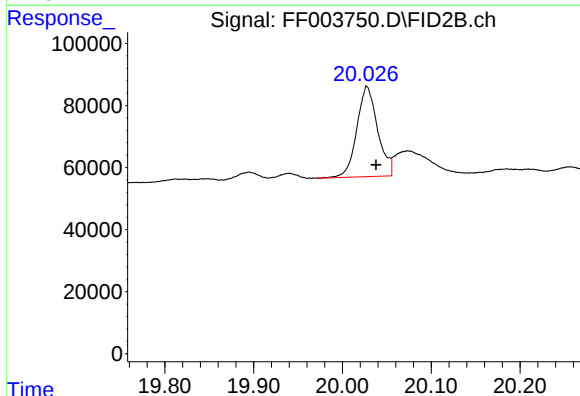

#16 N-HEXATRIACONTANE

R.T.: 20.028 min
Delta R.T.: -0.010 min
Response: 473974
Conc: 3.63 ug/ml

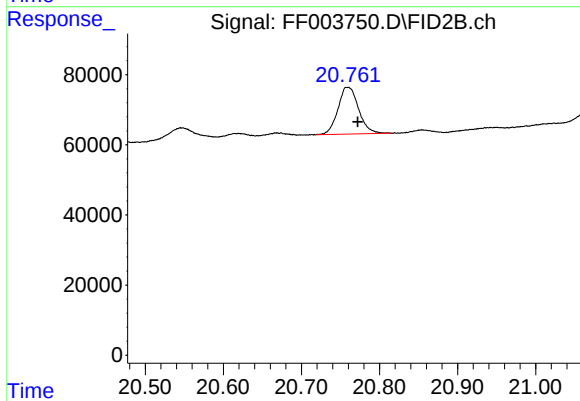

#17 N-OCTATRIACONTANE

R.T.: 20.759 min
Delta R.T.: -0.013 min
Response: 245185
Conc: 2.12 ug/ml