

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030719\
 Data File : FF003751.D
 Signal(s) : FID2B.ch
 Acq On : 07 Mar 2019 12:02
 Operator : AJ\SJ
 Sample : PB117510BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 PB117510BL

Integration File: autoint1.e
 Quant Time: Mar 07 23:48:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.592	2088034	14.997 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.507	183833	1.293 ug/ml
16) N-HEXATRIACONTANE	20.066	403456	3.092 ug/ml
18) N-TETRACONTANE	21.674	588560	4.731 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030719\
Data File : FF003751.D
Signal(s) : FID2B.ch
Acq On : 07 Mar 2019 12:02
Operator : AJ\SJ
Sample : PB117510BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
PB117510BL

Integration File: autoint1.e
Quant Time: Mar 07 23:48:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

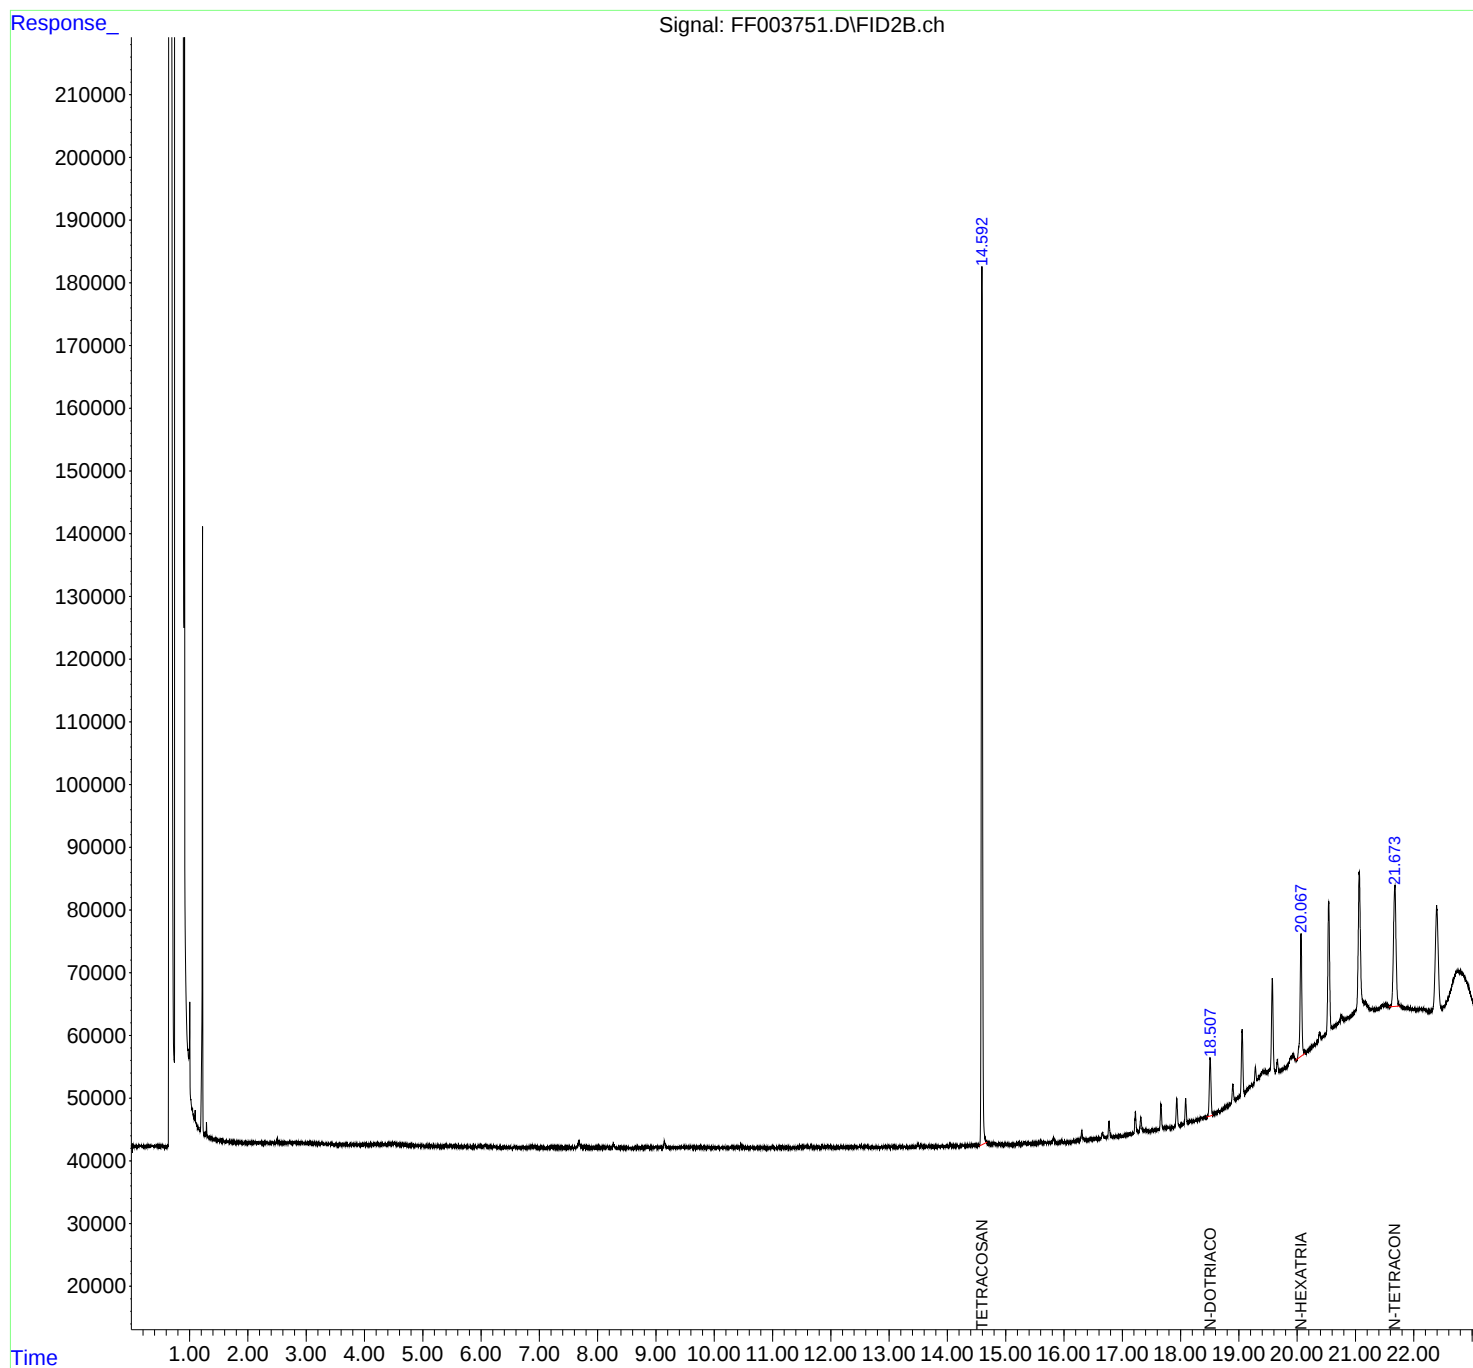


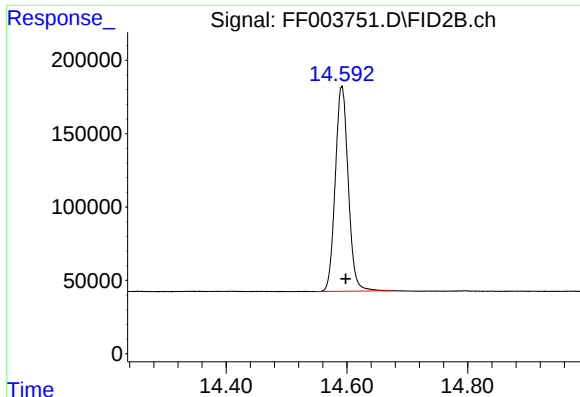

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.592 min
Delta R.T.: -0.007 min
Response: 2088034
Conc: 15.00 ug/ml

Instrument :
FID_F
ClientSampleId :
PB117510BL

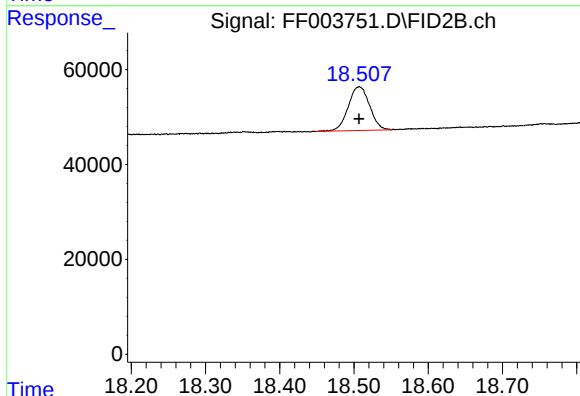


#14 N-DOTRIACONTANE

R.T.: 18.507 min
Delta R.T.: 0.000 min
Response: 183833
Conc: 1.29 ug/ml

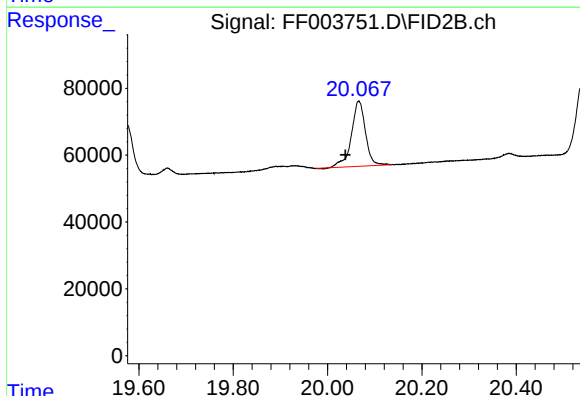

#16 N-HEXATRIACONTANE

R.T.: 20.066 min
Delta R.T.: 0.028 min
Response: 403456
Conc: 3.09 ug/ml

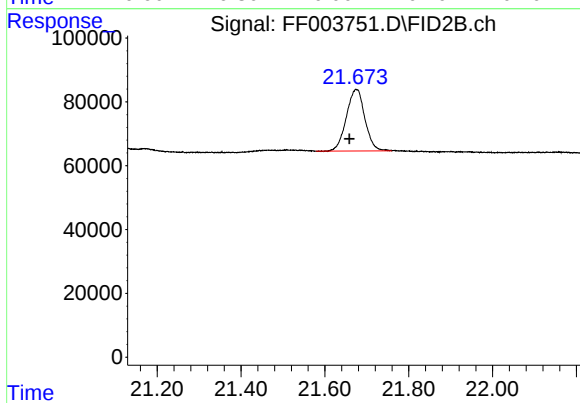

#18 N-TETRACONTANE

R.T.: 21.674 min
Delta R.T.: 0.016 min
Response: 588560
Conc: 4.73 ug/ml