

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF030719\  
Data File : FF003753.D  
Signal(s) : FID2B.ch  
Acq On : 07 Mar 2019 13:10  
Operator : AJ\SJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Mar 07 23:48:22 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF030119.M  
Quant Title :  
QLast Update : Mon Mar 04 08:35:38 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.590 | 2163938  | 15.542 ug/ml |
| Target Compounds              |        |          |              |
| 14) N-DOTRIACONTANE           | 18.500 | 166028   | 1.167 ug/ml  |
| 16) N-HEXATRIACONTANE         | 20.070 | 1160941  | 8.897 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF030719\  
Data File : FF003753.D  
Signal(s) : FID2B.ch  
Acq On : 07 Mar 2019 13:10  
Operator : AJ\SJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Mar 07 23:48:22 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF030119.M  
Quant Title :  
QLast Update : Mon Mar 04 08:35:38 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

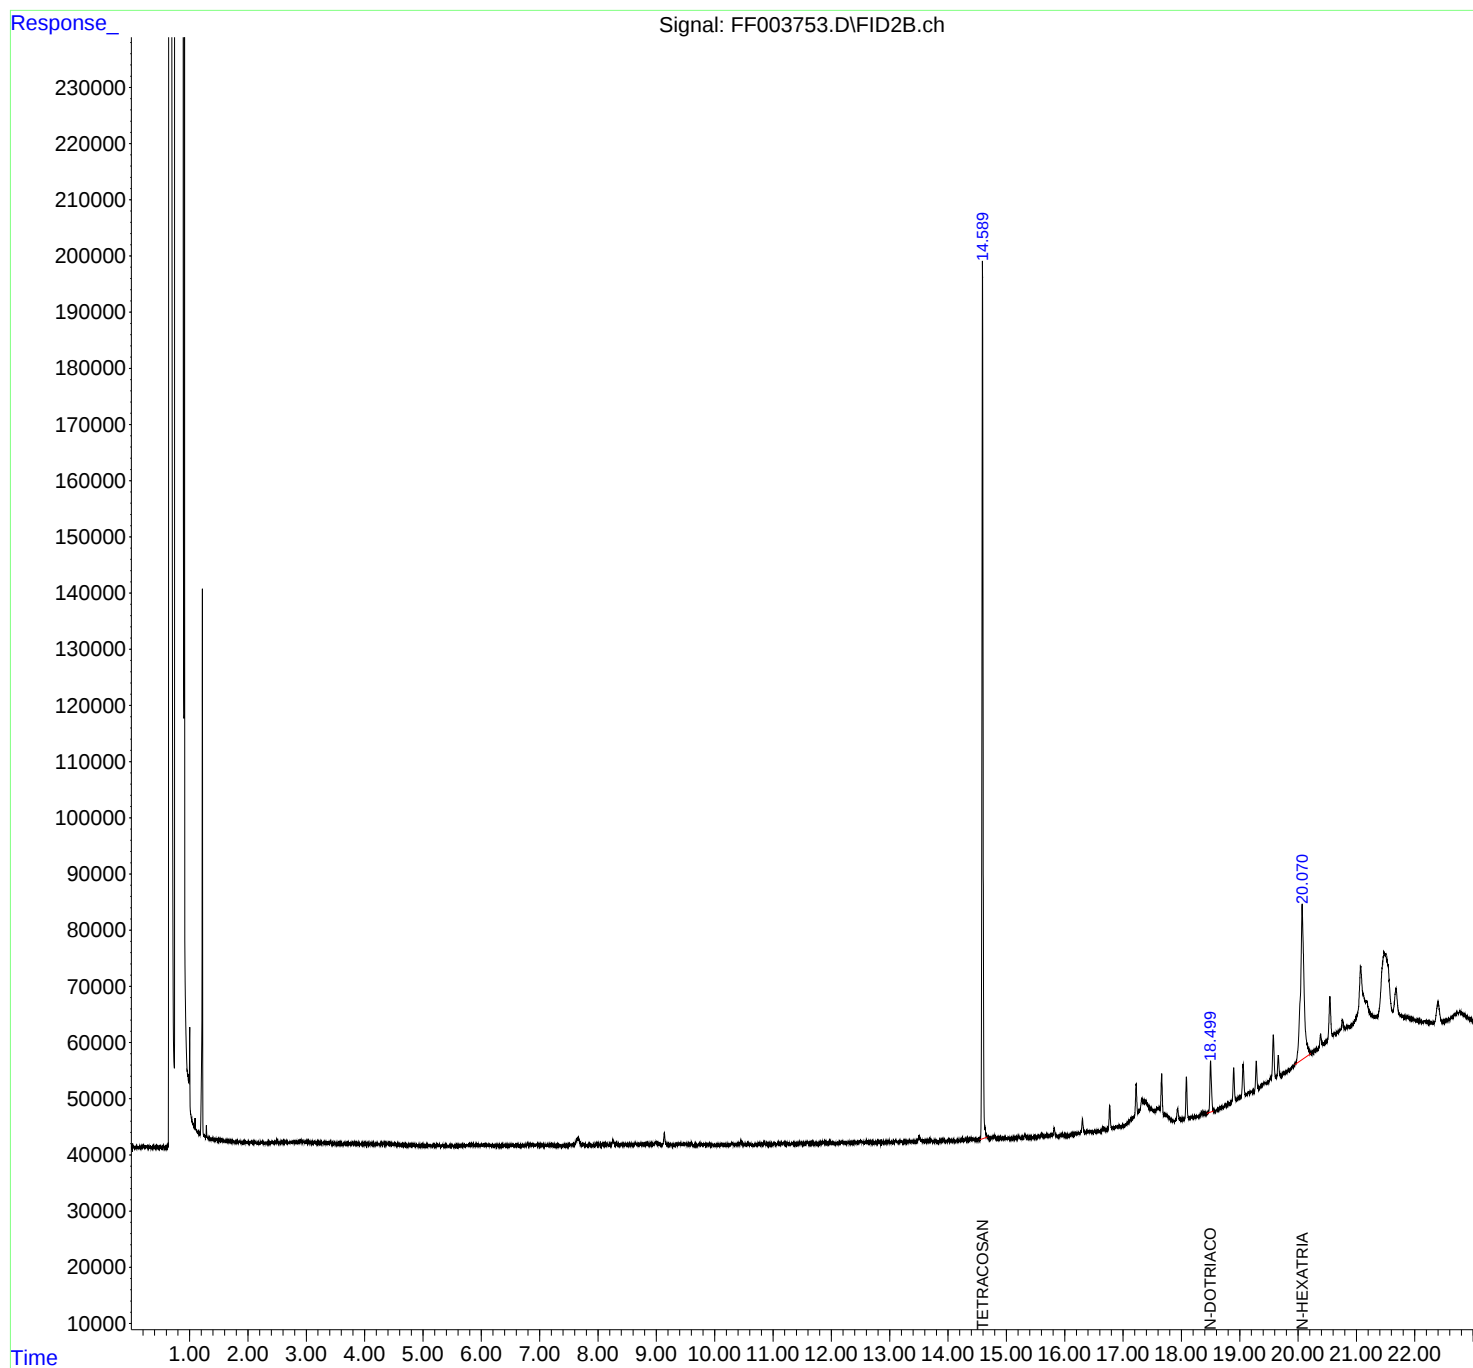


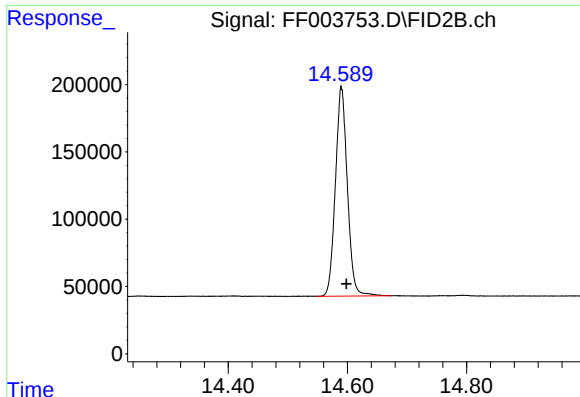

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.590 min  
Delta R.T.: -0.008 min  
Response: 2163938  
Conc: 15.54 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
I.BLK

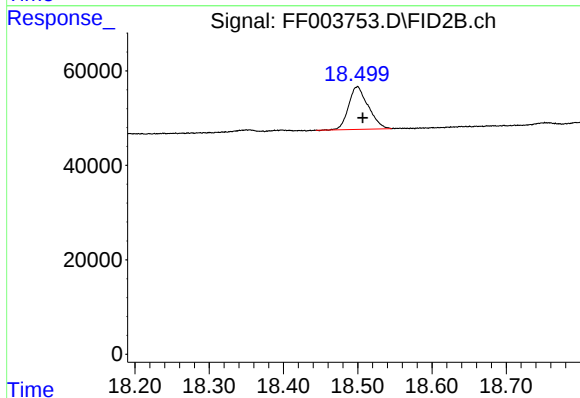

#14 N-DOTRIACONTANE

R.T.: 18.500 min  
Delta R.T.: -0.007 min  
Response: 166028  
Conc: 1.17 ug/ml

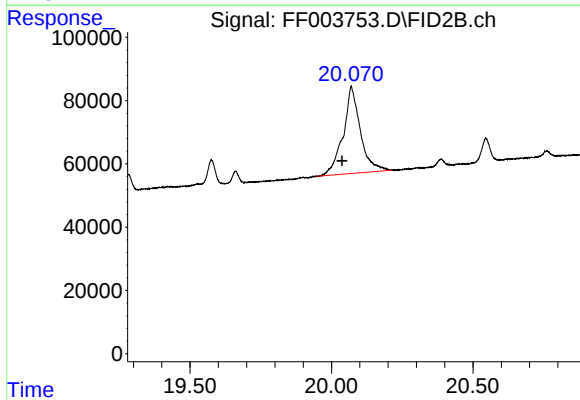

#16 N-HEXATRIACONTANE

R.T.: 20.070 min  
Delta R.T.: 0.032 min  
Response: 1160941  
Conc: 8.90 ug/ml