

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030819\
 Data File : FF003758.D
 Signal(s) : FID2B.ch
 Acq On : 08 Mar 2019 10:37
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Mar 08 21:46:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.337	3654397	23.416 ug/ml
11) N-HEXACOSANE	15.815	109382	0.709 ug/ml
12) N-OCTACOSANE	16.770	3707095	24.532 ug/ml
13) N-TRIACONTANE	17.658	976174	6.636 ug/ml
14) N-DOTRIACONTANE	18.496	2063276	14.509 ug/ml
15) N-TETRATRIACONTANE	19.280	770871	5.757 ug/ml
16) N-HEXATRIACONTANE	20.026	556843	4.268 ug/ml
17) N-OCTATRIACONTANE	20.757	307430	2.663 ug/ml
18) N-TETRACONTANE	21.678	4671729	37.552 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030819\
Data File : FF003758.D
Signal(s) : FID2B.ch
Acq On : 08 Mar 2019 10:37
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 08 21:46:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

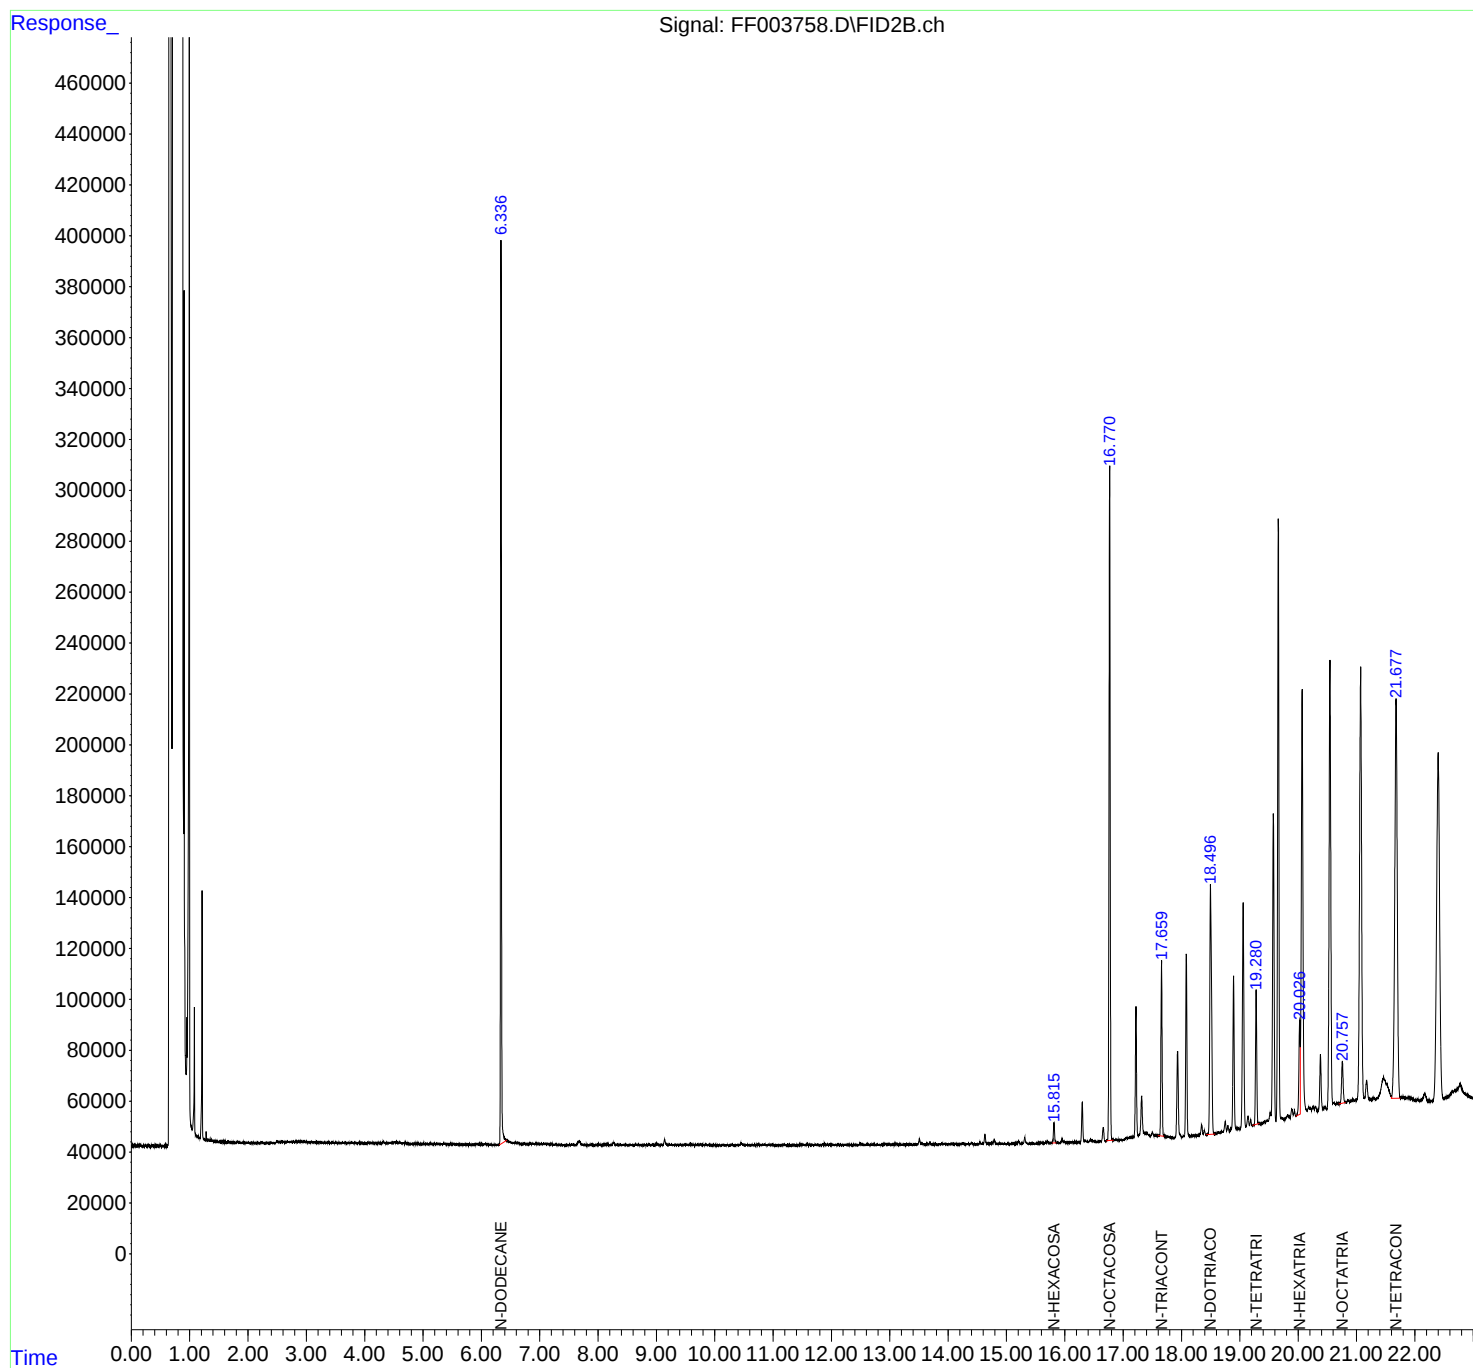


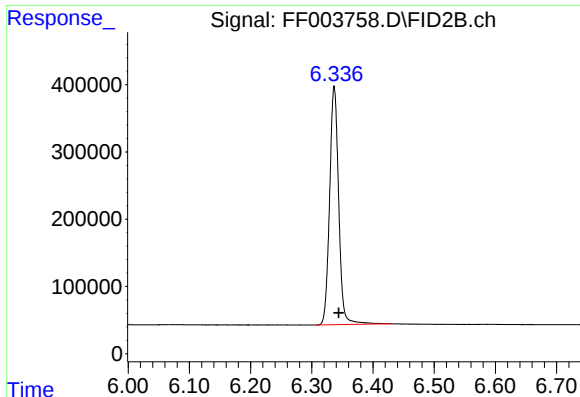

#3 N-DODECANE


R.T.: 6.337 min
Delta R.T.: -0.007 min
Response: 3654397
Conc: 23.42 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

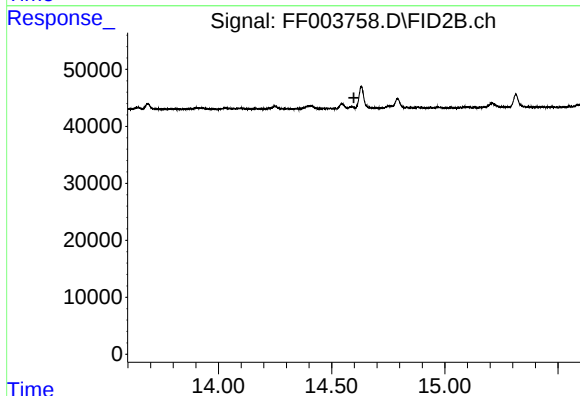


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.598 min
Response: 0
Conc: N.D.

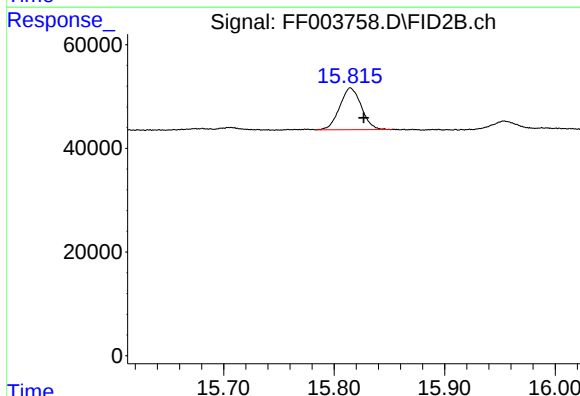


#11 N-HEXACOSANE

R.T.: 15.815 min
Delta R.T.: -0.012 min
Response: 109382
Conc: 0.71 ug/ml

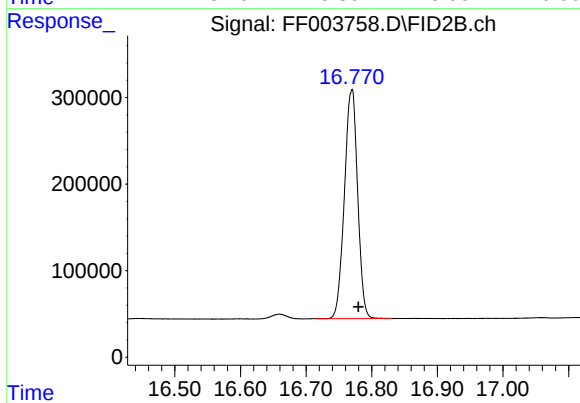

#12 N-OCTACOSANE


R.T.: 16.770 min
Delta R.T.: -0.010 min
Response: 3707095
Conc: 24.53 ug/ml

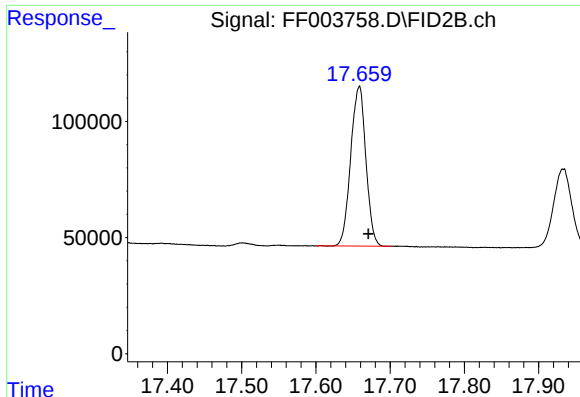

#13 N-TRIACONTANE


R.T.: 17.658 min
Delta R.T.: -0.012 min
Response: 976174
Conc: 6.64 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

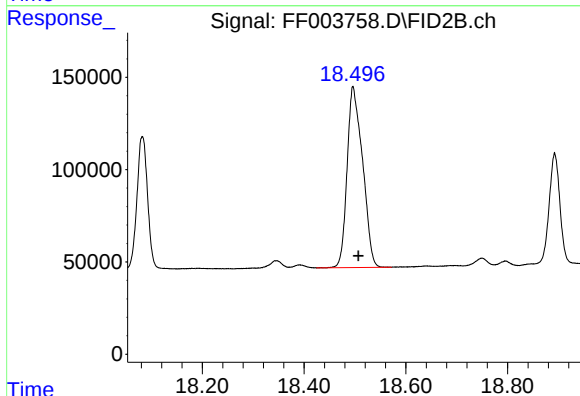


#14 N-DOTRIACONTANE

R.T.: 18.496 min
Delta R.T.: -0.011 min
Response: 2063276
Conc: 14.51 ug/ml

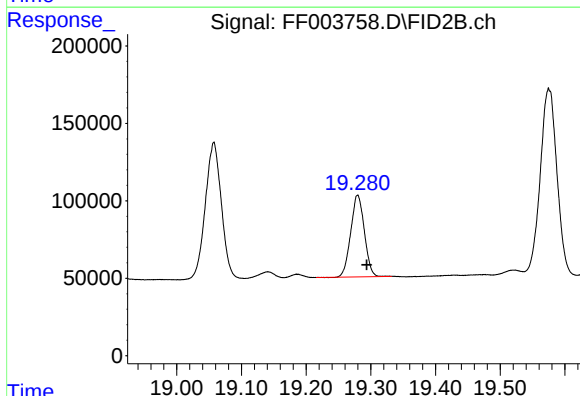


#15 N-TETRATRIACONTANE

R.T.: 19.280 min
Delta R.T.: -0.014 min
Response: 770871
Conc: 5.76 ug/ml

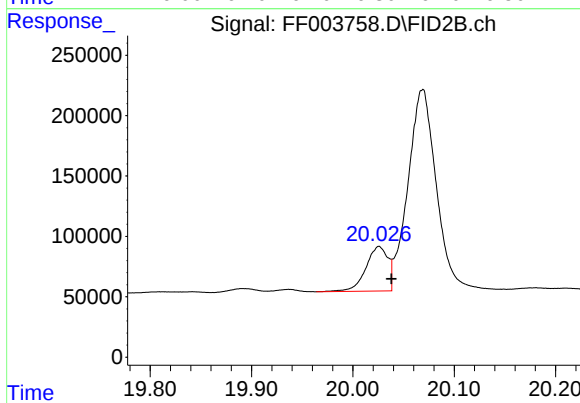

#16 N-HEXATRIACONTANE


R.T.: 20.026 min
Delta R.T.: -0.012 min
Response: 556843
Conc: 4.27 ug/ml

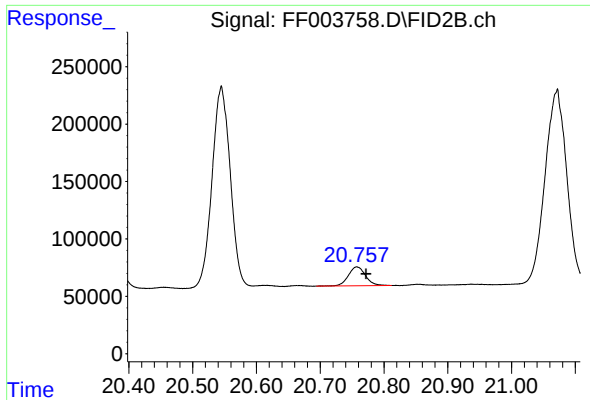

#17 N-OCTATRIACONTANE

R.T.: 20.757 min
Delta R.T.: -0.015 min
Response: 307430
Conc: 2.66 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

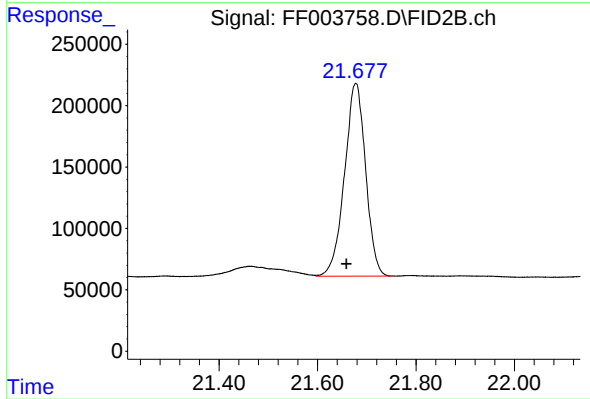

#18 N-TETRACONTANE

R.T.: 21.678 min
Delta R.T.: 0.019 min
Response: 4671729
Conc: 37.55 ug/ml