

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030819\
 Data File : FF003761.D
 Signal(s) : FID2B.ch
 Acq On : 08 Mar 2019 13:38
 Operator : AJ\SJ
 Sample : K1732-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SB-07(22-23)-20190301

Integration File: autoint1.e
 Quant Time: Mar 08 21:46:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.587	2392221	17.182 ug/ml
Target Compounds			
4) N-TETRADECANE	8.195f	183061	1.142 ug/ml
11) N-HEXACOSANE	15.814	97184	0.630 ug/ml
12) N-OCTACOSANE	16.766	127771	0.846 ug/ml
13) N-TRIACONTANE	17.657	147052	1.000 ug/ml
14) N-DOTRIACONTANE	18.493	126213	0.888 ug/ml
16) N-HEXATRIACONTANE	20.068	270750	2.075 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030819\
Data File : FF003761.D
Signal(s) : FID2B.ch
Acq On : 08 Mar 2019 13:38
Operator : AJ\SJ
Sample : K1732-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SB-07(22-23)-20190301

Integration File: autoint1.e
Quant Time: Mar 08 21:46:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

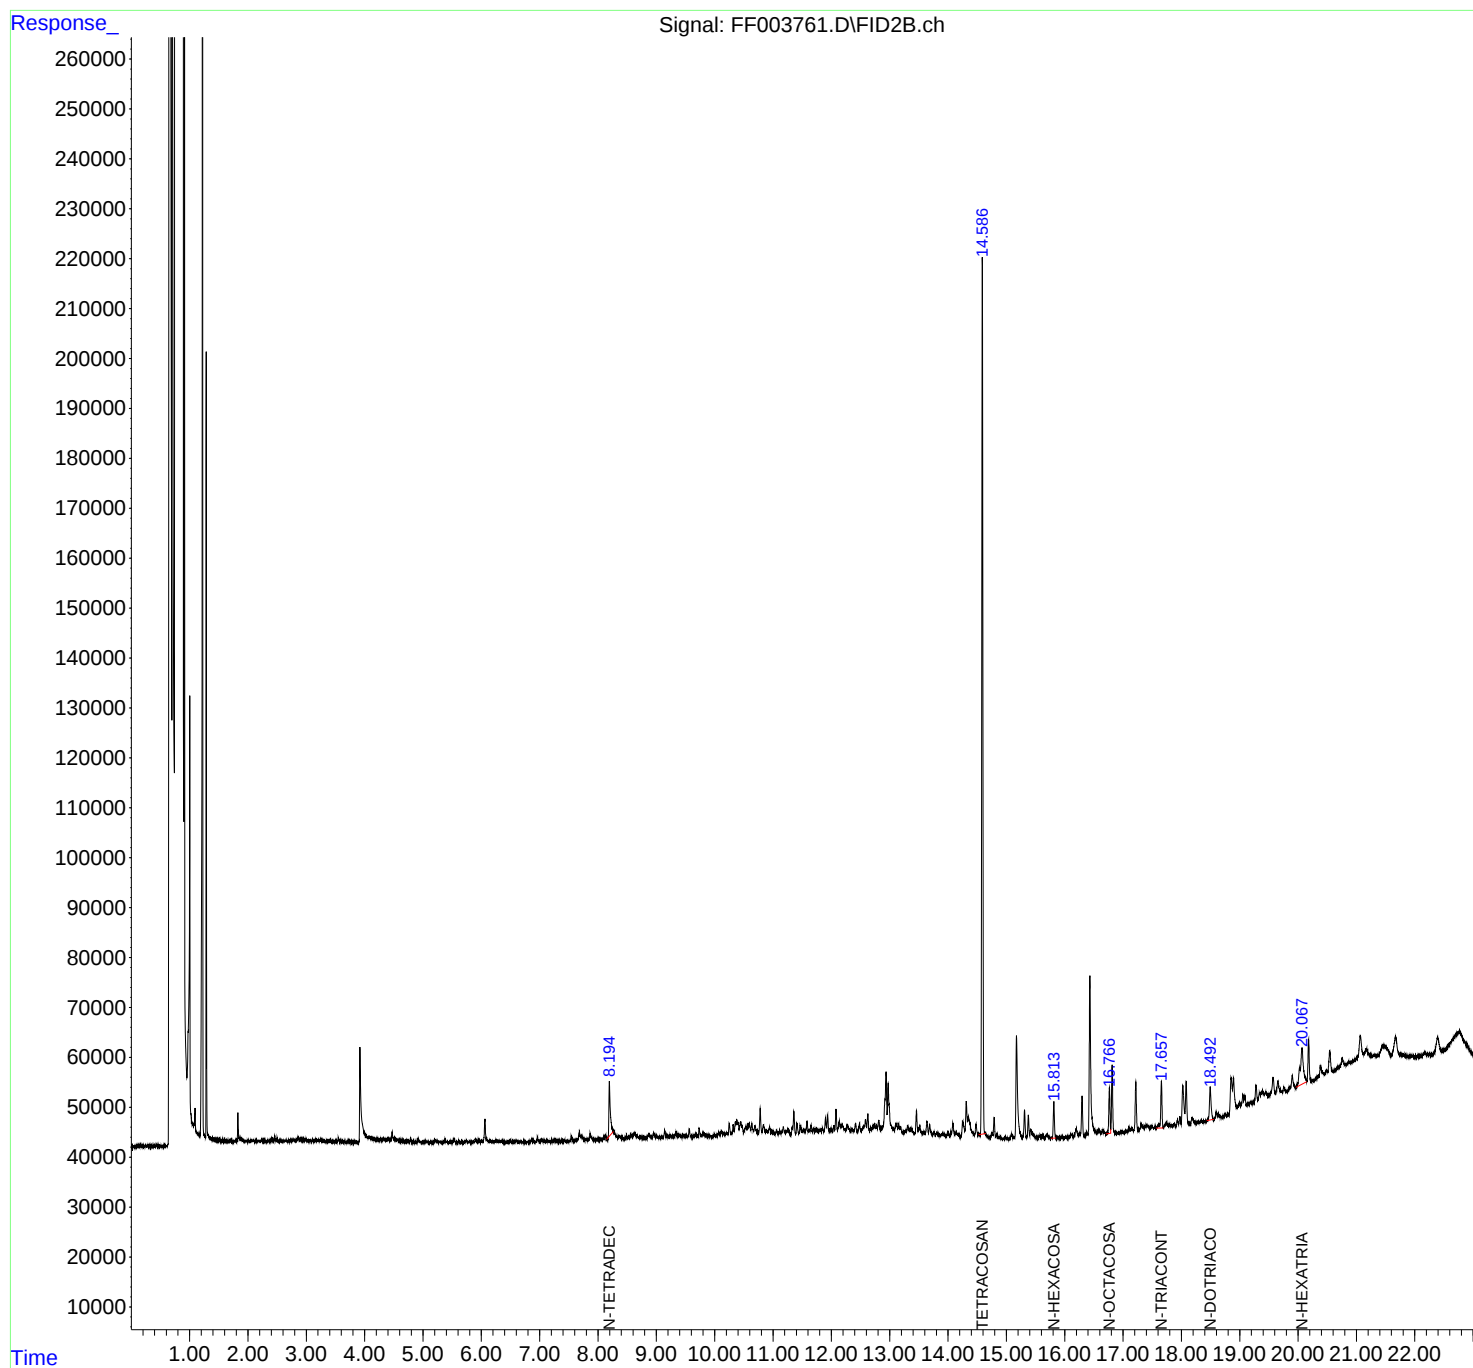


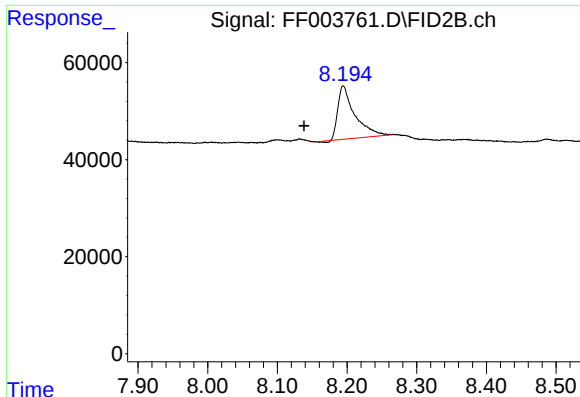

#4 N-TETRADECANE


R.T.: 8.195 min
Delta R.T.: 0.056 min
Response: 183061
Conc: 1.14 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-07(22-23)-20190301

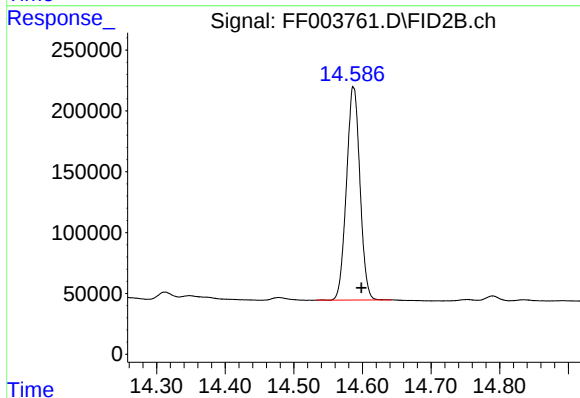


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.587 min
Delta R.T.: -0.011 min
Response: 2392221
Conc: 17.18 ug/ml

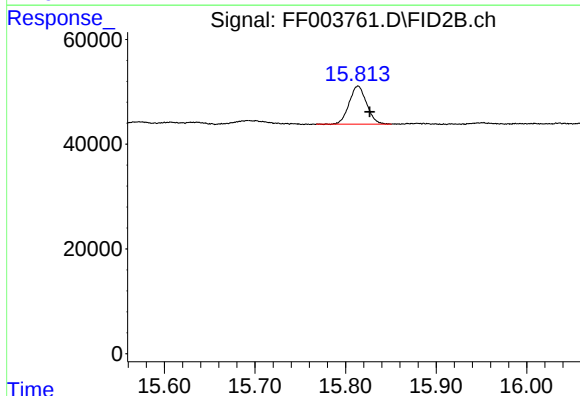


#11 N-HEXACOSANE

R.T.: 15.814 min
Delta R.T.: -0.013 min
Response: 97184
Conc: 0.63 ug/ml

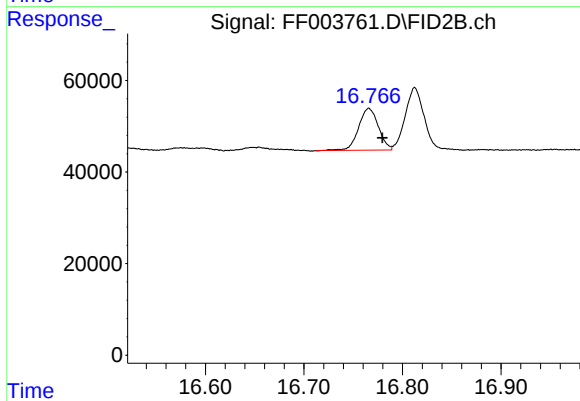

#12 N-OCTACOSANE


R.T.: 16.766 min
Delta R.T.: -0.014 min
Response: 127771
Conc: 0.85 ug/ml

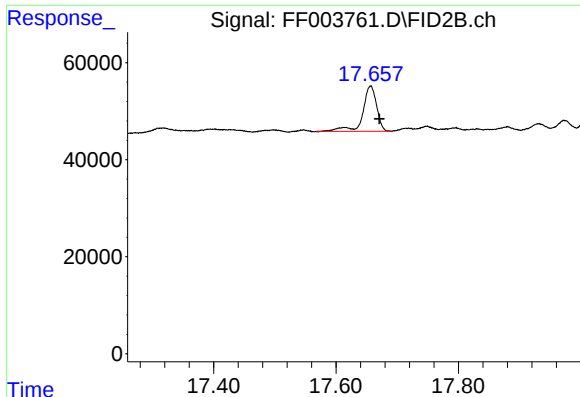

#13 N-TRIACONTANE


R.T.: 17.657 min
Delta R.T.: -0.014 min
Response: 147052
Conc: 1.00 ug/ml

Instrument :
FID_F
ClientSampleId :
SB-07(22-23)-20190301

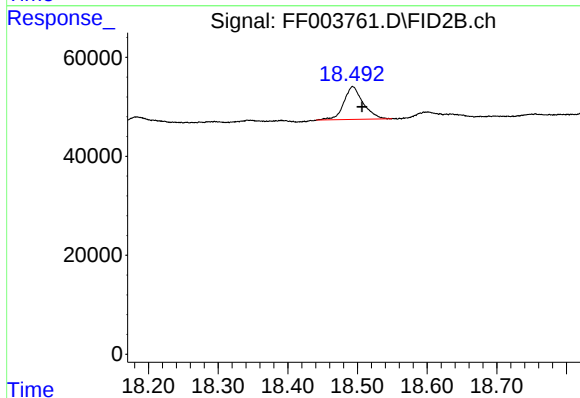

#14 N-DOTRIACONTANE

R.T.: 18.493 min
Delta R.T.: -0.013 min
Response: 126213
Conc: 0.89 ug/ml

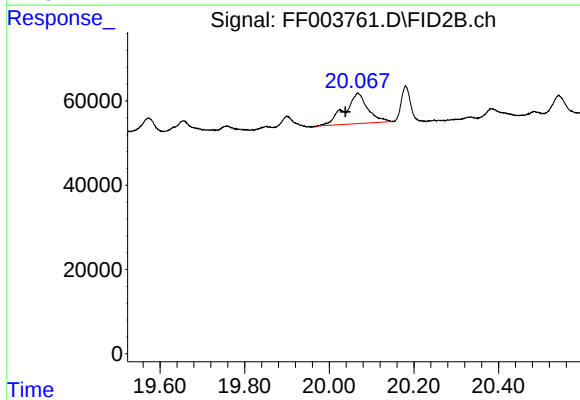

#16 N-HEXATRIACONTANE

R.T.: 20.068 min
Delta R.T.: 0.030 min
Response: 270750
Conc: 2.08 ug/ml