

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030819\
 Data File : FF003765.D
 Signal(s) : FID2B.ch
 Acq On : 08 Mar 2019 15:38
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Mar 08 21:47:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.587	2246747	16.137 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.658	107648	0.732 ug/ml
14) N-DOTRIACONTANE	18.495	167766	1.180 ug/ml
16) N-HEXATRIACONTANE	20.069	210457	1.613 ug/ml
18) N-TETRACONTANE	21.676	224994	1.809 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030819\
Data File : FF003765.D
Signal(s) : FID2B.ch
Acq On : 08 Mar 2019 15:38
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 08 21:47:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

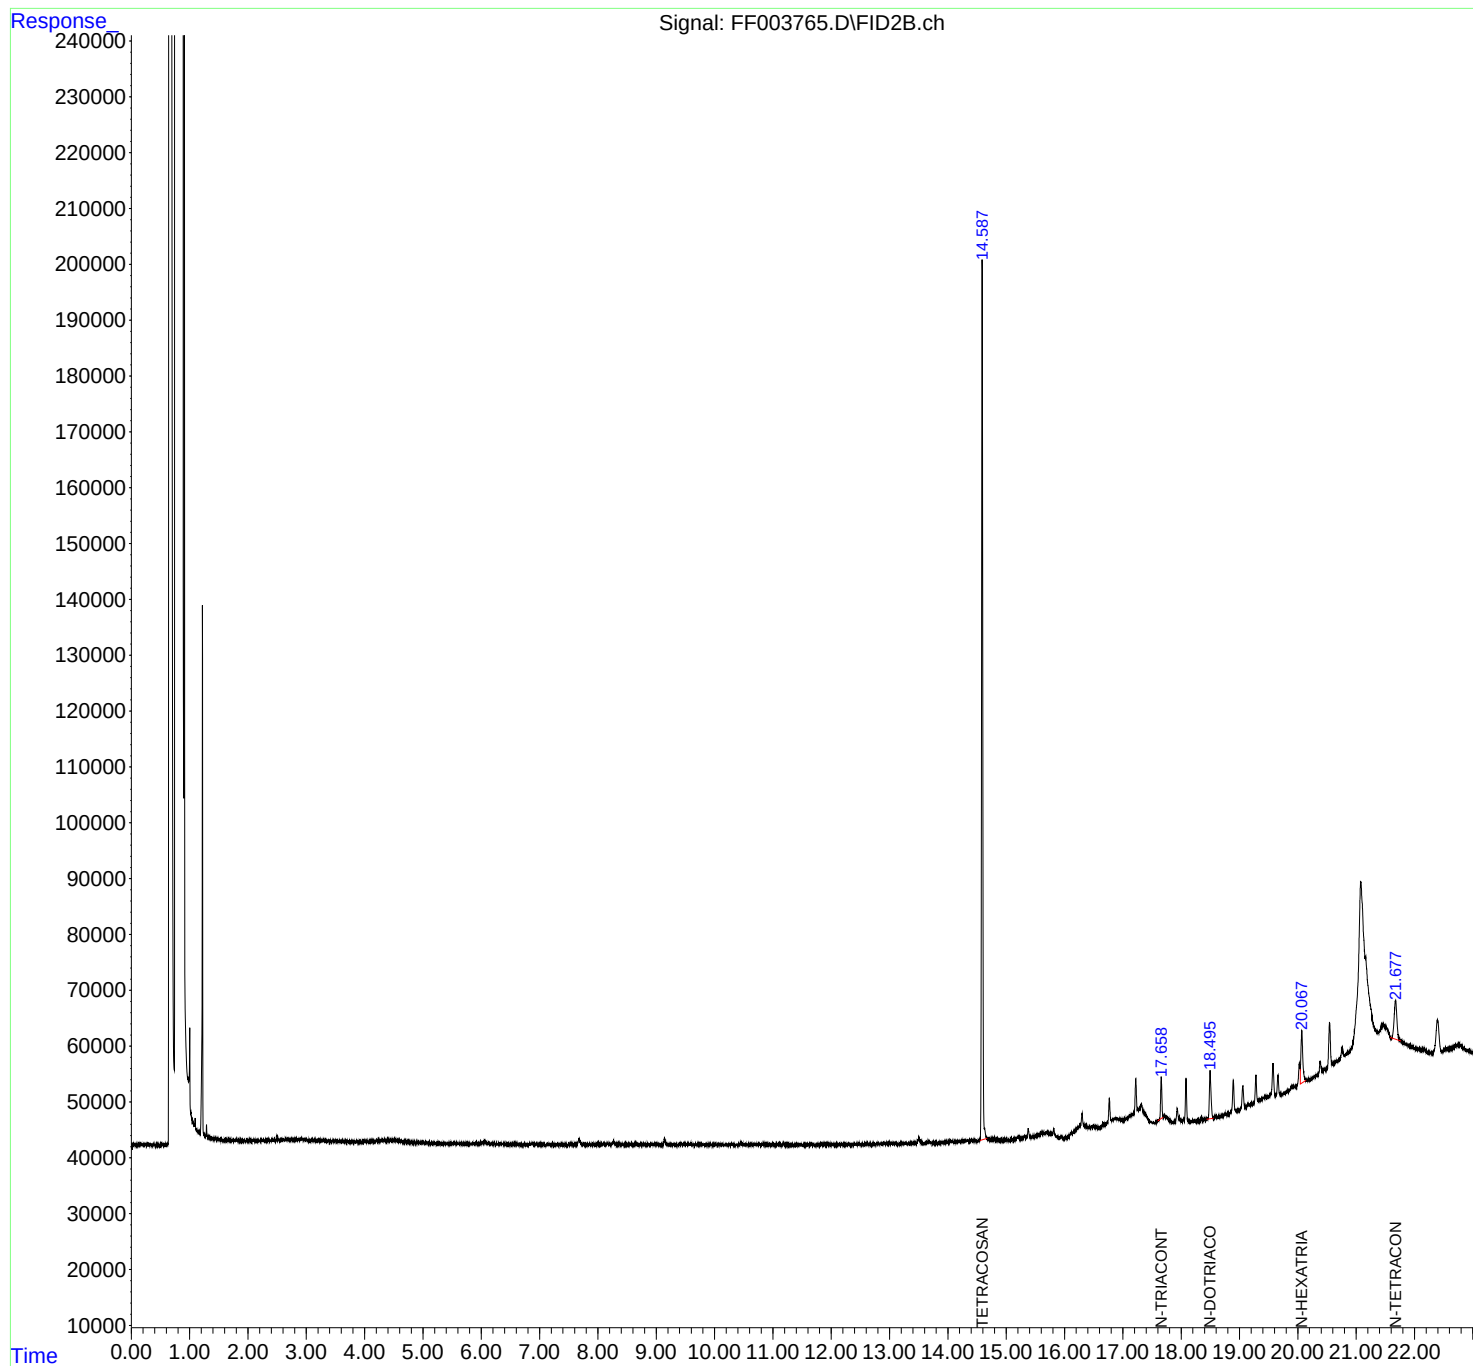


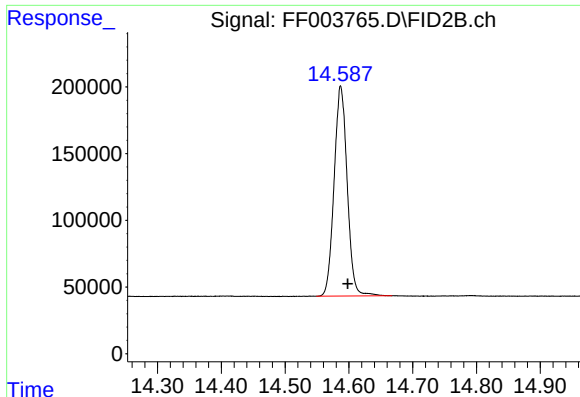

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.587 min
Delta R.T.: -0.011 min
Response: 2246747
Conc: 16.14 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

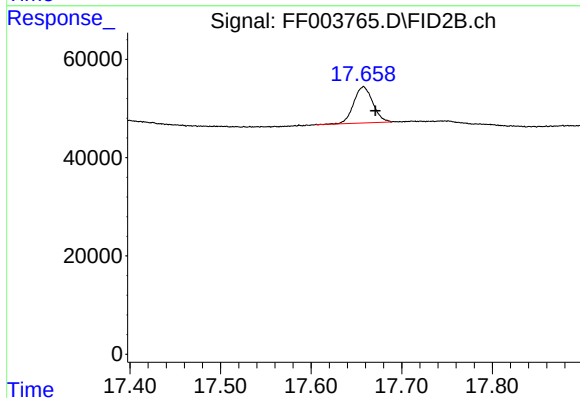


#13 N-TRIACONTANE

R.T.: 17.658 min
Delta R.T.: -0.013 min
Response: 107648
Conc: 0.73 ug/ml

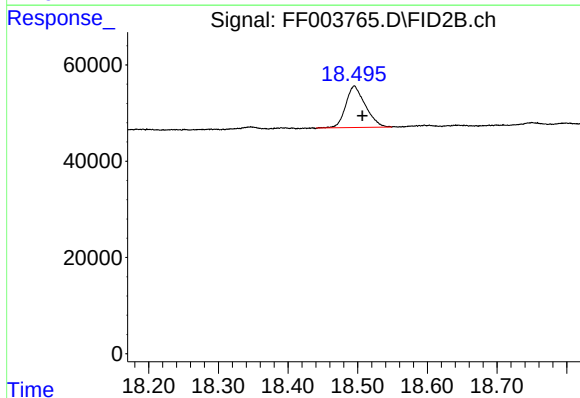


#14 N-DOTRIACONTANE

R.T.: 18.495 min
Delta R.T.: -0.012 min
Response: 167766
Conc: 1.18 ug/ml

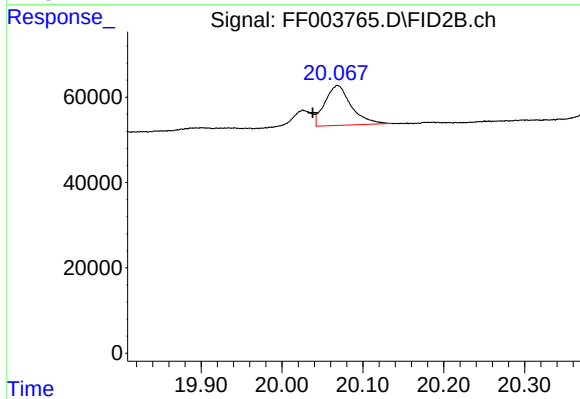

#16 N-HEXATRIACONTANE

R.T.: 20.069 min
Delta R.T.: 0.031 min
Response: 210457
Conc: 1.61 ug/ml

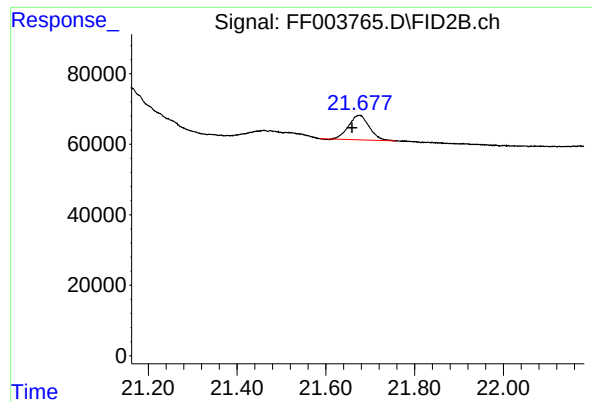

#18 N-TETRACONTANE

R.T.: 21.676 min
Delta R.T.: 0.018 min
Response: 224994
Conc: 1.81 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK