

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030921\
Data File : FF008201.D
Signal(s) : FID2B.ch
Acq On : 09 Mar 2021 15:35
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 10 07:54:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030421.M
Quant Title :
QLast Update : Fri Mar 05 09:17:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.666	2621066	18.560 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.732	118021	0.766 ug/ml
14) N-DOTRIACONTANE	18.564	151905	1.026 ug/ml
15) N-TETRATRIACONTANE	19.349	105702	0.761 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF030921\
Data File : FF008201.D
Signal(s) : FID2B.ch
Acq On : 09 Mar 2021 15:35
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 10 07:54:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030421.M
Quant Title :
QLast Update : Fri Mar 05 09:17:37 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

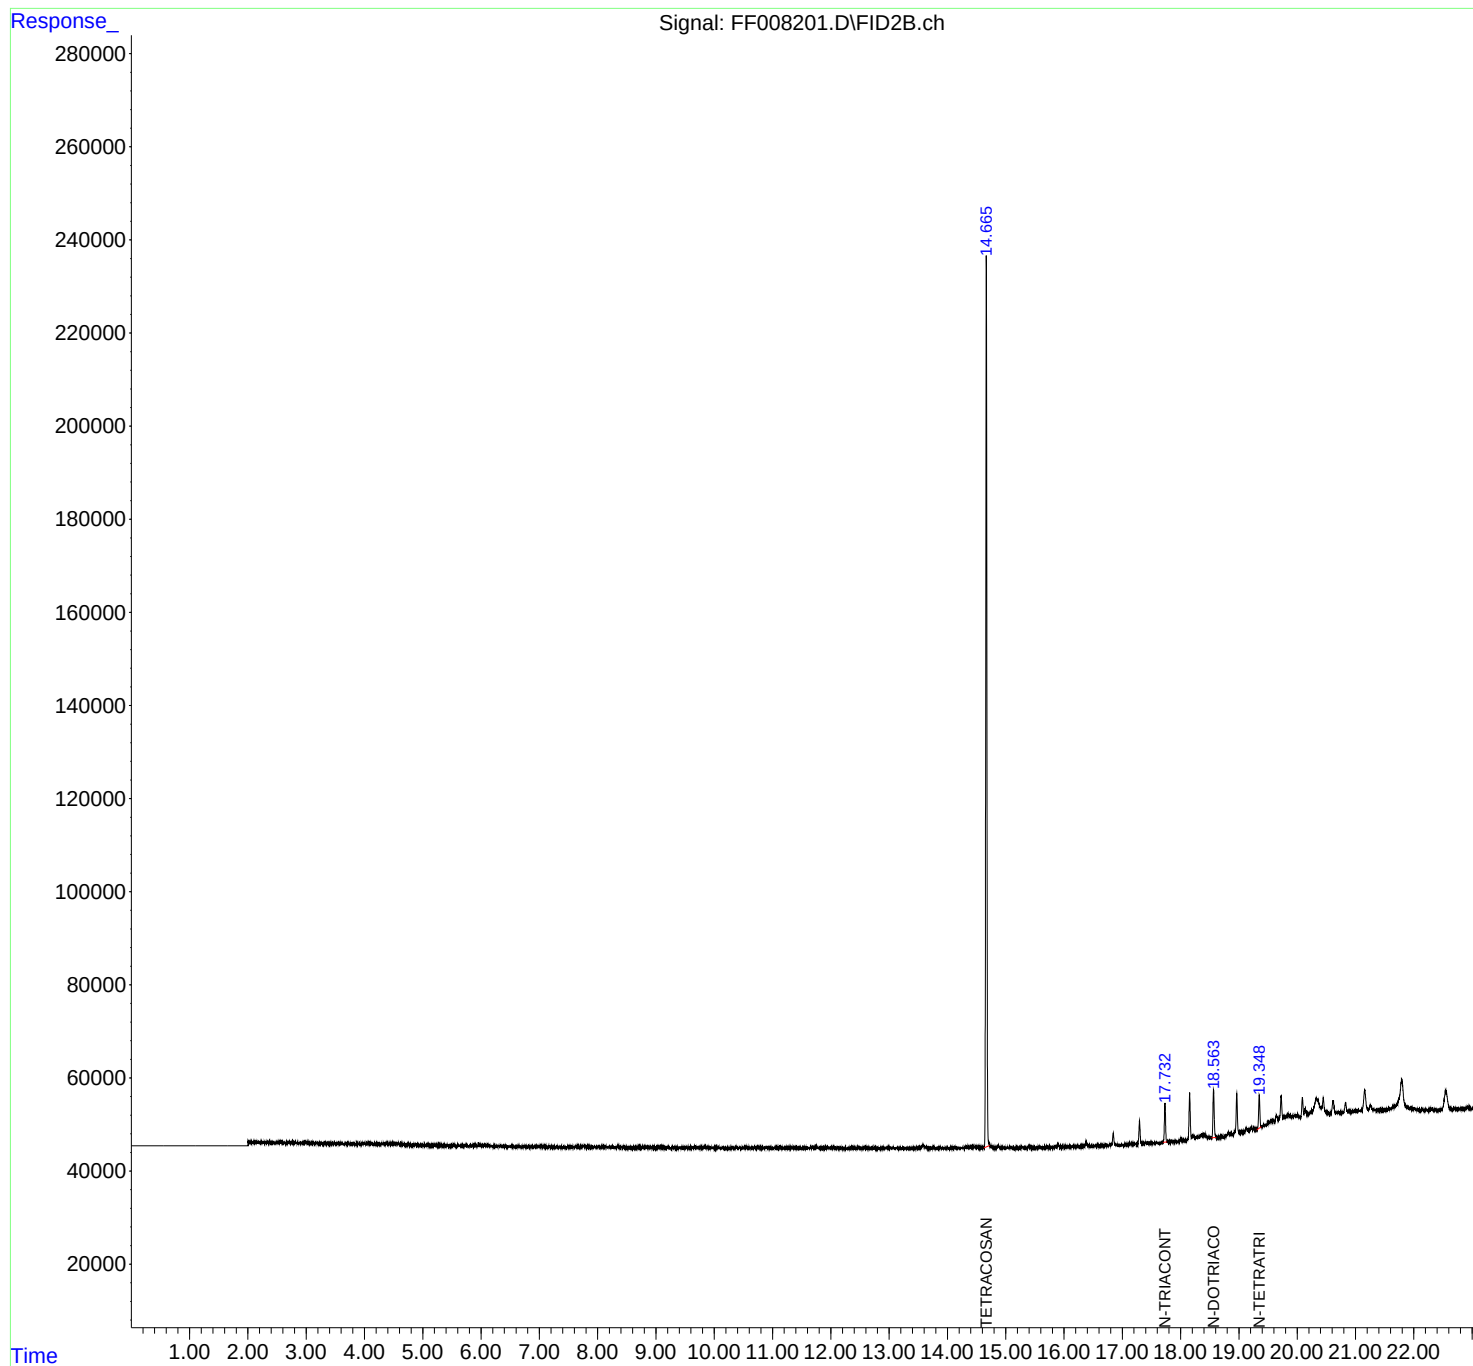


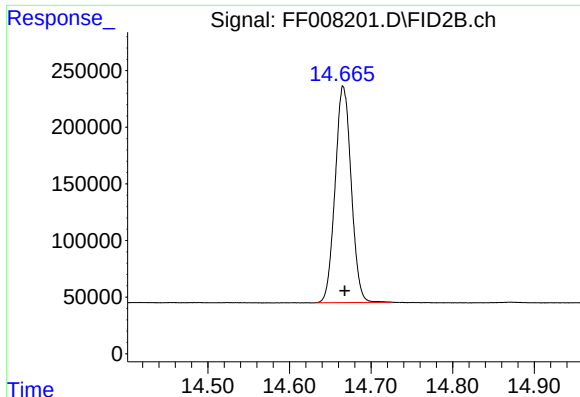

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.666 min
Delta R.T.: -0.002 min
Response: 2621066
Conc: 18.56 ug/ml

Instrument :
FID_F
ClientSampleId :

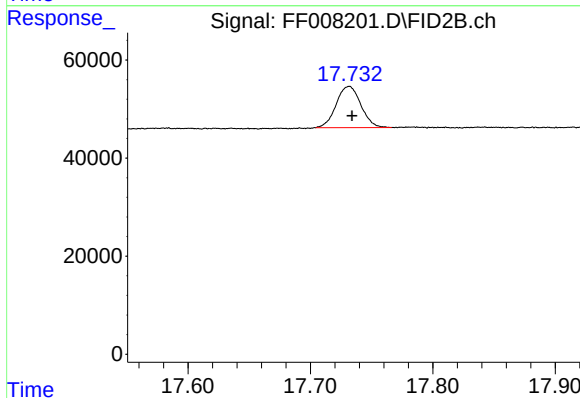


#13 N-TRIACONTANE

R.T.: 17.732 min
Delta R.T.: -0.002 min
Response: 118021
Conc: 0.77 ug/ml

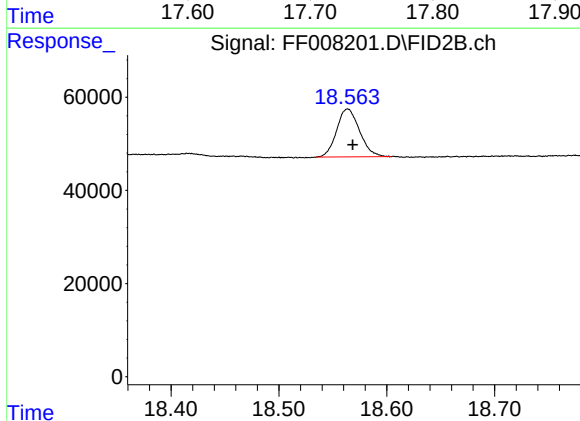

#14 N-DOTRIACONTANE

R.T.: 18.564 min
Delta R.T.: -0.005 min
Response: 151905
Conc: 1.03 ug/ml

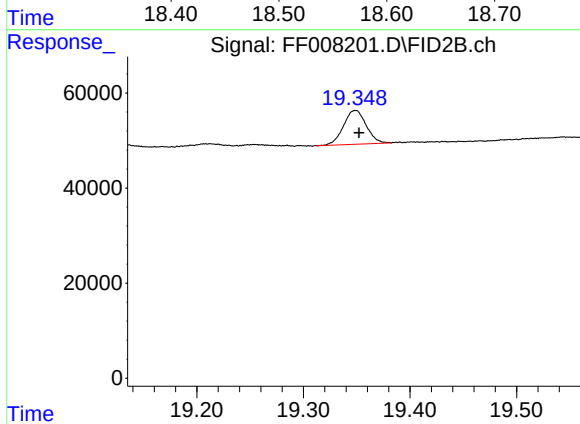

#15 N-TETRATRIACONTANE

R.T.: 19.349 min
Delta R.T.: -0.003 min
Response: 105702
Conc: 0.76 ug/ml