

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031119\
 Data File : FF003780.D
 Signal(s) : FID2B.ch
 Acq On : 11 Mar 2019 19:49
 Operator : AJ\SJ
 Sample : K1835-01
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 12 00:51:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.588	1931791	13.875 ug/ml
Target Compounds			
4) N-TETRADECANE	8.190f	591417	3.689 ug/ml
11) N-HEXACOSANE	15.815	89892	0.582 ug/ml
12) N-OCTACOSANE	16.768	131879	0.873 ug/ml
13) N-TRIACONTANE	17.660	193019	1.312 ug/ml
14) N-DOTRIACONTANE	18.508	367640	2.585 ug/ml
15) N-TETRATRIACONTANE	19.321	417157	3.116 ug/ml
16) N-HEXATRIACONTANE	20.071	736559	5.645 ug/ml
18) N-TETRACONTANE	21.681	552323	4.440 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031119\
Data File : FF003780.D
Signal(s) : FID2B.ch
Acq On : 11 Mar 2019 19:49
Operator : AJ\SJ
Sample : K1835-01
Misc :
ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 12 00:51:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

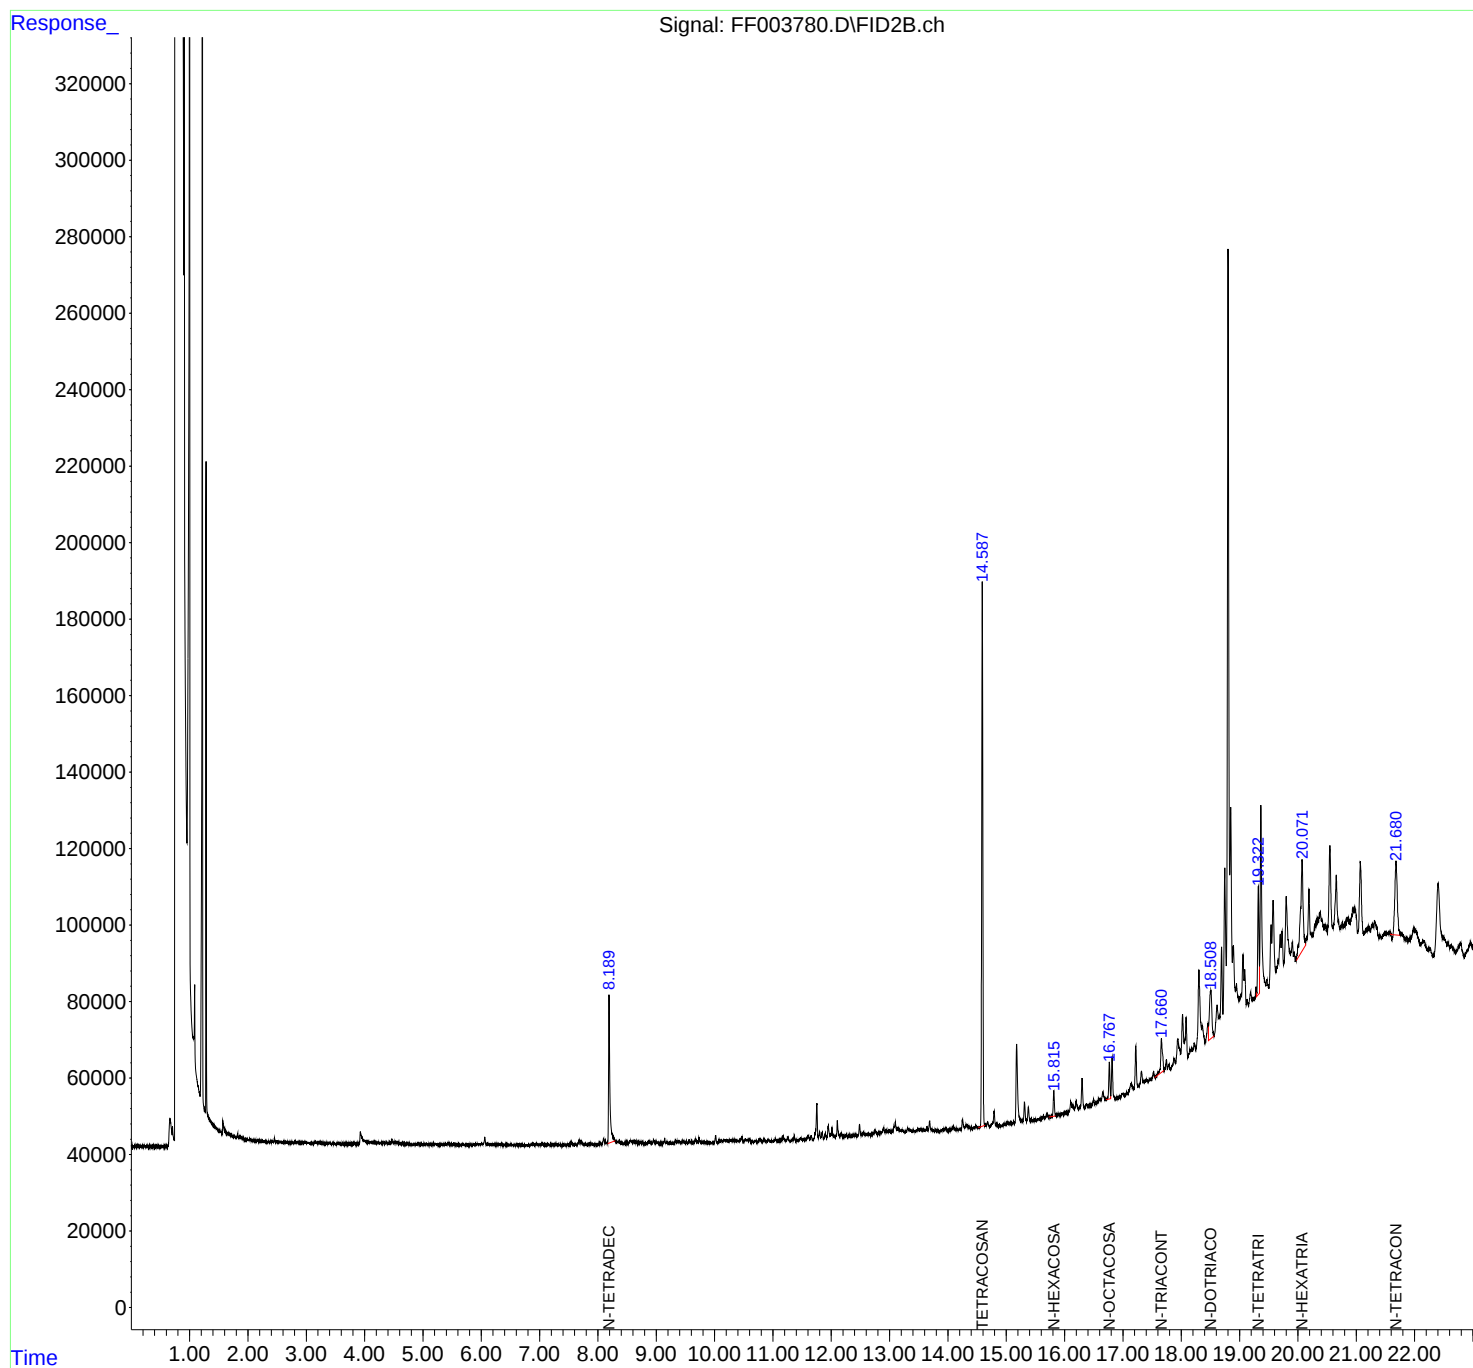

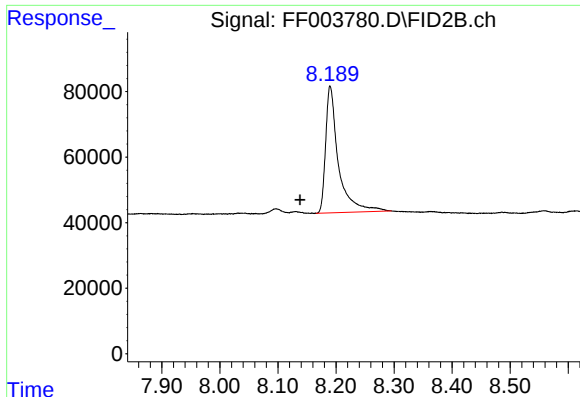


#4 N-TETRADECANE

R.T.: 8.190 min
Delta R.T.: 0.052 min
Response: 591417
Conc: 3.69 ug/ml

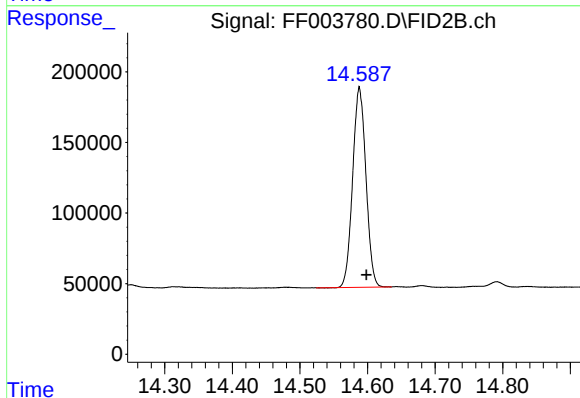


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.588 min
Delta R.T.: -0.010 min
Response: 1931791
Conc: 13.88 ug/ml

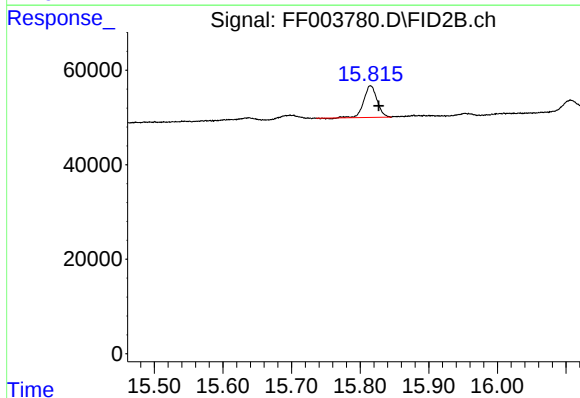


#11 N-HEXACOSANE

R.T.: 15.815 min
Delta R.T.: -0.012 min
Response: 89892
Conc: 0.58 ug/ml

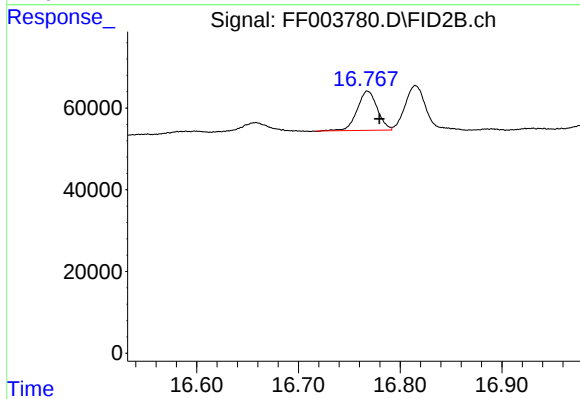


#12 N-OCTACOSANE

R.T.: 16.768 min
Delta R.T.: -0.012 min
Response: 131879
Conc: 0.87 ug/ml

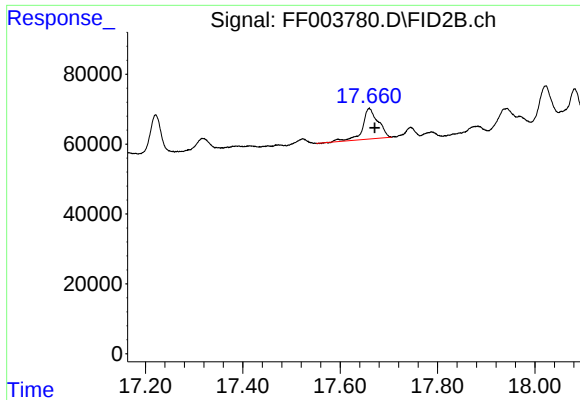


#13 N-TRIACONTANE

R.T.: 17.660 min
Delta R.T.: -0.011 min
Response: 193019
Conc: 1.31 ug/ml

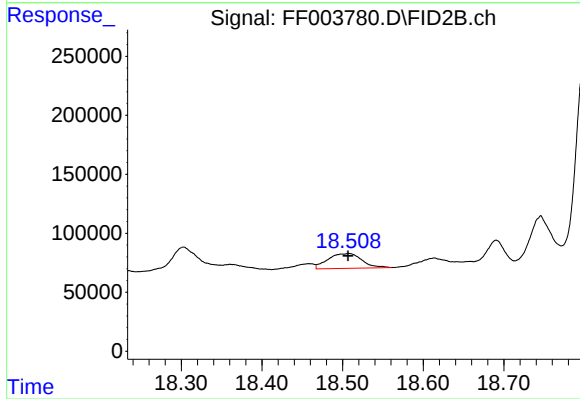


#14 N-DOTRIACONTANE

R.T.: 18.508 min
Delta R.T.: 0.001 min
Response: 367640
Conc: 2.59 ug/ml

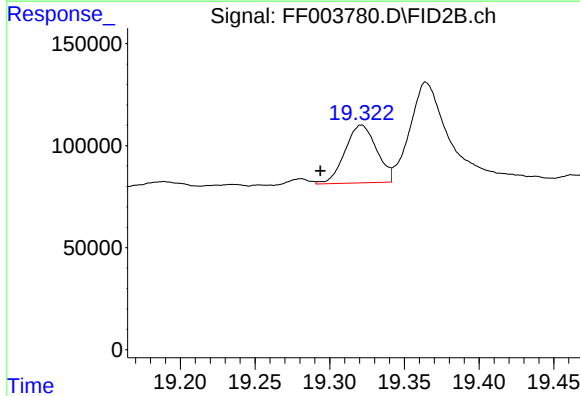


#15 N-TETRATRIACONTANE

R.T.: 19.321 min
Delta R.T.: 0.028 min
Response: 417157
Conc: 3.12 ug/ml

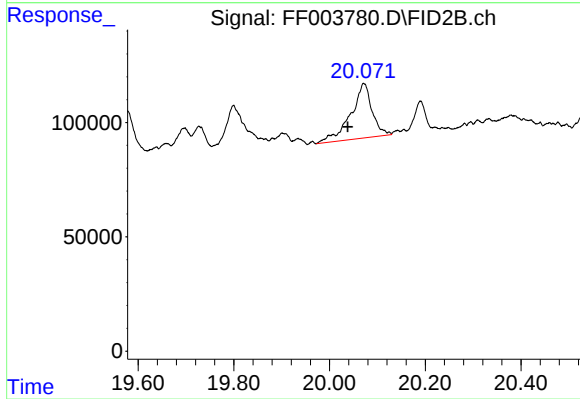

#16 N-HEXATRIACONTANE

R.T.: 20.071 min
Delta R.T.: 0.033 min
Response: 736559
Conc: 5.64 ug/ml

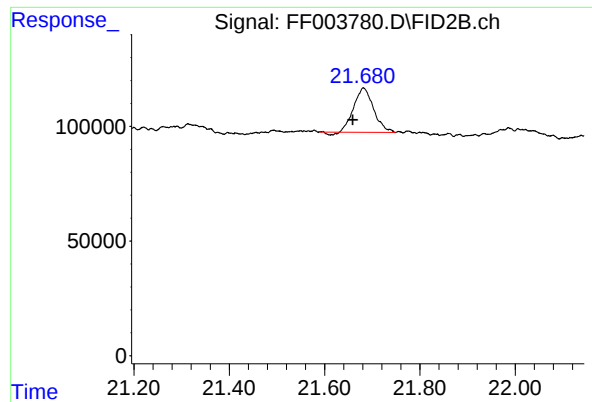

#18 N-TETRACONTANE

R.T.: 21.681 min
Delta R.T.: 0.023 min
Response: 552323
Conc: 4.44 ug/ml