

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
Data File : FF003788.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2019 10:31
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 13 00:58:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.335	2709174	17.359 ug/ml
12)	N-OCTACOSANE	16.769	2531509	16.752 ug/ml
13)	N-TRIACONTANE	17.658	141507	0.962 ug/ml
14)	N-DOTRIACONTANE	18.493	166956	1.174 ug/ml
15)	N-TETRATRIACONTANE	19.280	104313	0.779 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
Data File : FF003788.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2019 10:31
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 13 00:58:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

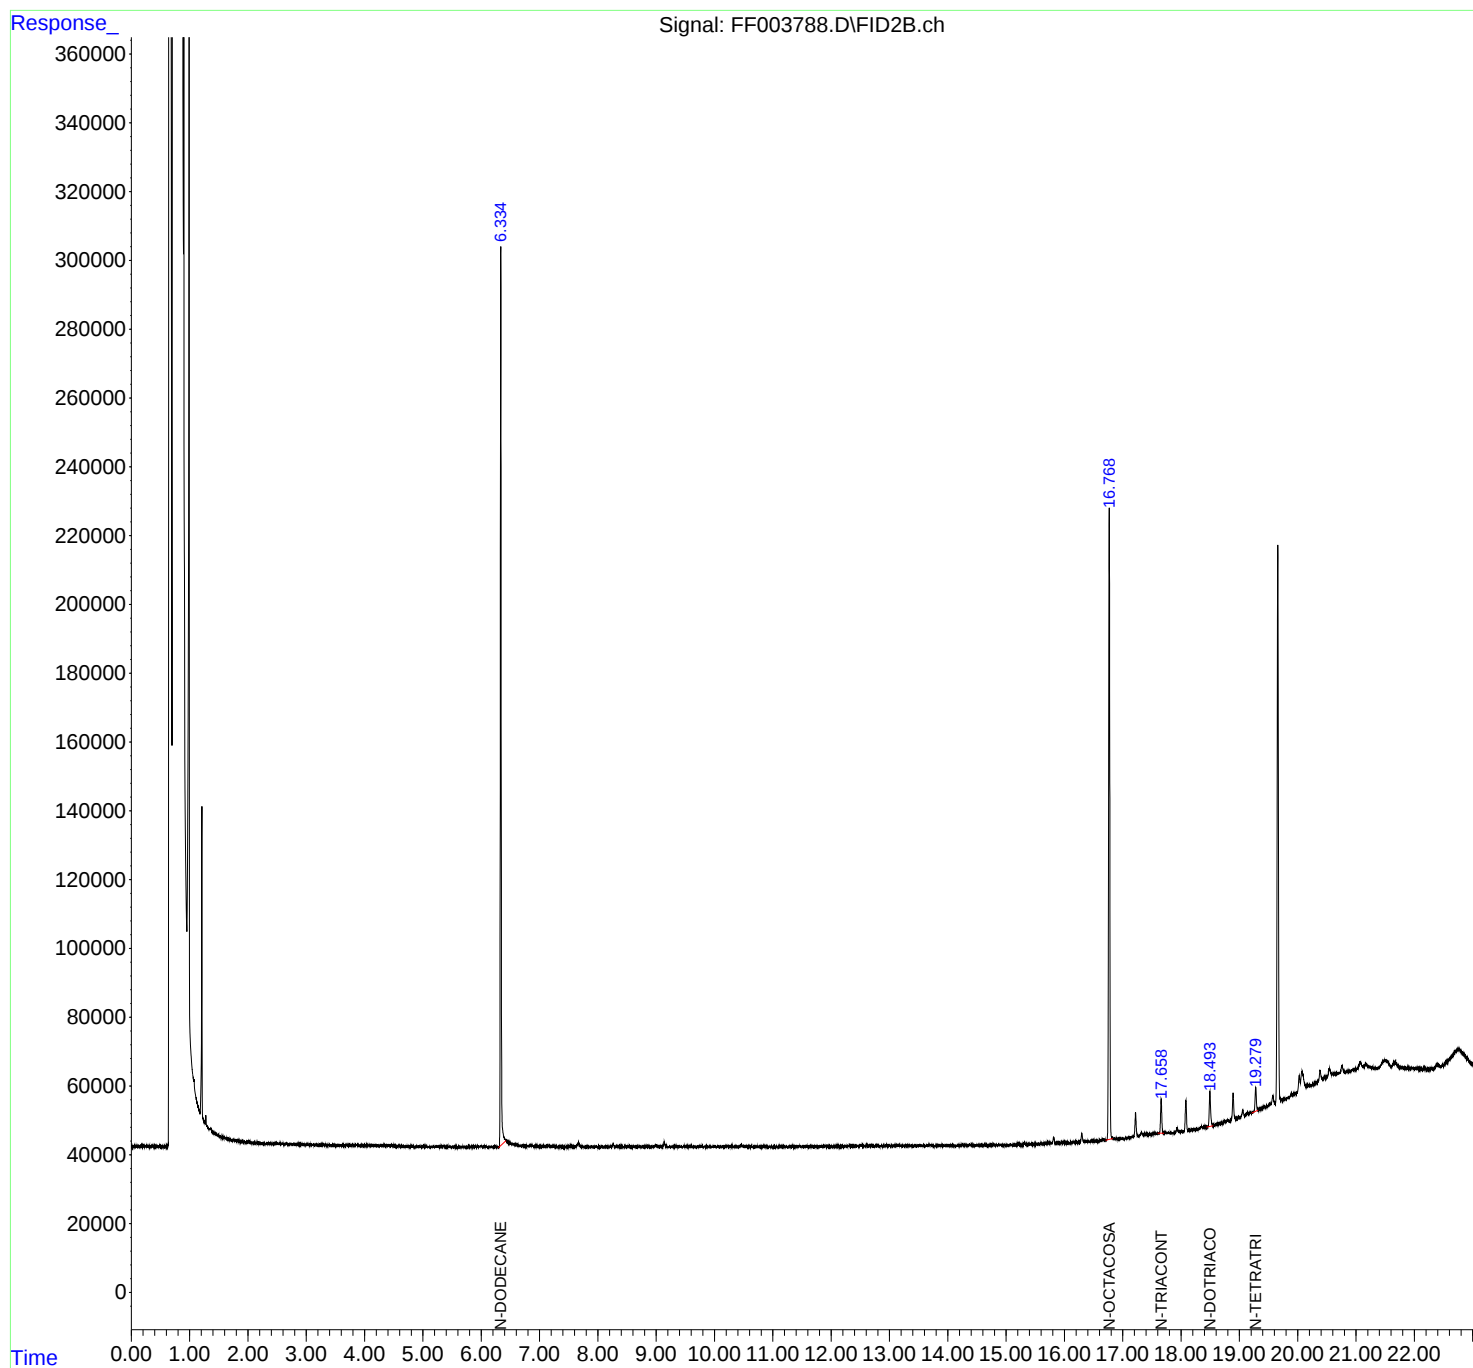


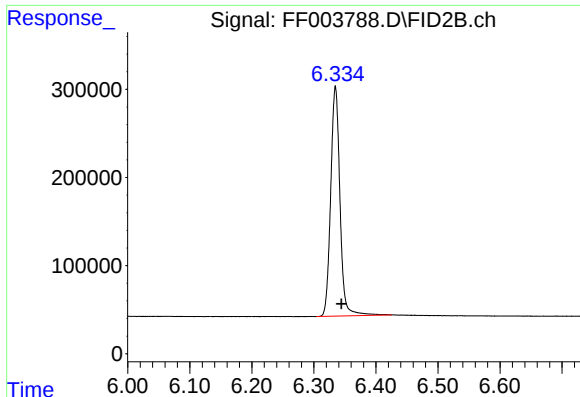

#3 N-DODECANE


R.T.: 6.335 min
Delta R.T.: -0.009 min
Response: 2709174
Conc: 17.36 ug/ml

Instrument :
FID_F
ClientSampleId :

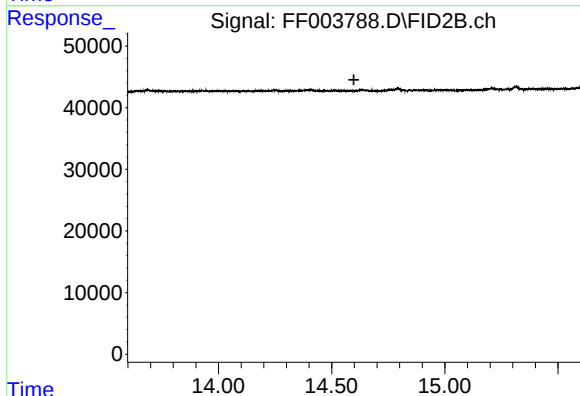


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.598 min
Response: 0
Conc: N.D.

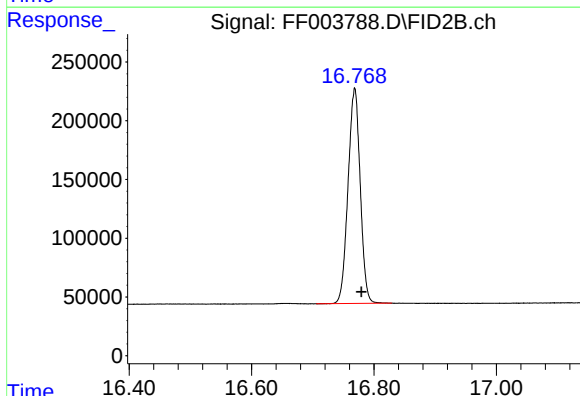


#12 N-OCTACOSANE

R.T.: 16.769 min
Delta R.T.: -0.011 min
Response: 2531509
Conc: 16.75 ug/ml

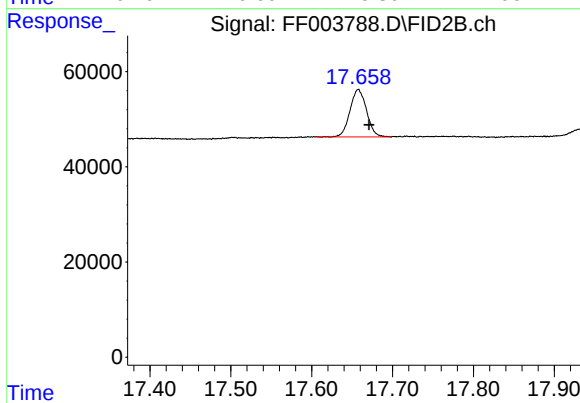

#13 N-TRIACONTANE


R.T.: 17.658 min
Delta R.T.: -0.013 min
Response: 141507
Conc: 0.96 ug/ml

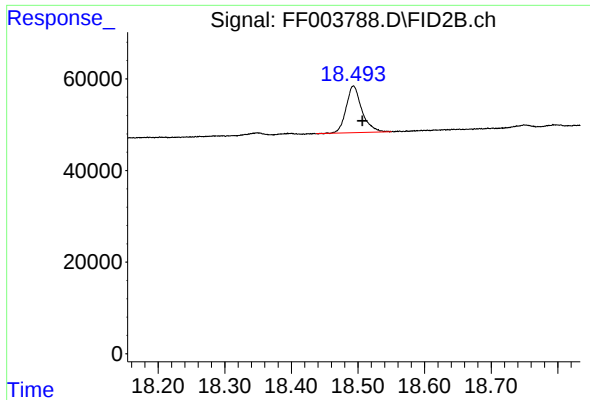

#14 N-DOTRIACONTANE

R.T.: 18.493 min
Delta R.T.: -0.014 min
Response: 166956
Conc: 1.17 ug/ml

Instrument :
FID_F
ClientSampleId :

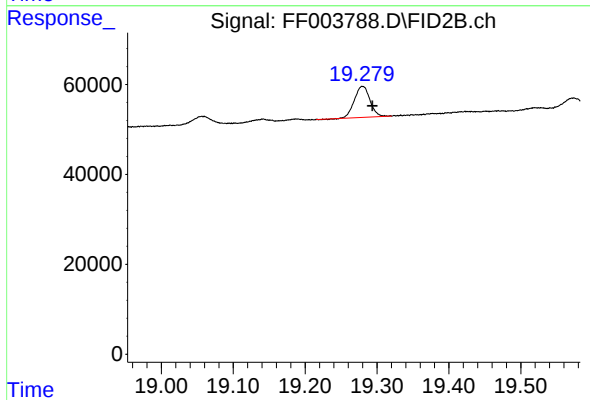

#15 N-TETRATRIACONTANE

R.T.: 19.280 min
Delta R.T.: -0.014 min
Response: 104313
Conc: 0.78 ug/ml