

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
 Data File : FF003789.D
 Signal(s) : FID2B.ch
 Acq On : 12 Mar 2019 11:03
 Operator : AJ\SJ
 Sample : K1691-01
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 13 00:58:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.590	2669671	19.175 ug/ml
Target Compounds			
4) N-TETRADECANE	8.187	347974	2.170 ug/ml
5) N-HEXADECANE	9.736	211693	1.300 ug/ml
6) N-OCTADECANE	11.253f	208704	1.267 ug/ml
7) N-EICOSANE	12.486	200814	1.228 ug/ml
8) N-DOCOSANE	13.705	349335	2.165 ug/ml
10) N-TETRACOSANE	14.766	2994279	18.925 ug/ml
11) N-HEXACOSANE	15.818	680069	4.406 ug/ml
12) N-OCTACOSANE	16.777	2049847	13.565 ug/ml
13) N-TRIACONTANE	17.663	2097791	14.261 ug/ml
14) N-DOTRIACONTANE	18.498	1798593	12.647 ug/ml
15) N-TETRATRIACONTANE	19.310	1918785	14.330 ug/ml
16) N-HEXATRIACONTANE	20.030	1321967	10.131 ug/ml
17) N-OCTATRIACONTANE	20.764	930207	8.056 ug/ml
18) N-TETRACONTANE	21.650	679827	5.465 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
Data File : FF003789.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2019 11:03
Operator : AJ\SJ
Sample : K1691-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 13 00:58:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

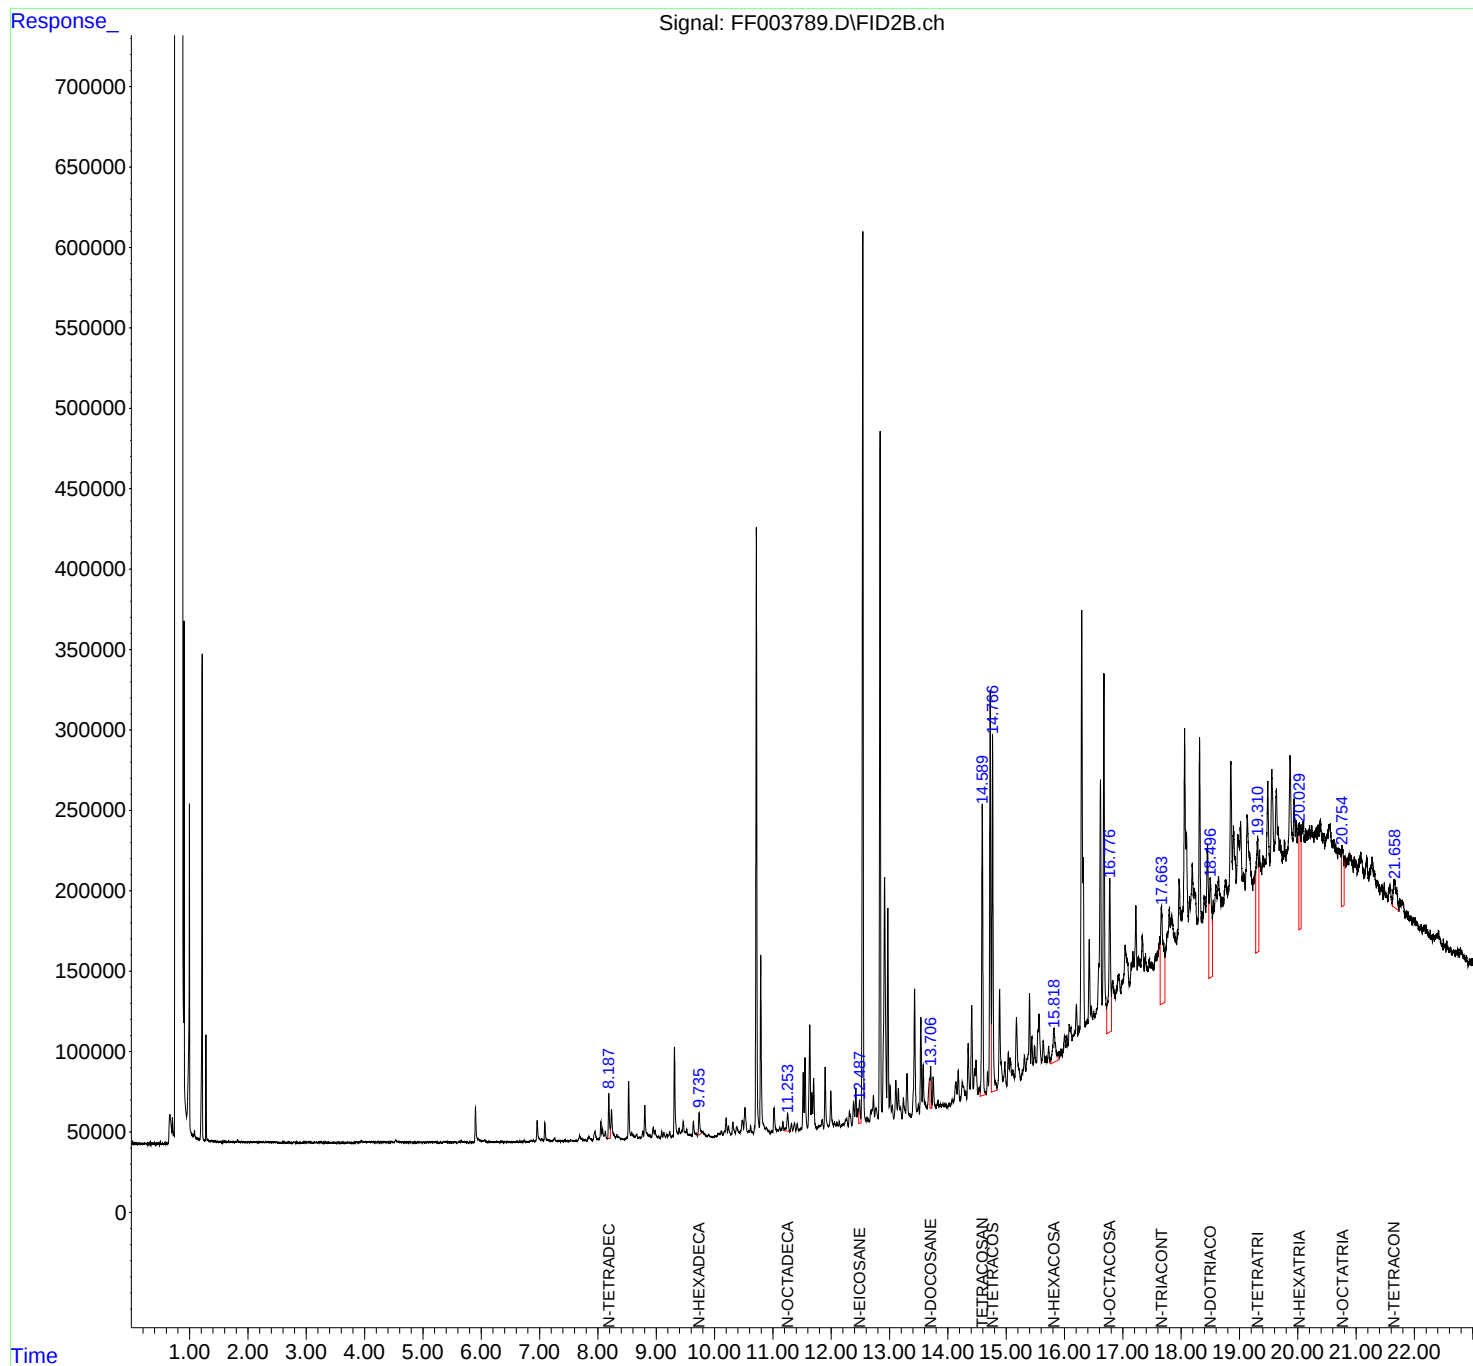


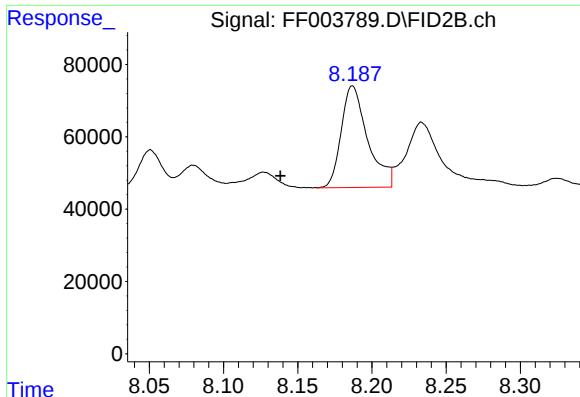

#4 N-TETRADECANE


R.T.: 8.187 min
Delta R.T.: 0.049 min
Response: 347974
Conc: 2.17 ug/ml

Instrument :
FID_F
ClientSampleId :

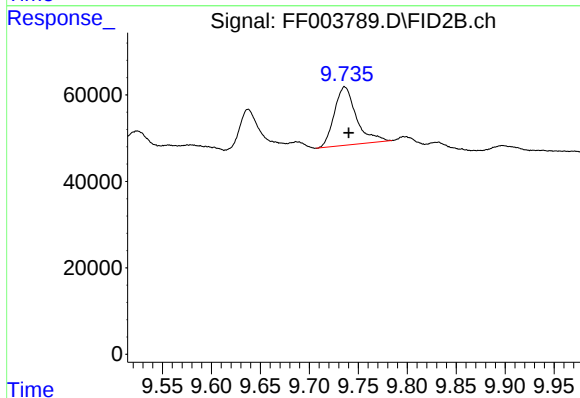


#5 N-HEXADECANE

R.T.: 9.736 min
Delta R.T.: -0.004 min
Response: 211693
Conc: 1.30 ug/ml

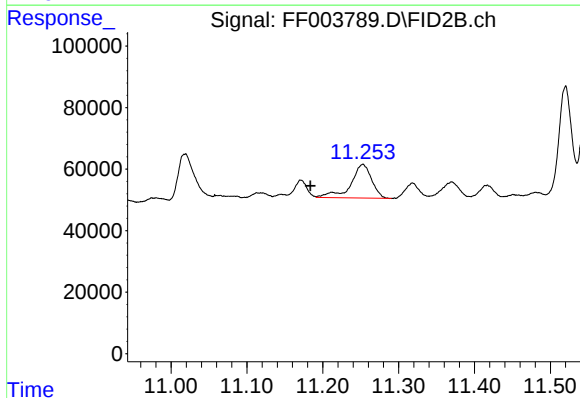


#6 N-OCTADECANE

R.T.: 11.253 min
Delta R.T.: 0.069 min
Response: 208704
Conc: 1.27 ug/ml

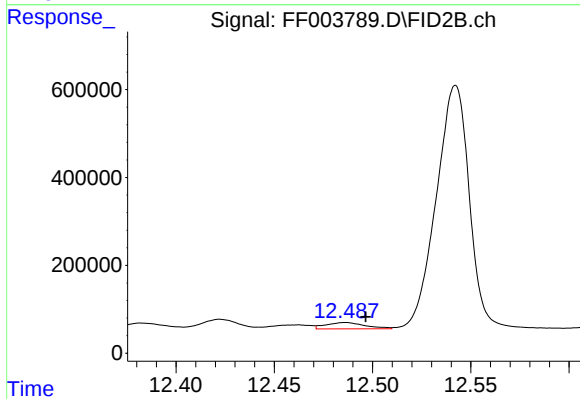

#7 N-EICOSANE


R.T.: 12.486 min
Delta R.T.: -0.010 min
Response: 200814
Conc: 1.23 ug/ml

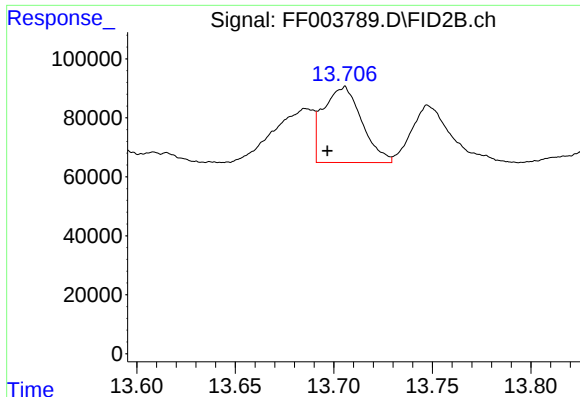

#8 N-DOCOSANE


R.T.: 13.705 min
Delta R.T.: 0.008 min
Response: 349335
Conc: 2.16 ug/ml

Instrument :
FID_F
ClientSampleId :

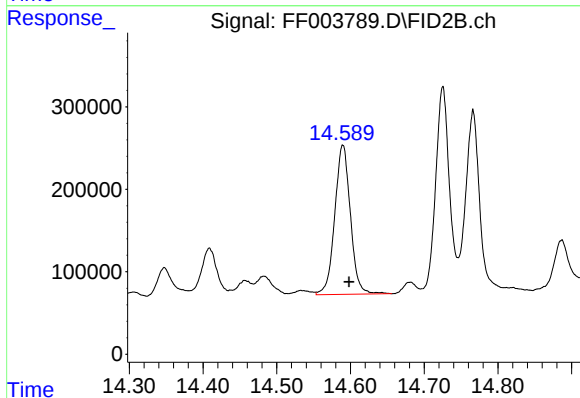


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.590 min
Delta R.T.: -0.008 min
Response: 2669671
Conc: 19.17 ug/ml

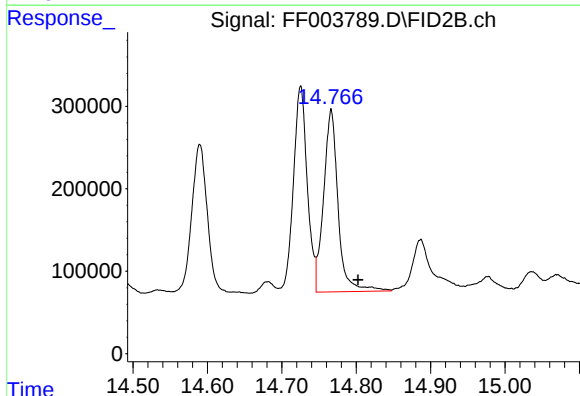


#10 N-TETRACOSANE

R.T.: 14.766 min
Delta R.T.: -0.036 min
Response: 2994279
Conc: 18.92 ug/ml

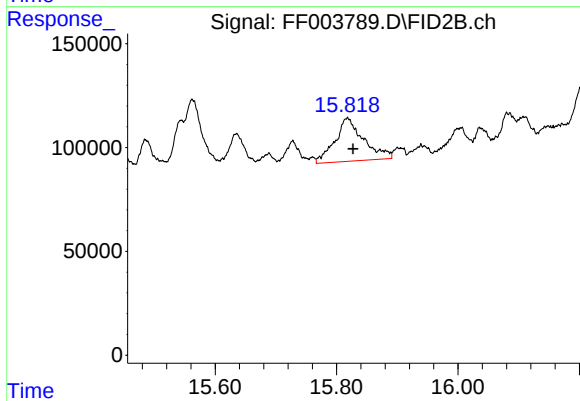

#11 N-HEXACOSANE


R.T.: 15.818 min
Delta R.T.: -0.009 min
Response: 680069
Conc: 4.41 ug/ml

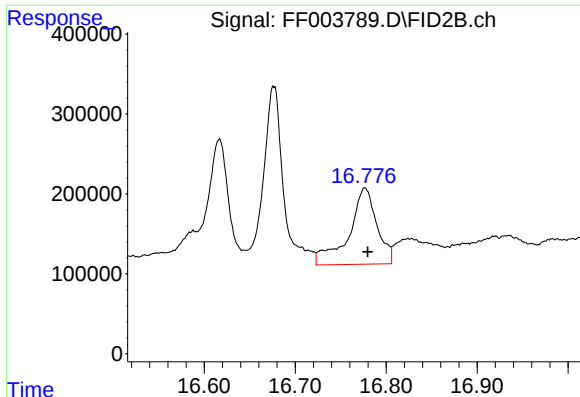

#12 N-OCTACOSANE


R.T.: 16.777 min
Delta R.T.: -0.003 min
Response: 2049847
Conc: 13.56 ug/ml

Instrument :
FID_F
ClientSampleId :

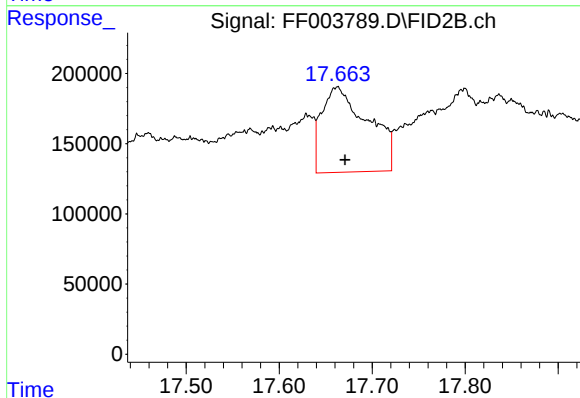


#13 N-TRIACONTANE

R.T.: 17.663 min
Delta R.T.: -0.008 min
Response: 2097791
Conc: 14.26 ug/ml

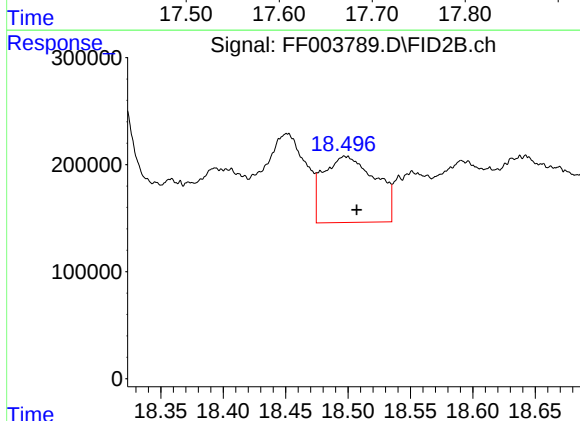


#14 N-DOTRIACONTANE

R.T.: 18.498 min
Delta R.T.: -0.009 min
Response: 1798593
Conc: 12.65 ug/ml

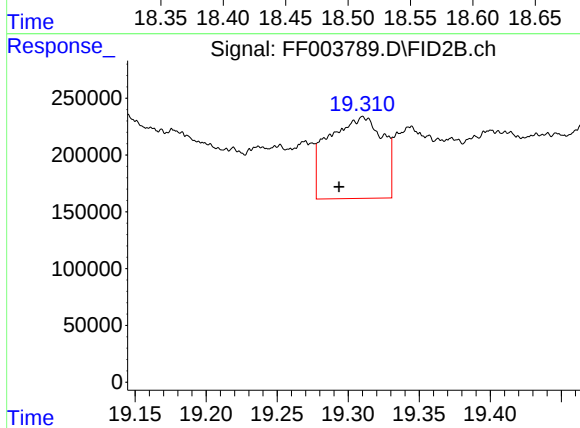

#15 N-TETRATRIACONTANE


R.T.: 19.310 min
Delta R.T.: 0.017 min
Response: 1918785
Conc: 14.33 ug/ml

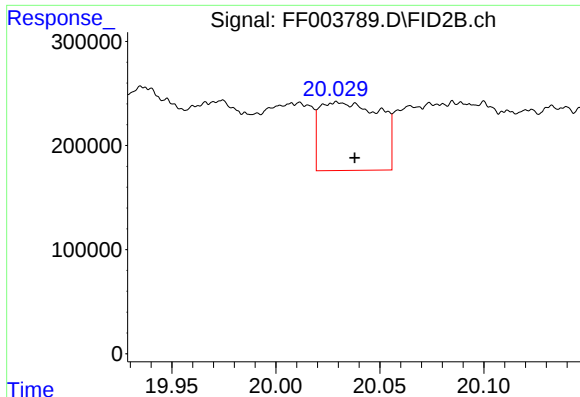

#16 N-HEXATRIACONTANE


R.T.: 20.030 min
Delta R.T.: -0.008 min
Response: 1321967
Conc: 10.13 ug/ml

Instrument :
FID_F
ClientSampleId :

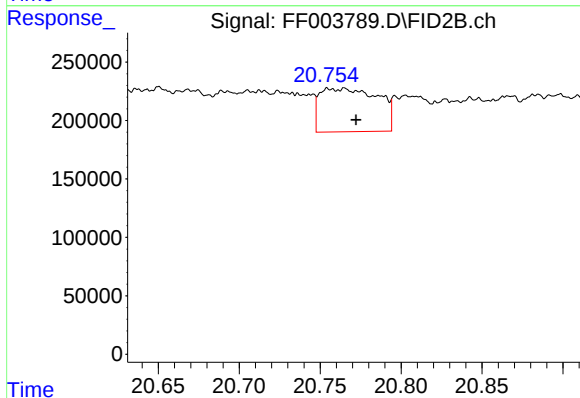

#17 N-OCTATRIACONTANE

R.T.: 20.764 min
Delta R.T.: -0.008 min
Response: 930207
Conc: 8.06 ug/ml

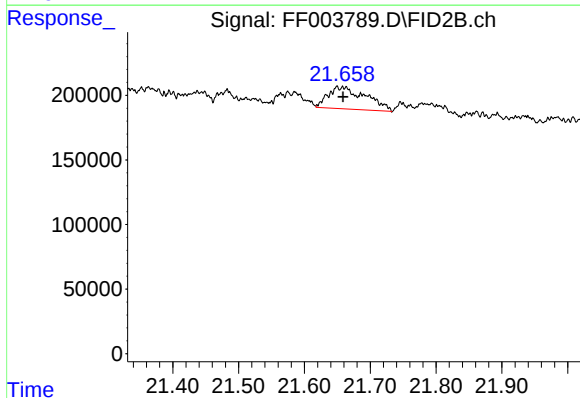

#18 N-TETRACONTANE

R.T.: 21.650 min
Delta R.T.: -0.008 min
Response: 679827
Conc: 5.46 ug/ml