

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
 Data File : FF003791.D
 Signal(s) : FID2B.ch
 Acq On : 12 Mar 2019 12:04
 Operator : AJ\SJ
 Sample : K1692-01 20X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 13 00:58:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.595	225820	1.622 ug/ml
Target Compounds			
7) N-EICOSANE	12.489	139447	0.852 ug/ml
8) N-DOCOSANE	13.710	341289	2.115 ug/ml
10) N-TETRACOSANE	14.767	1180409	7.461 ug/ml
12) N-OCTACOSANE	16.779	417508	2.763 ug/ml
13) N-TRIACONTANE	17.664	530944	3.609 ug/ml
14) N-DOTRIACONTANE	18.499	438852	3.086 ug/ml
15) N-TETRATRIACONTANE	19.291	446302	3.333 ug/ml
16) N-HEXATRIACONTANE	20.029	597247	4.577 ug/ml
17) N-OCTATRIACONTANE	20.757	544765	4.718 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
Data File : FF003791.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2019 12:04
Operator : AJ\SJ
Sample : K1692-01 20X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 13 00:58:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

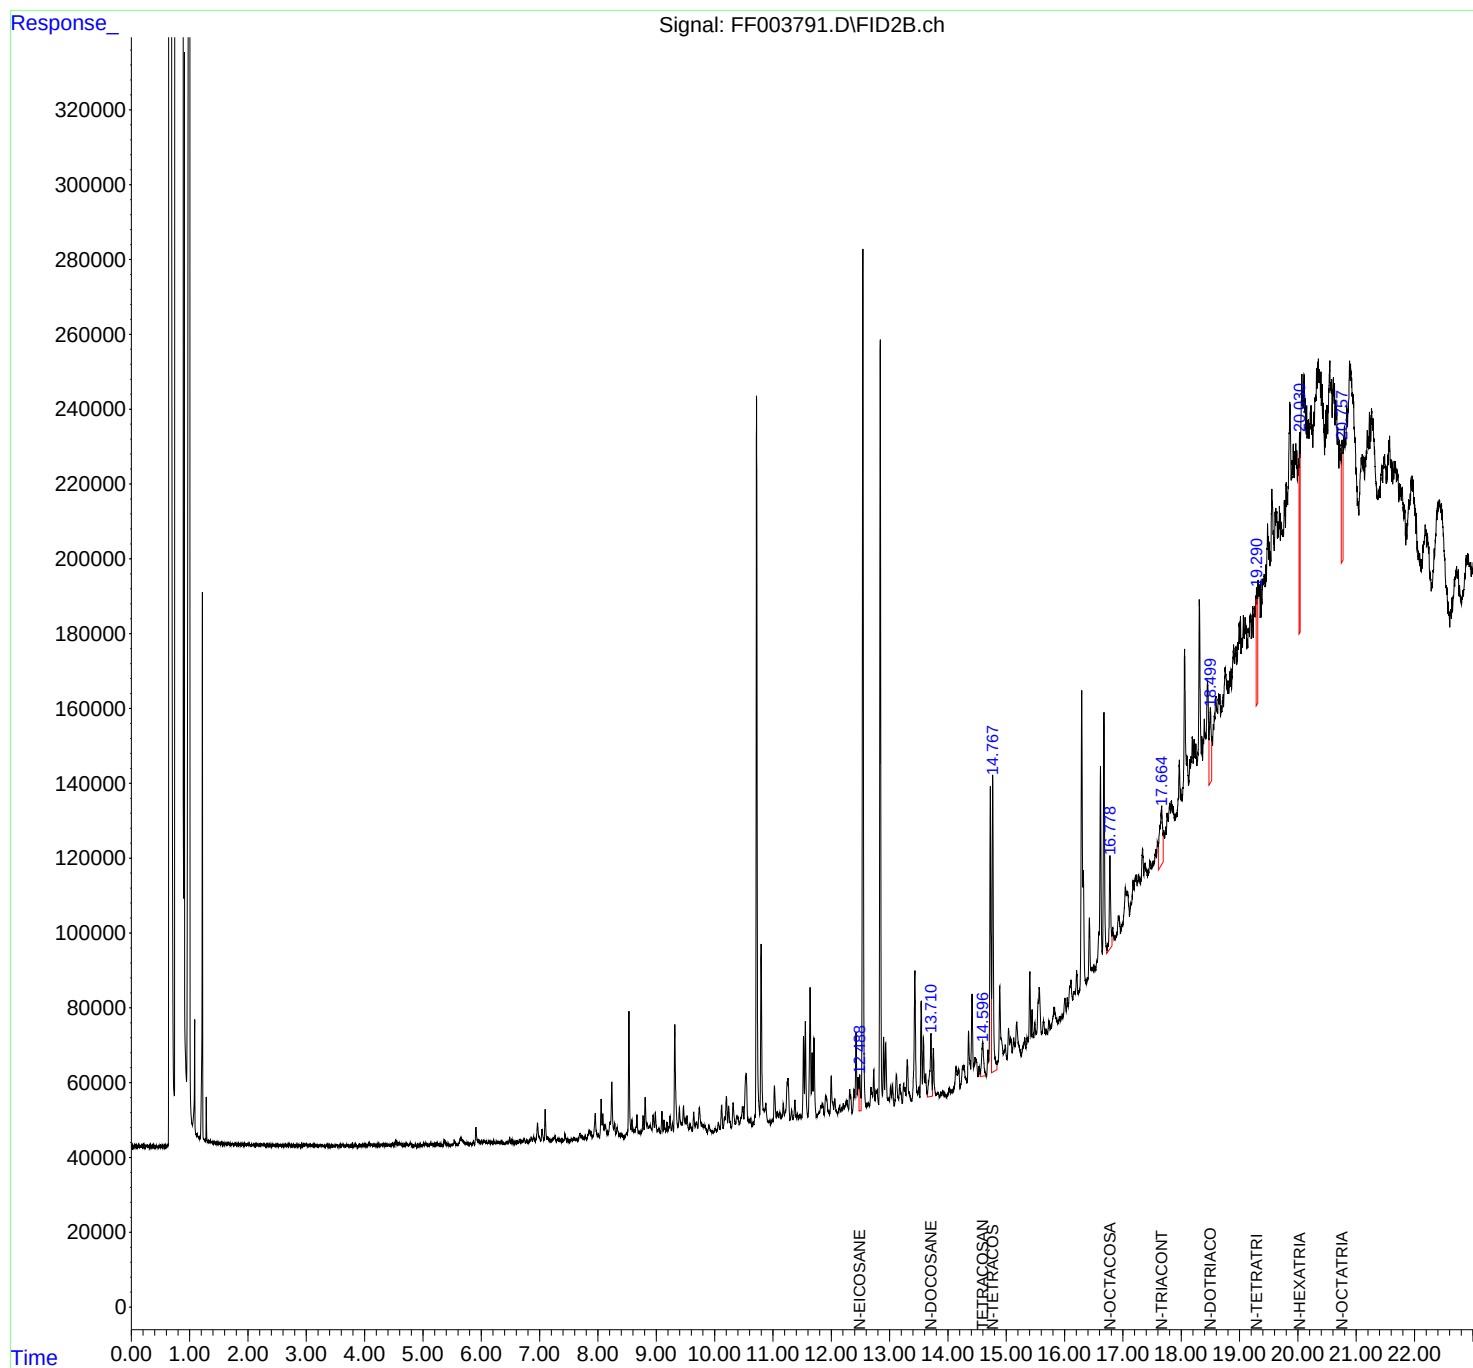


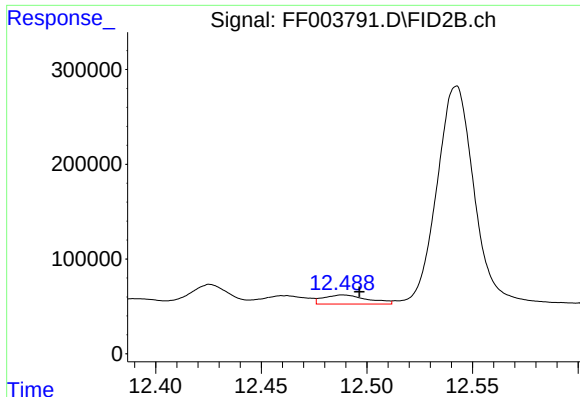

#7 N-EICOSANE


R.T.: 12.489 min
Delta R.T.: -0.008 min
Response: 139447
Conc: 0.85 ug/ml

Instrument :
FID_F
ClientSampleId :

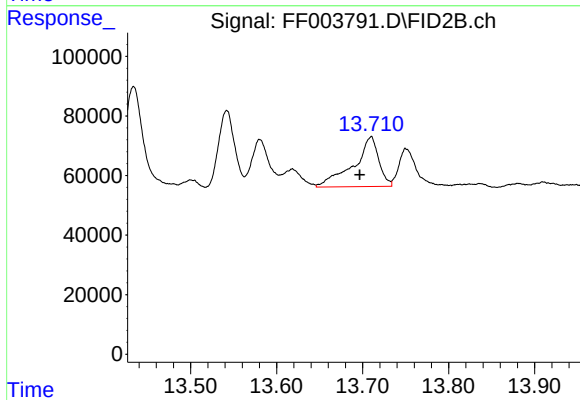


#8 N-DOCOSANE

R.T.: 13.710 min
Delta R.T.: 0.013 min
Response: 341289
Conc: 2.11 ug/ml

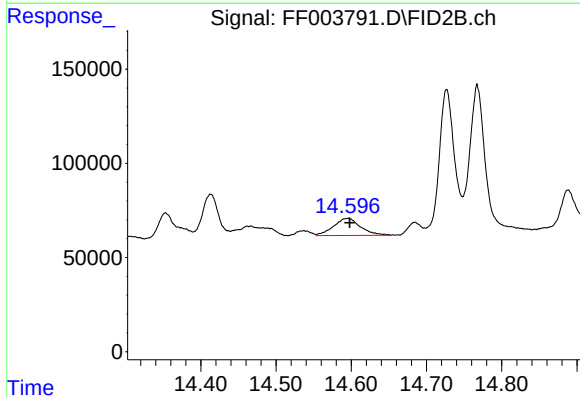


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.595 min
Delta R.T.: -0.003 min
Response: 225820
Conc: 1.62 ug/ml

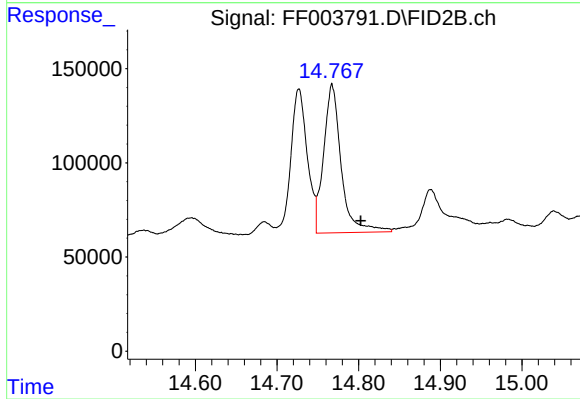

#10 N-TETRACOSANE


R.T.: 14.767 min
Delta R.T.: -0.035 min
Response: 1180409
Conc: 7.46 ug/ml

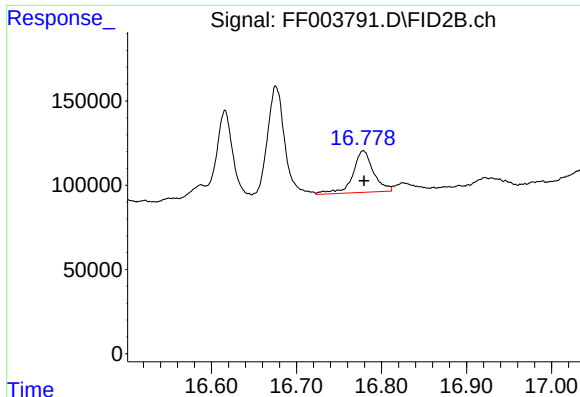

#12 N-OCTACOSANE


R.T.: 16.779 min
Delta R.T.: -0.001 min
Response: 417508
Conc: 2.76 ug/ml

Instrument :
FID_F
ClientSampleId :

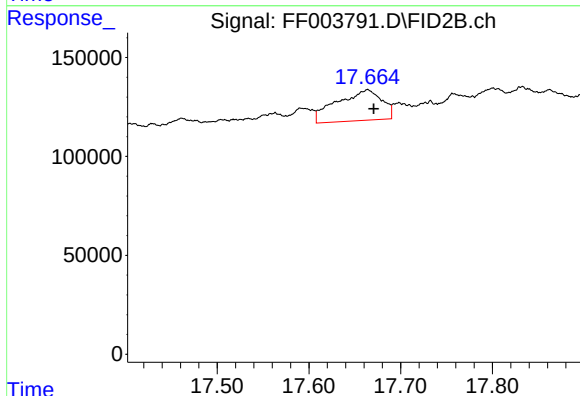


#13 N-TRIACONTANE

R.T.: 17.664 min
Delta R.T.: -0.007 min
Response: 530944
Conc: 3.61 ug/ml

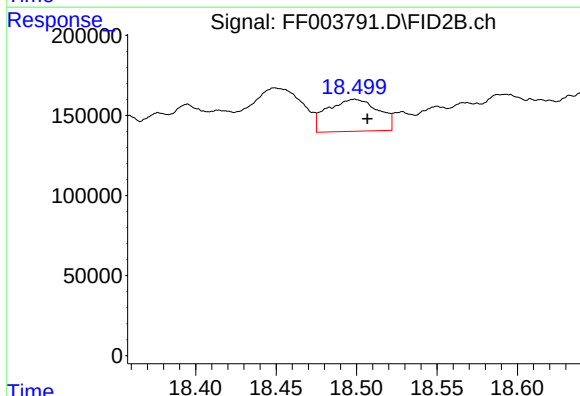


#14 N-DOTRIACONTANE

R.T.: 18.499 min
Delta R.T.: -0.008 min
Response: 438852
Conc: 3.09 ug/ml

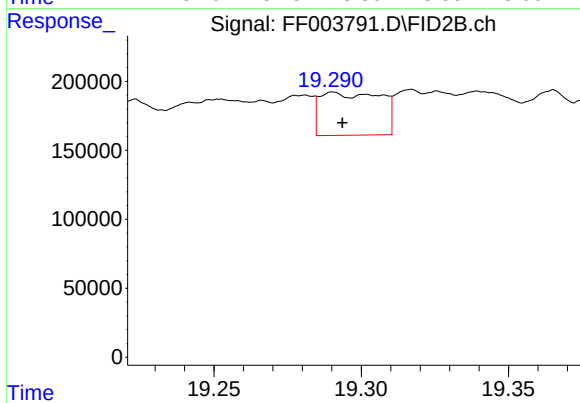

#15 N-TETRATRIACONTANE


R.T.: 19.291 min
Delta R.T.: -0.003 min
Response: 446302
Conc: 3.33 ug/ml

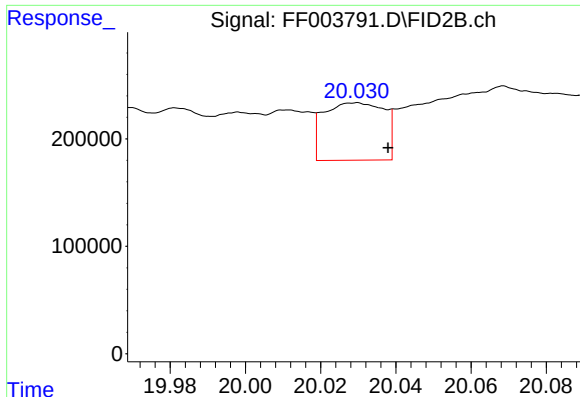

#16 N-HEXATRIACONTANE

R.T.: 20.029 min
Delta R.T.: -0.009 min
Response: 597247
Conc: 4.58 ug/ml

Instrument :
FID_F
ClientSampleId :

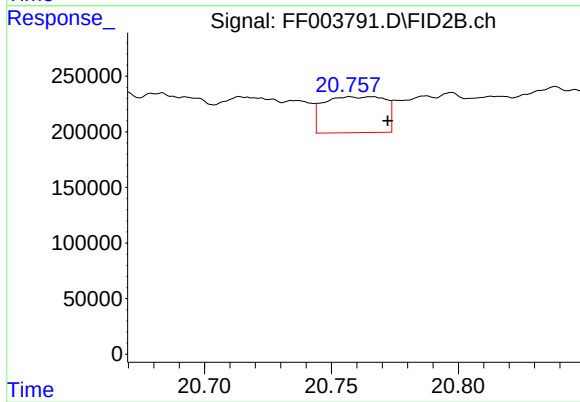

#17 N-OCTATRIACONTANE

R.T.: 20.757 min
Delta R.T.: -0.015 min
Response: 544765
Conc: 4.72 ug/ml