

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
 Data File : FF003794.D
 Signal(s) : FID2B.ch
 Acq On : 12 Mar 2019 13:35
 Operator : AJ\SJ
 Sample : K1691-05 5X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 13 00:59:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.592	308405	2.215 ug/ml
Target Compounds			
7) N-EICOSANE	12.544	407631	2.492 ug/ml
10) N-TETRACOSANE	14.773	248779	1.572 ug/ml
11) N-HEXACOSANE	15.820	91667	0.594 ug/ml
12) N-OCTACOSANE	16.778	262486	1.737 ug/ml
13) N-TRIACONTANE	17.661	424184	2.884 ug/ml
14) N-DOTRIACONTANE	18.503	438310	3.082 ug/ml
15) N-TETRATRIACONTANE	19.299	1276698	9.535 ug/ml
16) N-HEXATRIACONTANE	20.080	10799885	82.770 ug/ml
17) N-OCTATRIACONTANE	20.771	433601	3.755 ug/ml
18) N-TETRACONTANE	21.675	914188	7.348 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
Data File : FF003794.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2019 13:35
Operator : AJ\SJ
Sample : K1691-05 5X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Mar 13 00:59:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

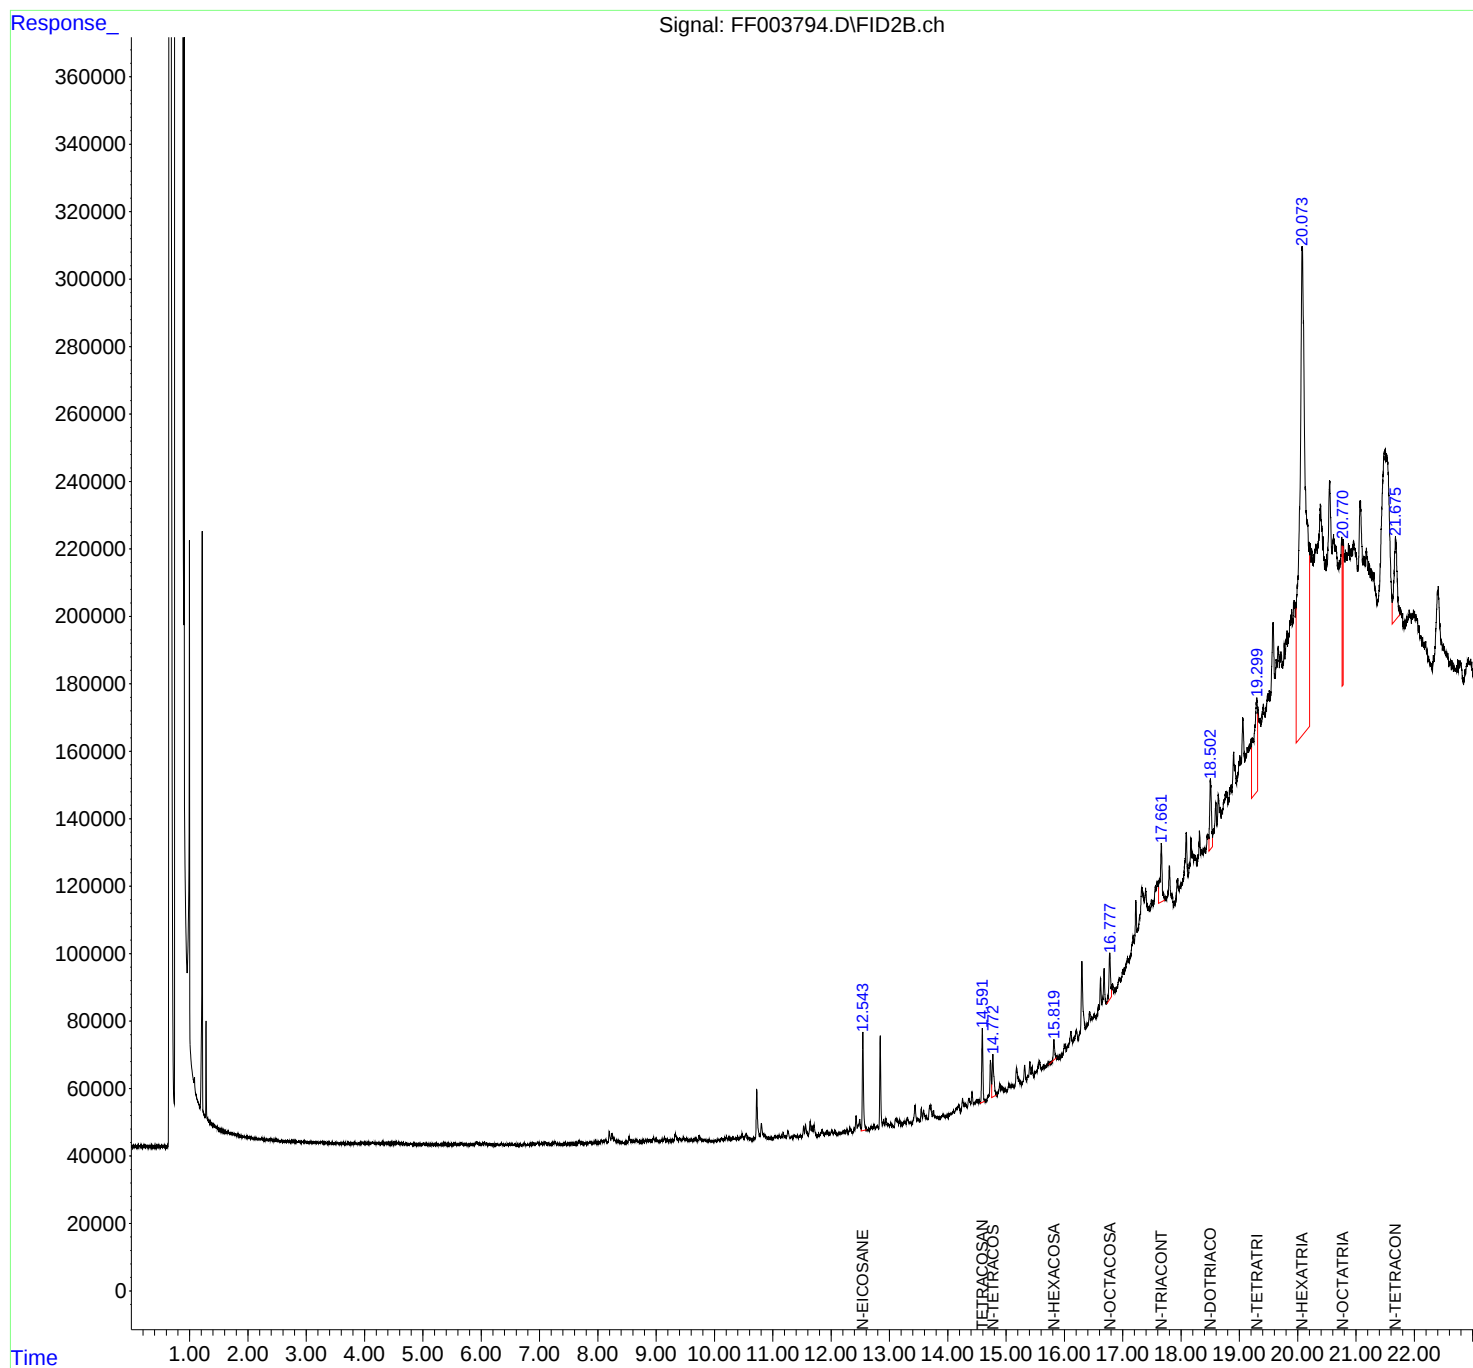


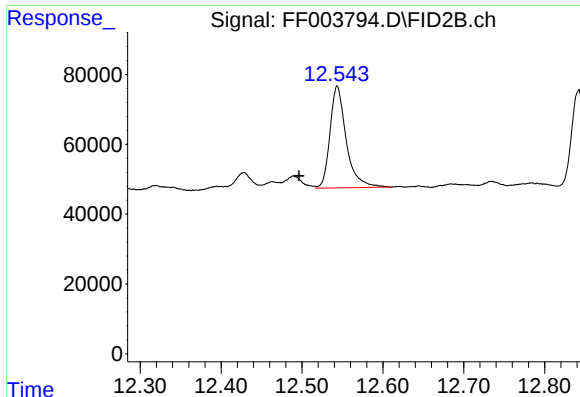

#7 N-EICOSANE


R.T.: 12.544 min
Delta R.T.: 0.047 min
Response: 407631
Conc: 2.49 ug/ml

Instrument :
FID_F
ClientSampleId :

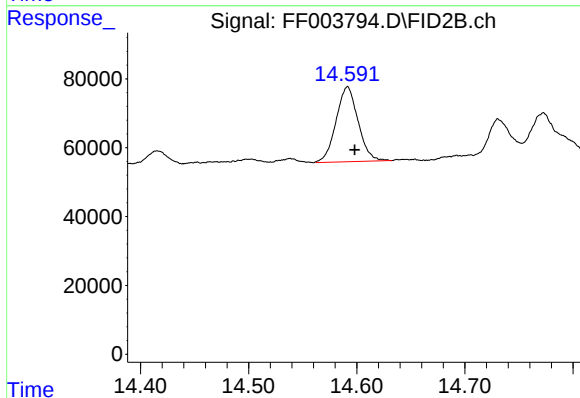


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.592 min
Delta R.T.: -0.007 min
Response: 308405
Conc: 2.22 ug/ml

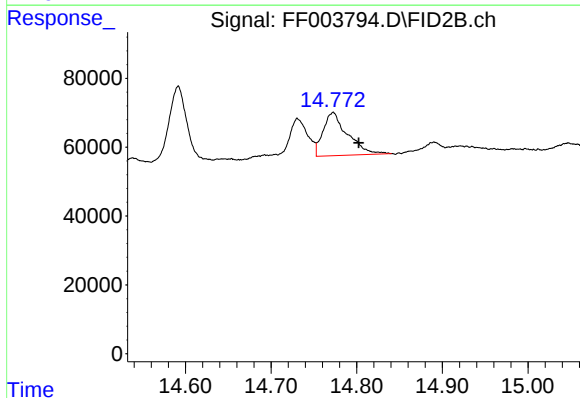


#10 N-TETRACOSANE

R.T.: 14.773 min
Delta R.T.: -0.030 min
Response: 248779
Conc: 1.57 ug/ml

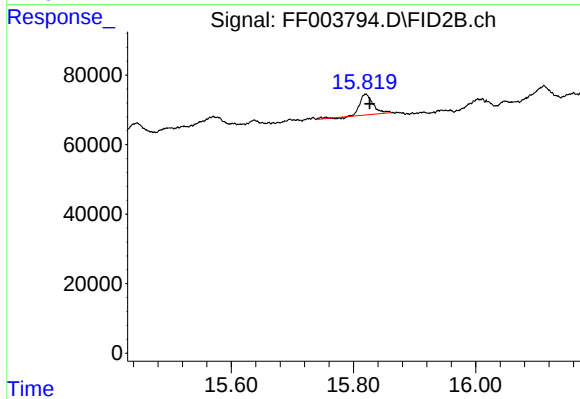

#11 N-HEXACOSANE


R.T.: 15.820 min
Delta R.T.: -0.007 min
Response: 91667
Conc: 0.59 ug/ml

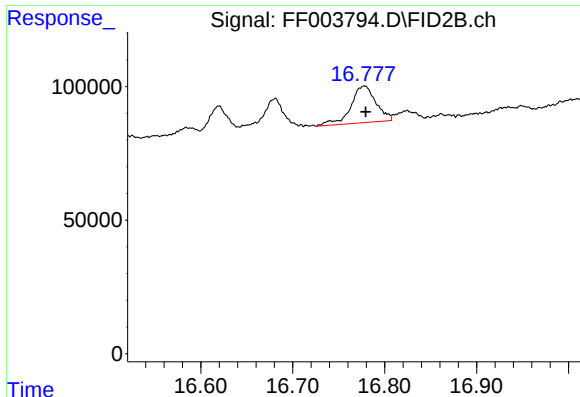

#12 N-OCTACOSANE


R.T.: 16.778 min
Delta R.T.: -0.002 min
Response: 262486
Conc: 1.74 ug/ml

Instrument :
FID_F
ClientSampleId :

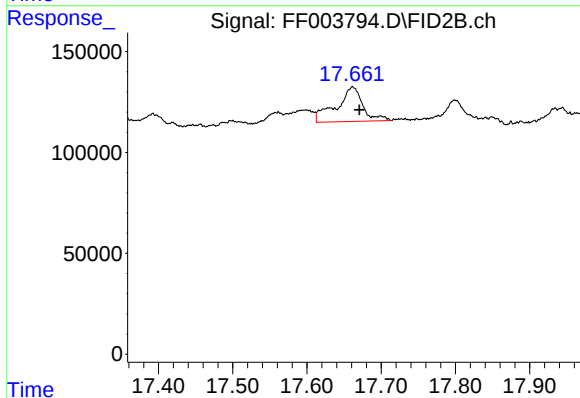


#13 N-TRIACONTANE

R.T.: 17.661 min
Delta R.T.: -0.009 min
Response: 424184
Conc: 2.88 ug/ml

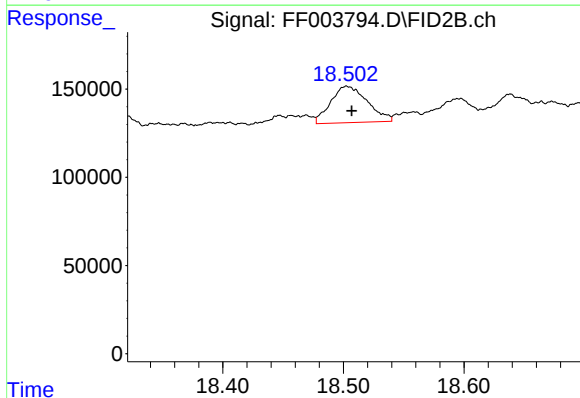


#14 N-DOTRIACONTANE

R.T.: 18.503 min
Delta R.T.: -0.004 min
Response: 438310
Conc: 3.08 ug/ml

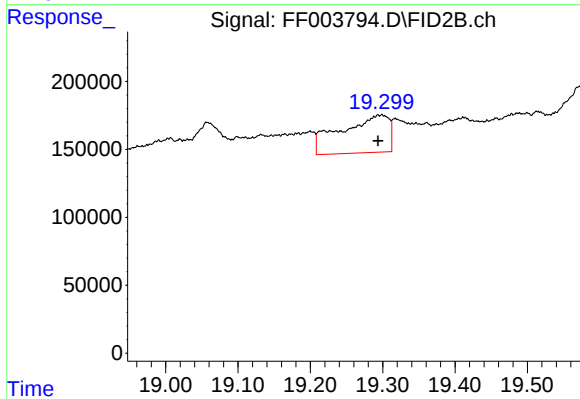

#15 N-TETRATRIACONTANE


R.T.: 19.299 min
Delta R.T.: 0.005 min
Response: 1276698
Conc: 9.53 ug/ml

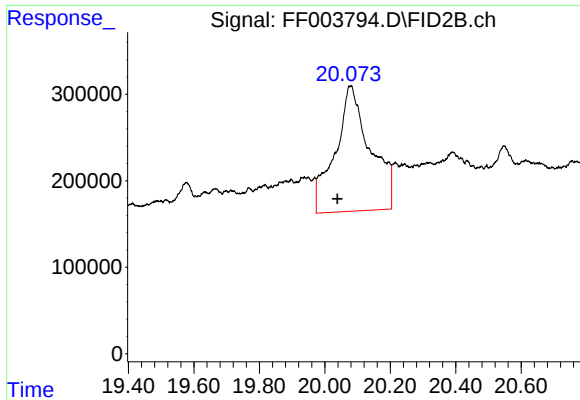

#16 N-HEXATRIACONTANE


R.T.: 20.080 min
Delta R.T.: 0.042 min
Response: 10799885
Conc: 82.77 ug/ml

Instrument :
FID_F
ClientSampleId :

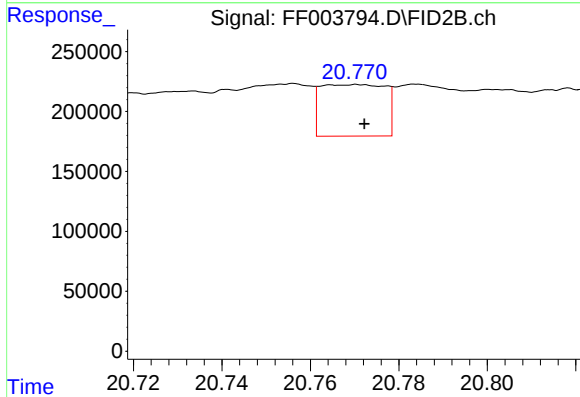

#17 N-OCTATRIACONTANE

R.T.: 20.771 min
Delta R.T.: -0.001 min
Response: 433601
Conc: 3.76 ug/ml

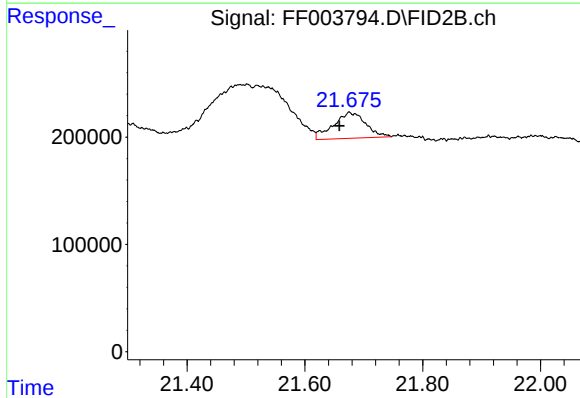

#18 N-TETRACONTANE

R.T.: 21.675 min
Delta R.T.: 0.017 min
Response: 914188
Conc: 7.35 ug/ml