

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
 Data File : FF003795.D
 Signal(s) : FID2B.ch
 Acq On : 12 Mar 2019 14:06
 Operator : AJ\SJ
 Sample : K1691-01 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 13 00:59:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.593	1300644	9.342 ug/ml
Target Compounds			
4) N-TETRADECANE	8.192f	148995	0.929 ug/ml
7) N-EICOSANE	12.545	3076636	18.807 ug/ml
8) N-DOCOSANE	13.711	298383	1.849 ug/ml
10) N-TETRACOSANE	14.770	1479598	9.351 ug/ml
11) N-HEXACOSANE	15.819	291865	1.891 ug/ml
12) N-OCTACOSANE	16.779	645239	4.270 ug/ml
13) N-TRIACONTANE	17.665	719603	4.892 ug/ml
14) N-DOTRIACONTANE	18.503	279801	1.968 ug/ml
15) N-TETRATRIACONTANE	19.287	250125	1.868 ug/ml
16) N-HEXATRIACONTANE	20.038	228558	1.752 ug/ml
17) N-OCTATRIACONTANE	20.769	70046	0.607 ug/ml
18) N-TETRACONTANE	21.652	70906	0.570 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
Data File : FF003795.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2019 14:06
Operator : AJ\SJ
Sample : K1691-01 2X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 13 00:59:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

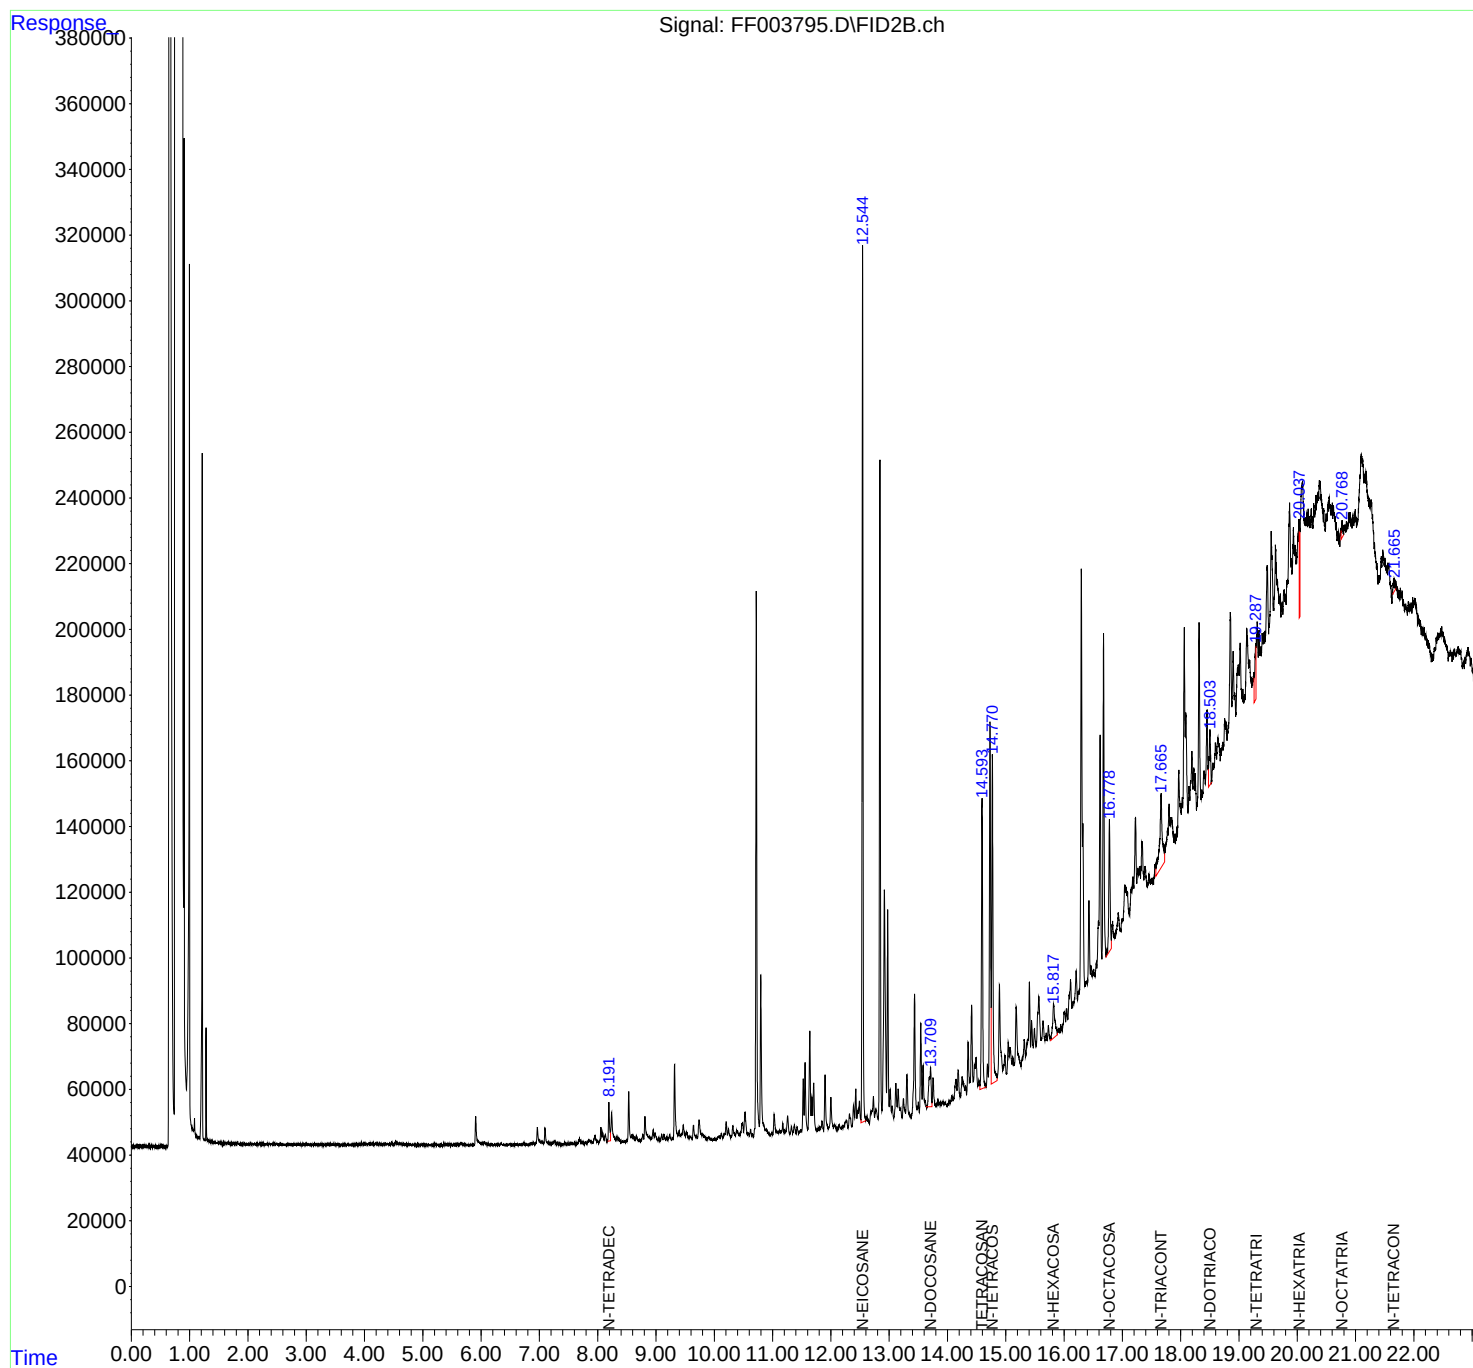


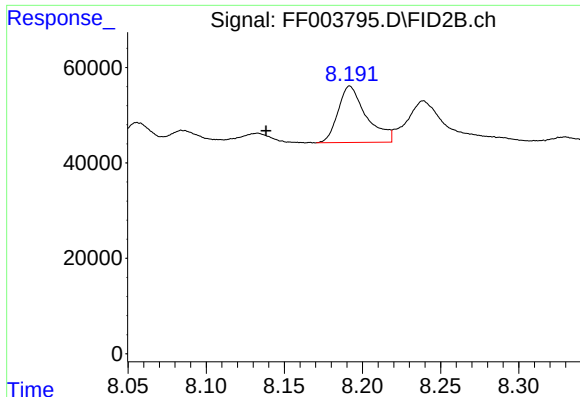

#4 N-TETRADECANE


R.T.: 8.192 min
Delta R.T.: 0.054 min
Response: 148995
Conc: 0.93 ug/ml

Instrument :
FID_F
ClientSampleId :

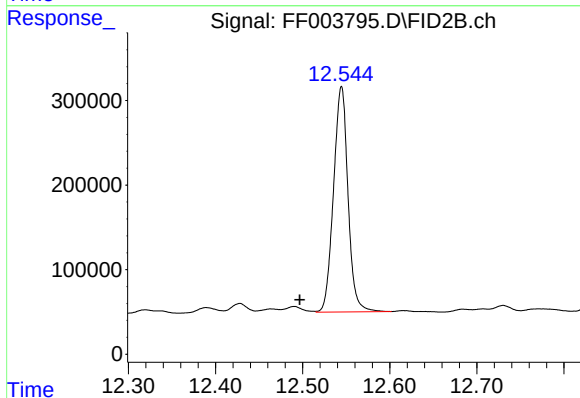


#7 N-EICOSANE

R.T.: 12.545 min
Delta R.T.: 0.048 min
Response: 3076636
Conc: 18.81 ug/ml

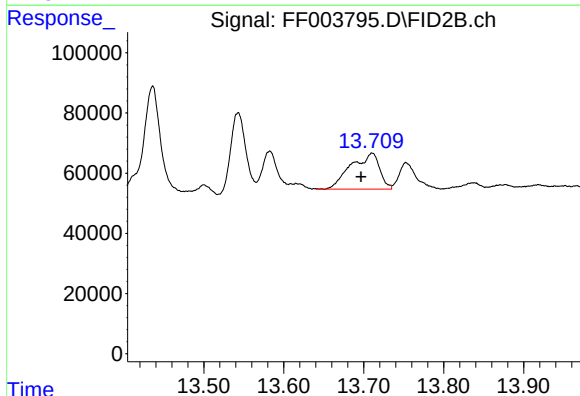


#8 N-DOCOSANE

R.T.: 13.711 min
Delta R.T.: 0.014 min
Response: 298383
Conc: 1.85 ug/ml

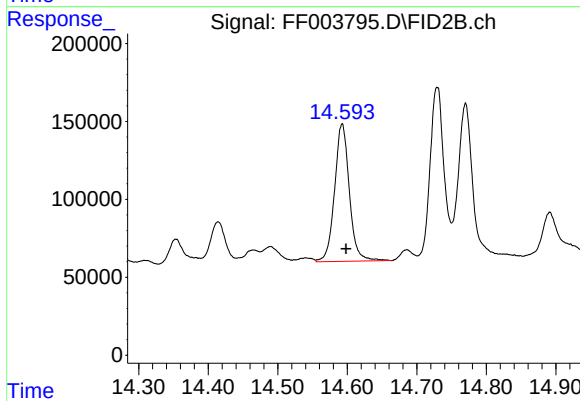

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.593 min
Delta R.T.: -0.006 min
Response: 1300644
Conc: 9.34 ug/ml

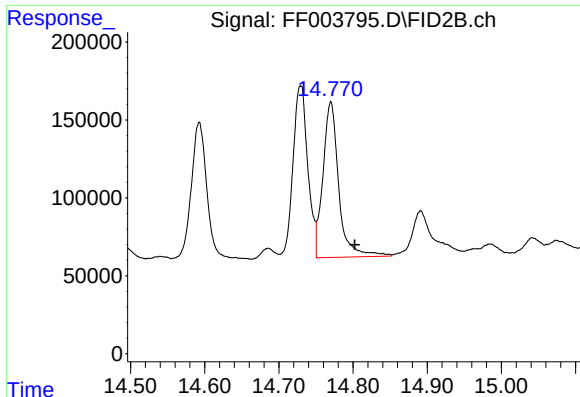

#10 N-TETRACOSANE


R.T.: 14.770 min
Delta R.T.: -0.032 min
Response: 1479598
Conc: 9.35 ug/ml

Instrument :
FID_F
ClientSampleId :

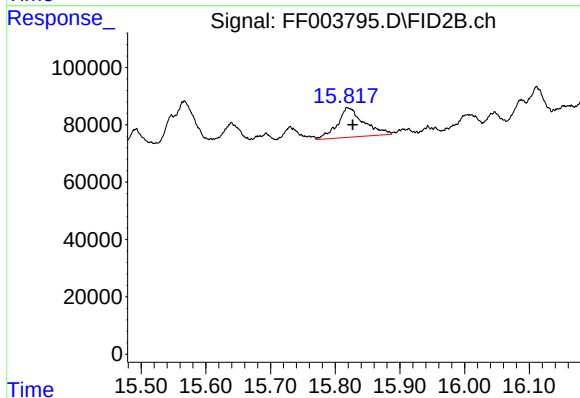


#11 N-HEXACOSANE

R.T.: 15.819 min
Delta R.T.: -0.008 min
Response: 291865
Conc: 1.89 ug/ml

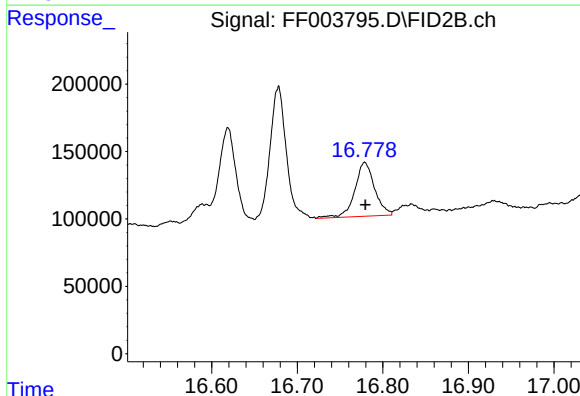


#12 N-OCTACOSANE

R.T.: 16.779 min
Delta R.T.: 0.000 min
Response: 645239
Conc: 4.27 ug/ml

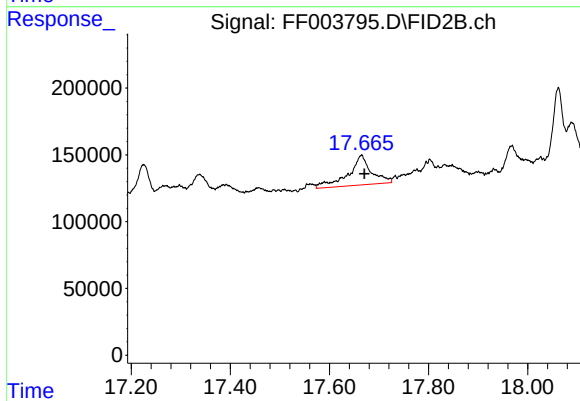

#13 N-TRIACONTANE


R.T.: 17.665 min
Delta R.T.: -0.006 min
Response: 719603
Conc: 4.89 ug/ml

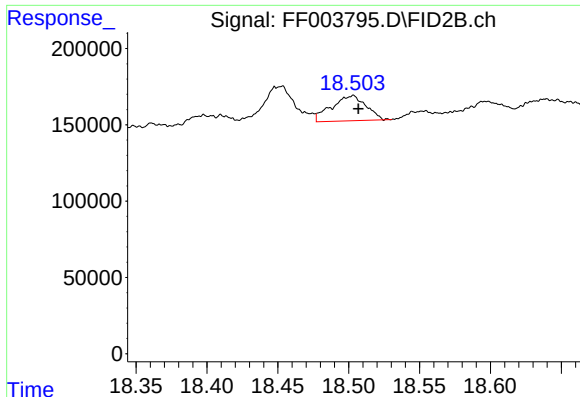

#14 N-DOTRIACONTANE


R.T.: 18.503 min
Delta R.T.: -0.004 min
Response: 279801
Conc: 1.97 ug/ml

Instrument :
FID_F
ClientSampleId :

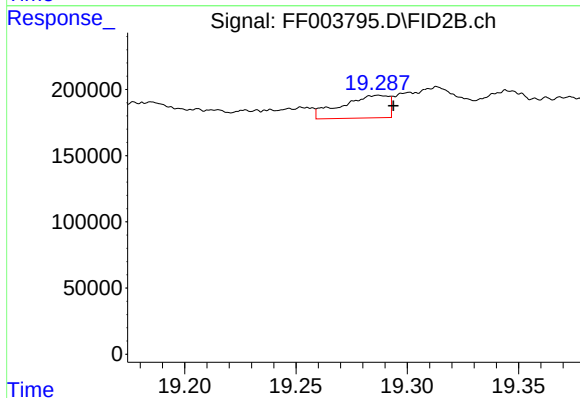


#15 N-TETRATRIACONTANE

R.T.: 19.287 min
Delta R.T.: -0.007 min
Response: 250125
Conc: 1.87 ug/ml

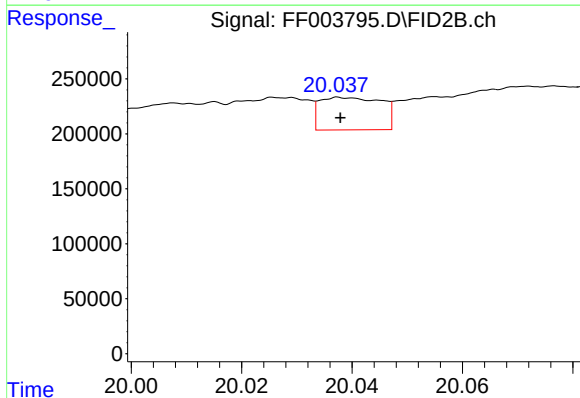


#16 N-HEXATRIACONTANE

R.T.: 20.038 min
Delta R.T.: 0.000 min
Response: 228558
Conc: 1.75 ug/ml

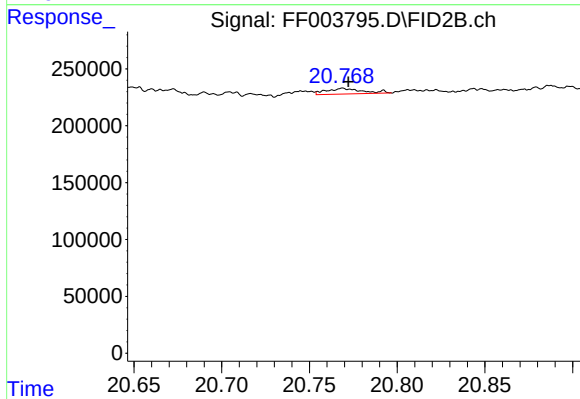

#17 N-OCTATRIACONTANE

R.T.: 20.769 min
Delta R.T.: -0.003 min
Response: 70046
Conc: 0.61 ug/ml

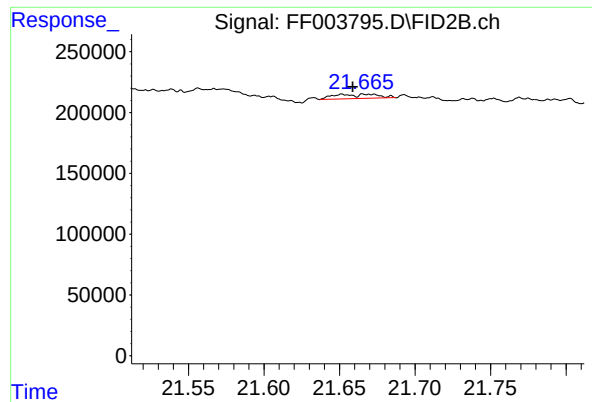

#18 N-TETRACONTANE

R.T.: 21.652 min
Delta R.T.: -0.007 min
Response: 70906
Conc: 0.57 ug/ml

Instrument :
FID_F
ClientSampleId :