

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
 Data File : FF003796.D
 Signal(s) : FID2B.ch
 Acq On : 12 Mar 2019 14:36
 Operator : AJ\SJ
 Sample : K1691-07 2X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 13 00:59:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.592	853134	6.128 ug/ml
Target Compounds			
4) N-TETRADECANE	8.192f	134282	0.838 ug/ml
7) N-EICOSANE	12.543	534676	3.268 ug/ml
10) N-TETRACOSANE	14.771	348210	2.201 ug/ml
11) N-HEXACOSANE	15.821	278502	1.804 ug/ml
12) N-OCTACOSANE	16.777	492185	3.257 ug/ml
13) N-TRIACONTANE	17.664	573815	3.901 ug/ml
14) N-DOTRIACONTANE	18.507	928460	6.529 ug/ml
15) N-TETRATRIACONTANE	19.293	942517	7.039 ug/ml
16) N-HEXATRIACONTANE	20.071	3080260	23.607 ug/ml
17) N-OCTATRIACONTANE	20.768	284401	2.463 ug/ml
18) N-TETRACONTANE	21.675	1846775	14.845 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
Data File : FF003796.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2019 14:36
Operator : AJ\SJ
Sample : K1691-07 2X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 13 00:59:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

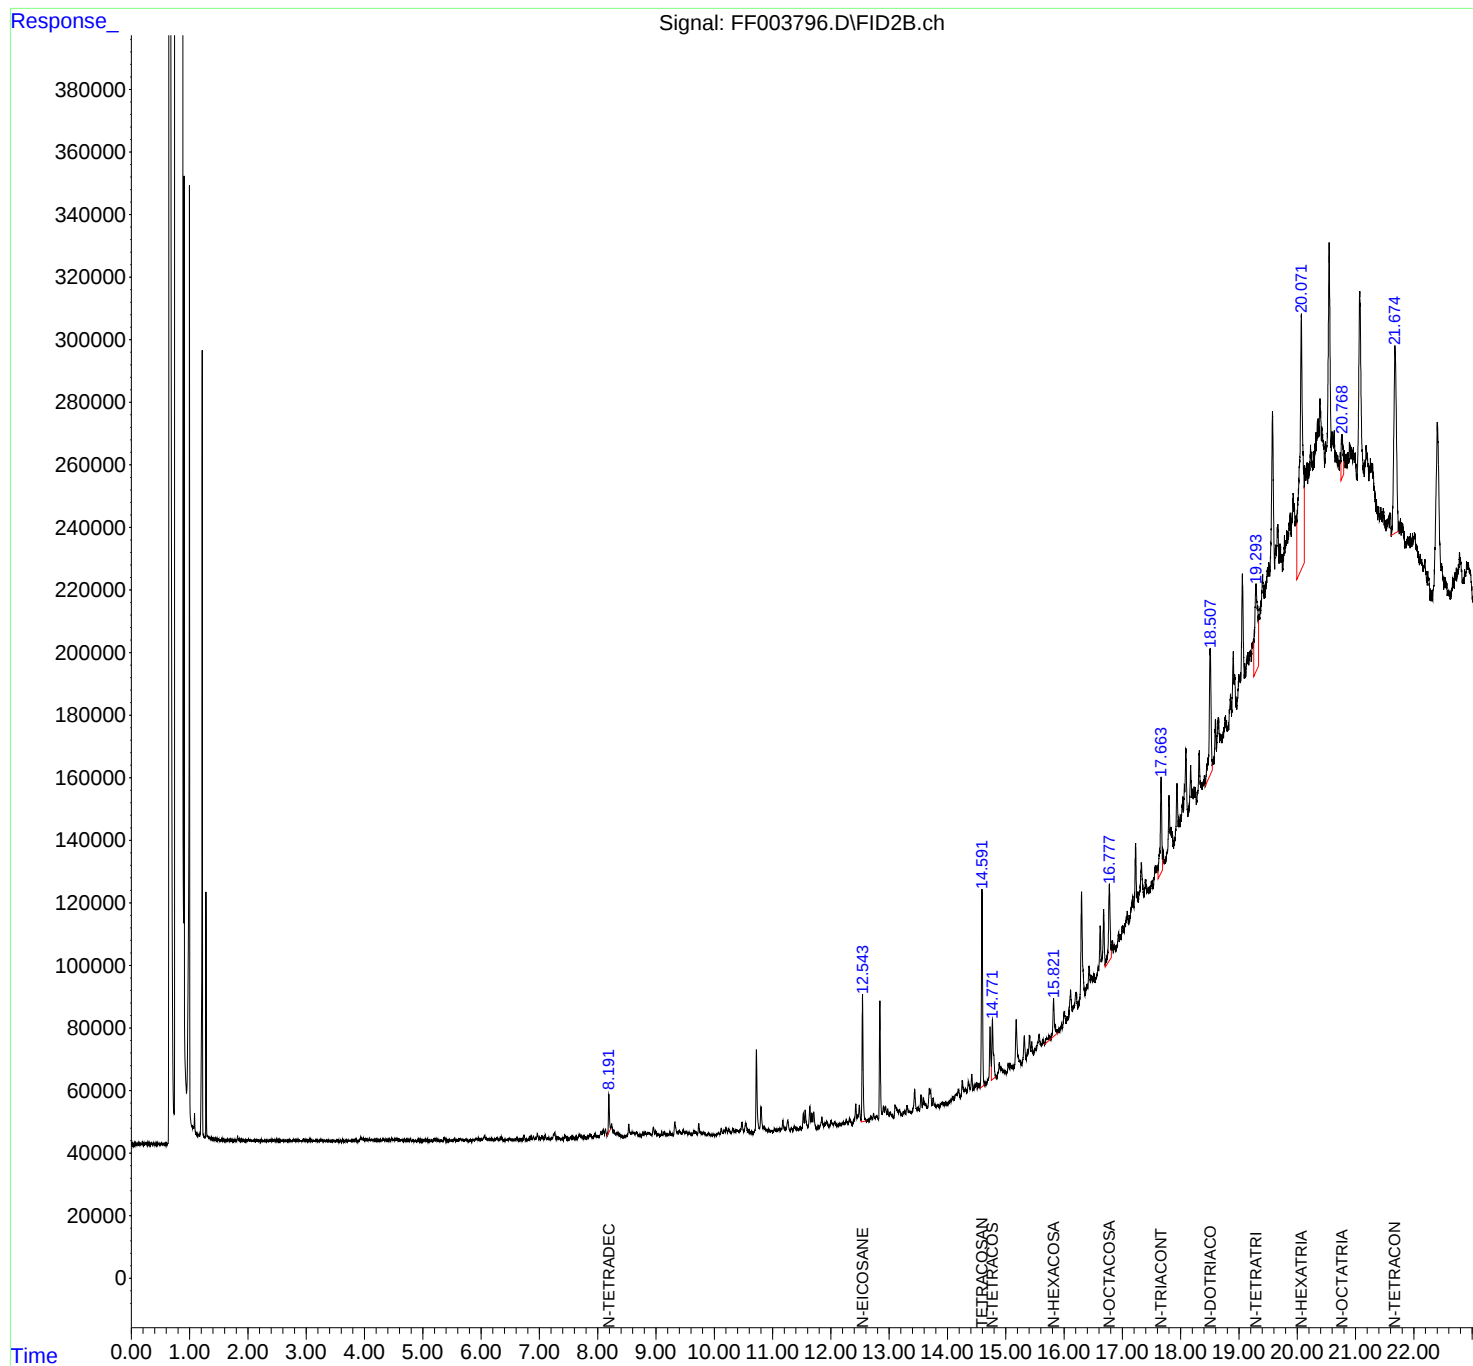


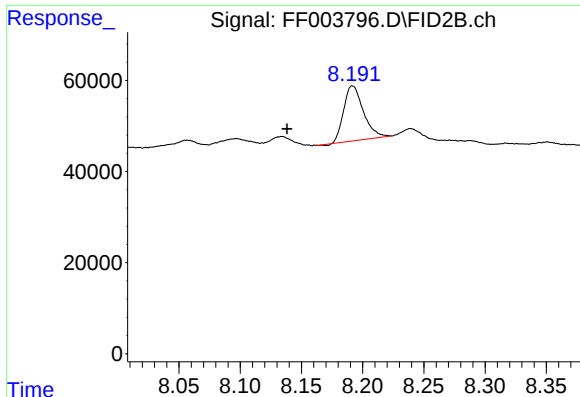

#4 N-TETRADECANE


R.T.: 8.192 min
Delta R.T.: 0.054 min
Response: 134282
Conc: 0.84 ug/ml

Instrument :
FID_F
ClientSampleId :

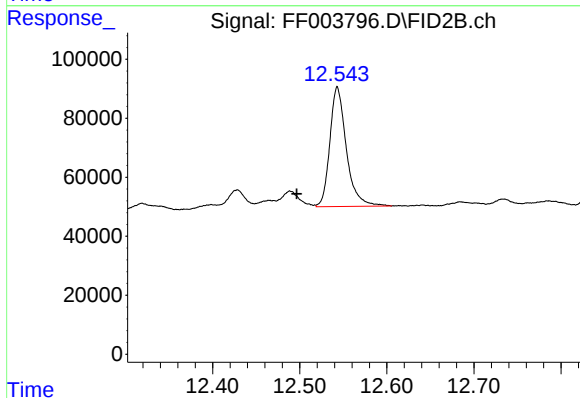


#7 N-EICOSANE

R.T.: 12.543 min
Delta R.T.: 0.047 min
Response: 534676
Conc: 3.27 ug/ml

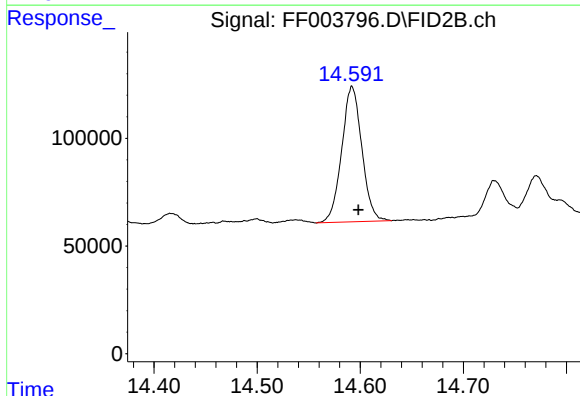


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.592 min
Delta R.T.: -0.006 min
Response: 853134
Conc: 6.13 ug/ml

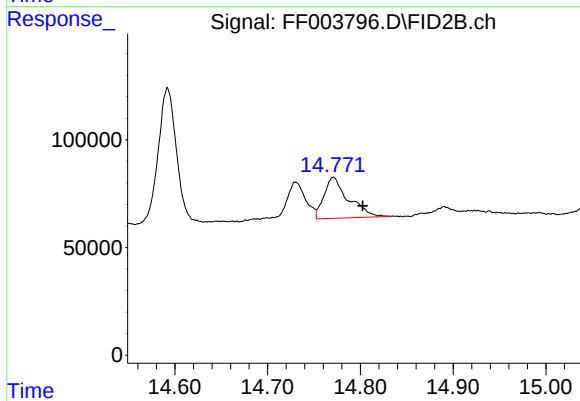

#10 N-TETRACOSANE


R.T.: 14.771 min
Delta R.T.: -0.032 min
Response: 348210
Conc: 2.20 ug/ml

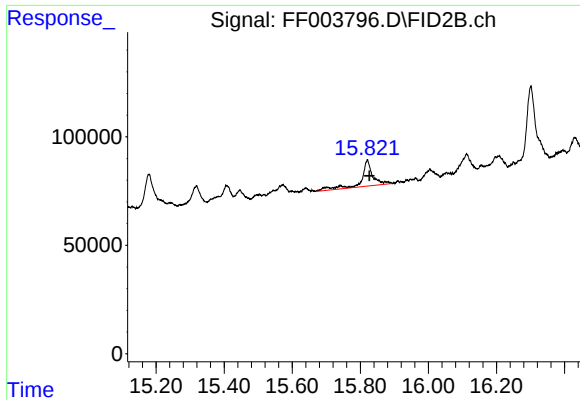

#11 N-HEXACOSANE


R.T.: 15.821 min
Delta R.T.: -0.006 min
Response: 278502
Conc: 1.80 ug/ml

Instrument :
FID_F
ClientSampleId :

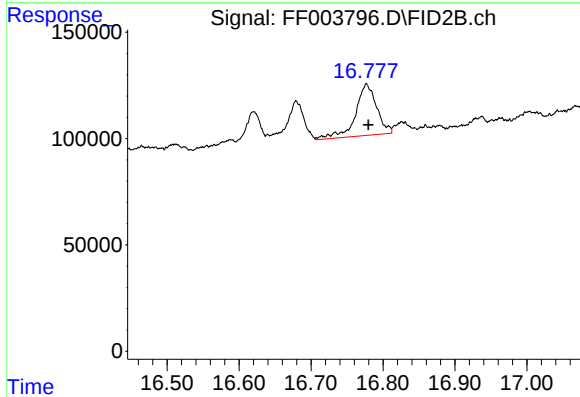


#12 N-OCTACOSANE

R.T.: 16.777 min
Delta R.T.: -0.003 min
Response: 492185
Conc: 3.26 ug/ml

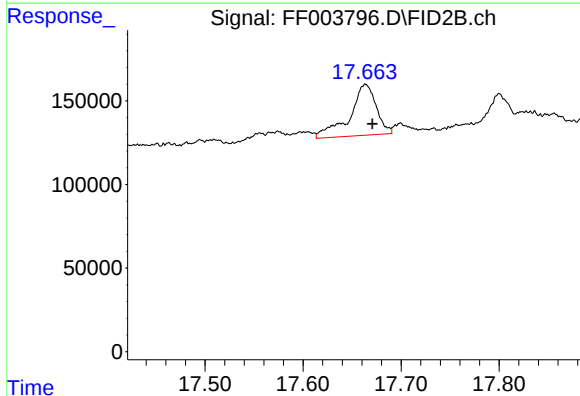


#13 N-TRIACONTANE

R.T.: 17.664 min
Delta R.T.: -0.007 min
Response: 573815
Conc: 3.90 ug/ml

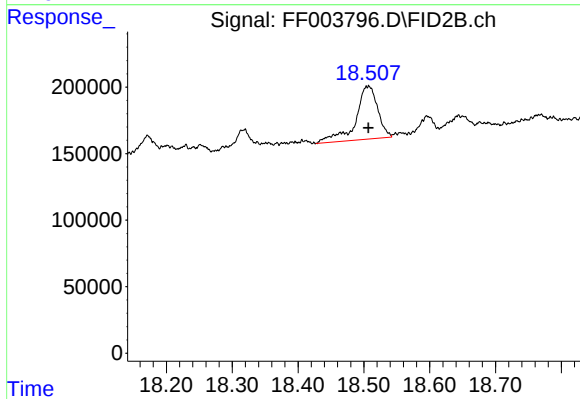

#14 N-DOTRIACONTANE


R.T.: 18.507 min
Delta R.T.: 0.000 min
Response: 928460
Conc: 6.53 ug/ml

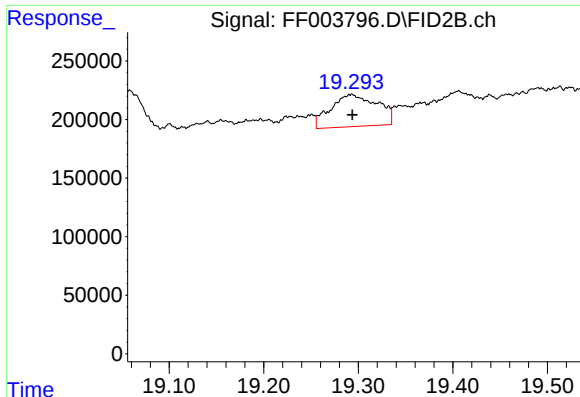

#15 N-TETRATRIACONTANE


R.T.: 19.293 min
Delta R.T.: 0.000 min
Response: 942517
Conc: 7.04 ug/ml

Instrument :
FID_F
ClientSampleId :

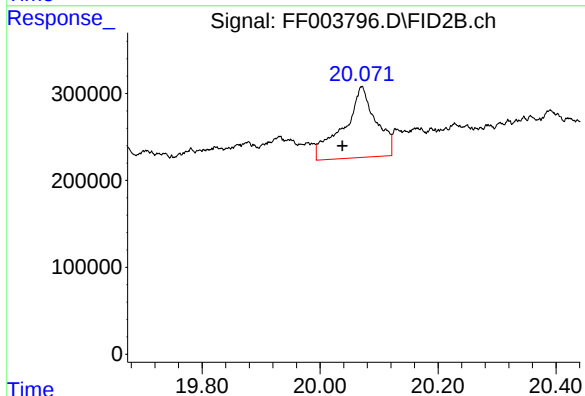


#16 N-HEXATRIACONTANE

R.T.: 20.071 min
Delta R.T.: 0.033 min
Response: 3080260
Conc: 23.61 ug/ml

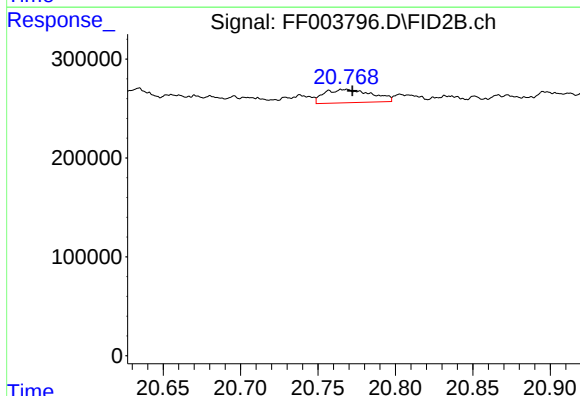

#17 N-OCTATRIACONTANE

R.T.: 20.768 min
Delta R.T.: -0.004 min
Response: 284401
Conc: 2.46 ug/ml

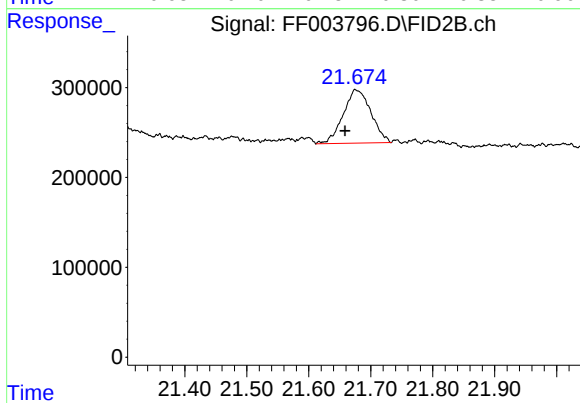

#18 N-TETRACONTANE

R.T.: 21.675 min
Delta R.T.: 0.016 min
Response: 1846775
Conc: 14.84 ug/ml