

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
 Data File : FF003799.D
 Signal(s) : FID2B.ch
 Acq On : 12 Mar 2019 16:08
 Operator : AJ\SJ
 Sample : K1846-06 2X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 13 01:00:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.593	784073	5.632 ug/ml
Target Compounds			
4) N-TETRADECANE	8.192f	120244	0.750 ug/ml
5) N-HEXADECANE	9.734	85070	0.522 ug/ml
7) N-EICOSANE	12.489	109815	0.671 ug/ml
8) N-DOCOSANE	13.689	104054	0.645 ug/ml
10) N-TETRACOSANE	14.772	283860	1.794 ug/ml
11) N-HEXACOSANE	15.821	156415	1.013 ug/ml
12) N-OCTACOSANE	16.780	442282	2.927 ug/ml
13) N-TRIACONTANE	17.664	674632	4.586 ug/ml
14) N-DOTRIACONTANE	18.500	542565	3.815 ug/ml
15) N-TETRATRIACONTANE	19.292	535174	3.997 ug/ml
16) N-HEXATRIACONTANE	20.038	585290	4.486 ug/ml
17) N-OCTATRIACONTANE	20.765	206997	1.793 ug/ml
18) N-TETRACONTANE	21.669	273535	2.199 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
Data File : FF003799.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2019 16:08
Operator : AJ\SJ
Sample : K1846-06 2X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Mar 13 01:00:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

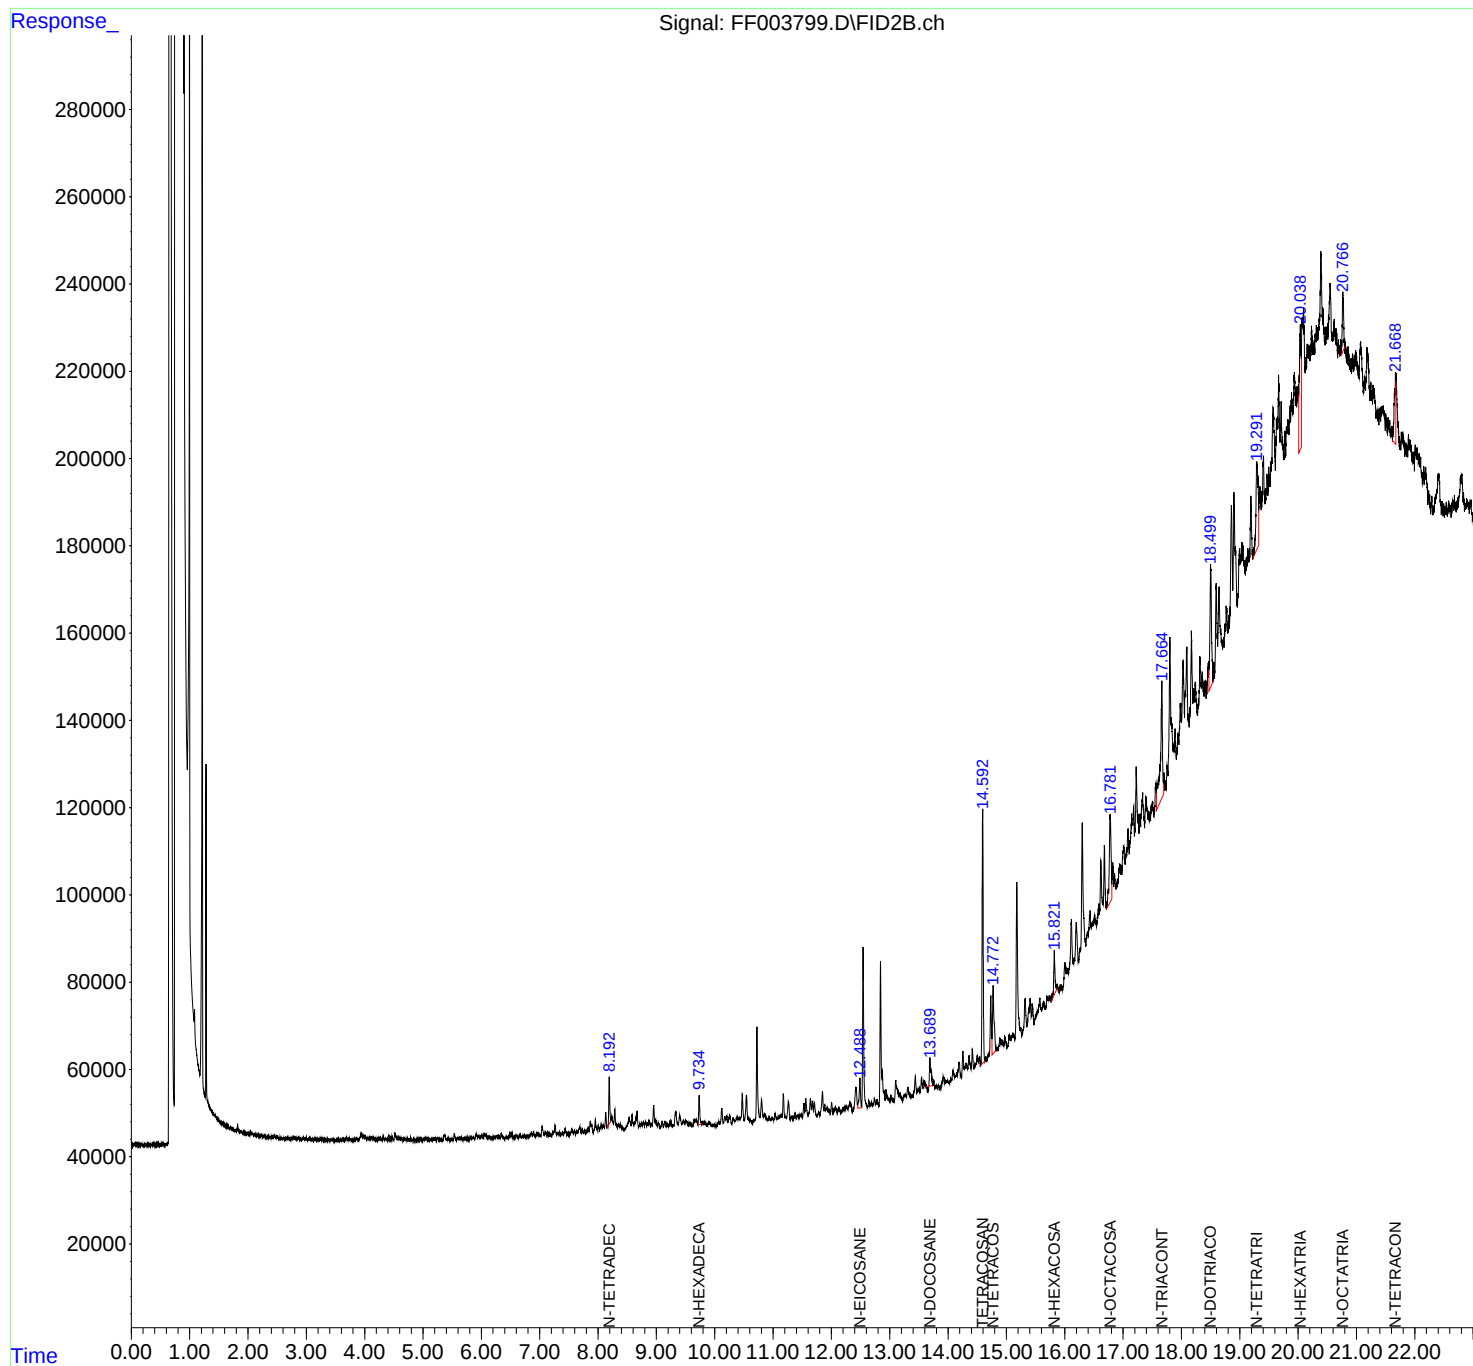


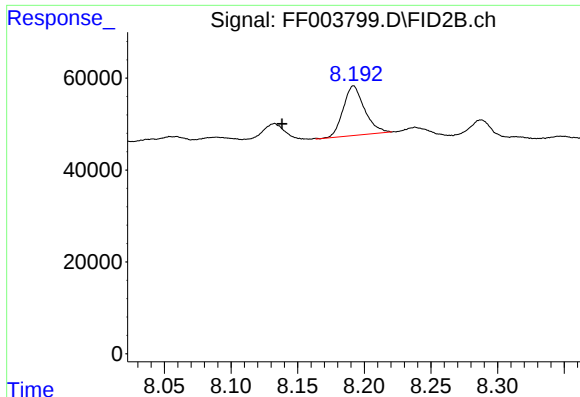

#4 N-TETRADECANE


R.T.: 8.192 min
Delta R.T.: 0.054 min
Response: 120244
Conc: 0.75 ug/ml

Instrument :
FID_F
ClientSampleId :

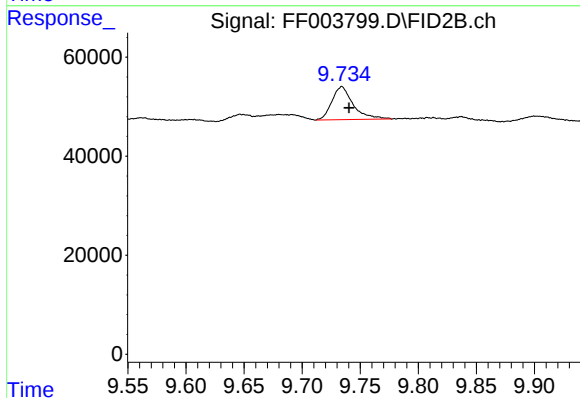


#5 N-HEXADECANE

R.T.: 9.734 min
Delta R.T.: -0.006 min
Response: 85070
Conc: 0.52 ug/ml

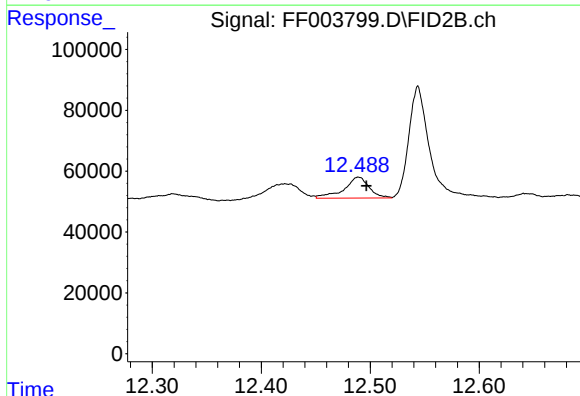


#7 N-EICOSANE

R.T.: 12.489 min
Delta R.T.: -0.007 min
Response: 109815
Conc: 0.67 ug/ml

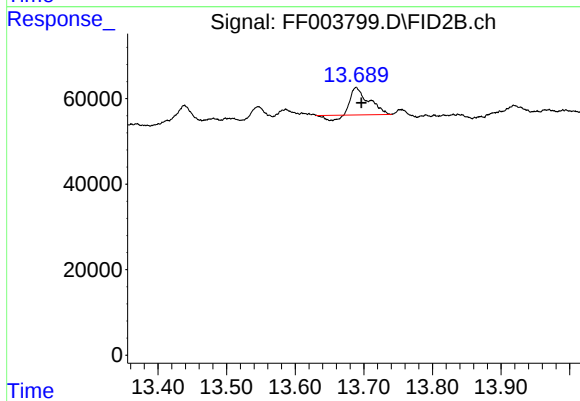

#8 N-DOCOSANE


R.T.: 13.689 min
Delta R.T.: -0.008 min
Response: 104054
Conc: 0.64 ug/ml

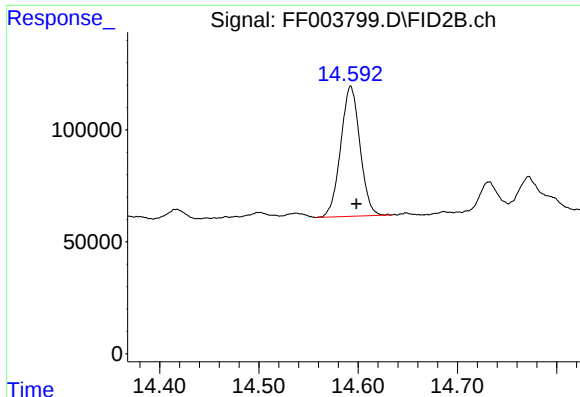

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.593 min
Delta R.T.: -0.006 min
Response: 784073
Conc: 5.63 ug/ml

Instrument :
FID_F
ClientSampleId :

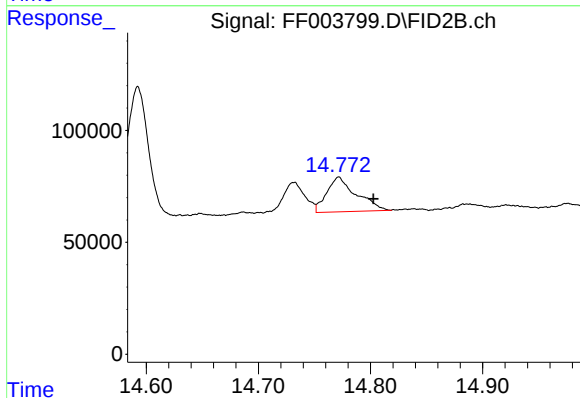


#10 N-TETRACOSANE

R.T.: 14.772 min
Delta R.T.: -0.031 min
Response: 283860
Conc: 1.79 ug/ml

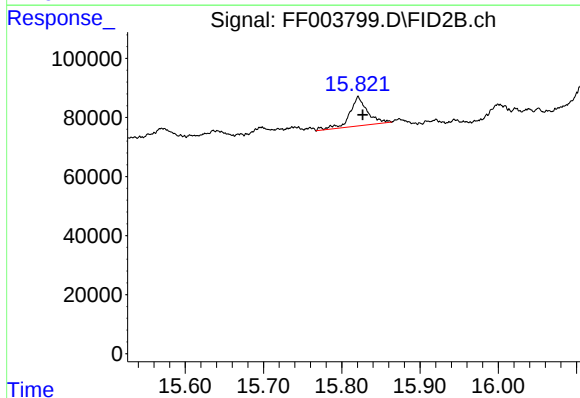


#11 N-HEXACOSANE

R.T.: 15.821 min
Delta R.T.: -0.006 min
Response: 156415
Conc: 1.01 ug/ml

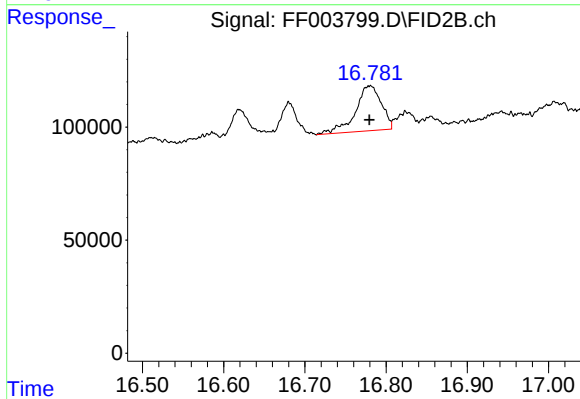

#12 N-OCTACOSANE


R.T.: 16.780 min
Delta R.T.: 0.000 min
Response: 442282
Conc: 2.93 ug/ml

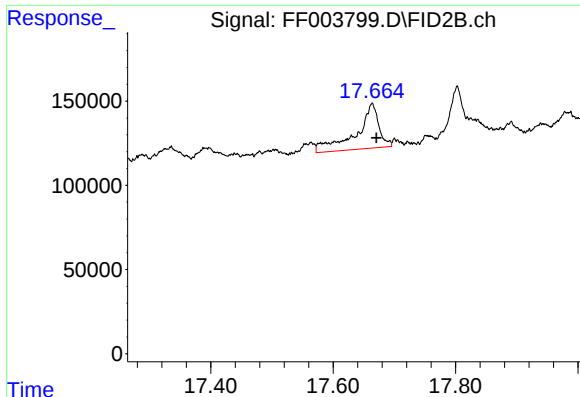

#13 N-TRIACONTANE


R.T.: 17.664 min
Delta R.T.: -0.007 min
Response: 674632
Conc: 4.59 ug/ml

Instrument :
FID_F
ClientSampleId :

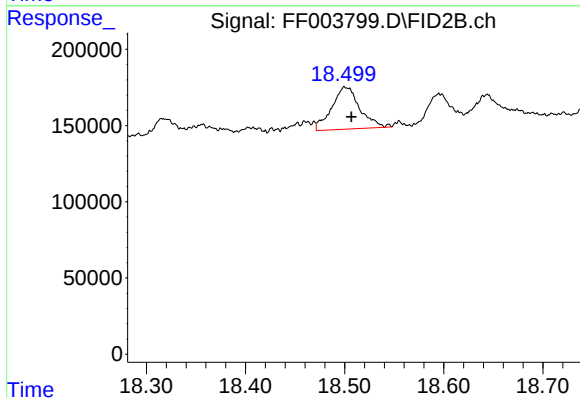


#14 N-DOTRIACONTANE

R.T.: 18.500 min
Delta R.T.: -0.006 min
Response: 542565
Conc: 3.82 ug/ml

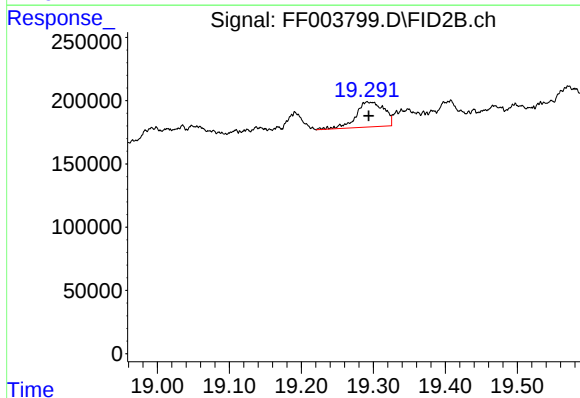


#15 N-TETRATRIACONTANE

R.T.: 19.292 min
Delta R.T.: -0.002 min
Response: 535174
Conc: 4.00 ug/ml

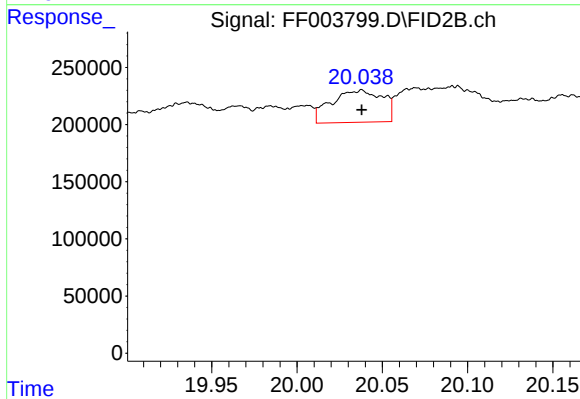

#16 N-HEXATRIACONTANE


R.T.: 20.038 min
Delta R.T.: 0.000 min
Response: 585290
Conc: 4.49 ug/ml

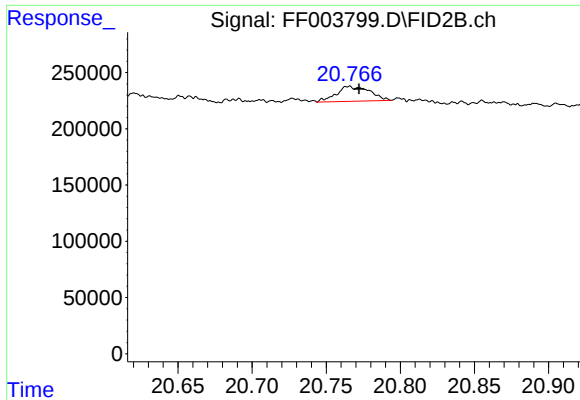

#17 N-OCTATRIACONTANE

R.T.: 20.765 min
Delta R.T.: -0.007 min
Response: 206997
Conc: 1.79 ug/ml

Instrument :
FID_F
ClientSampleId :

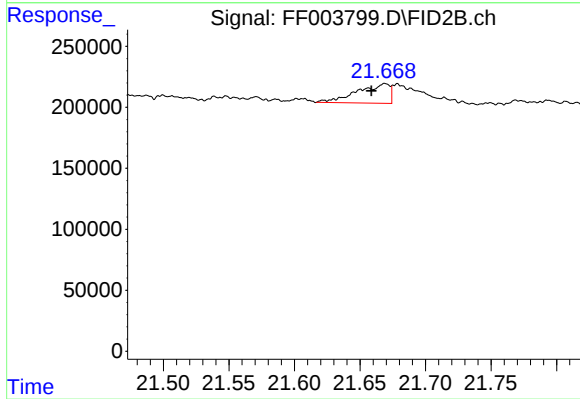

#18 N-TETRACONTANE

R.T.: 21.669 min
Delta R.T.: 0.010 min
Response: 273535
Conc: 2.20 ug/ml