

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
 Data File : FF003800.D
 Signal(s) : FID2B.ch
 Acq On : 12 Mar 2019 16:38
 Operator : AJ\SJ
 Sample : K1846-05 2X
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 13 01:00:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.593	1046203	7.514 ug/ml
Target Compounds			
4) N-TETRADECANE	8.191f	176258	1.099 ug/ml
7) N-EICOSANE	12.543	1366305	8.352 ug/ml
8) N-DOCOSANE	13.688	131669	0.816 ug/ml
10) N-TETRACOSANE	14.771	710563	4.491 ug/ml
11) N-HEXACOSANE	15.821	252092	1.633 ug/ml
12) N-OCTACOSANE	16.780	523566	3.465 ug/ml
13) N-TRIACONTANE	17.664	567288	3.856 ug/ml
14) N-DOTRIACONTANE	18.501	474771	3.339 ug/ml
15) N-TETRATRIACONTANE	19.302	702888	5.249 ug/ml
16) N-HEXATRIACONTANE	20.038	753246	5.773 ug/ml
17) N-OCTATRIACONTANE	20.770	716478	6.205 ug/ml
18) N-TETRACONTANE	21.667	479136	3.851 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
Data File : FF003800.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2019 16:38
Operator : AJ\SJ
Sample : K1846-05 2X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Mar 13 01:00:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

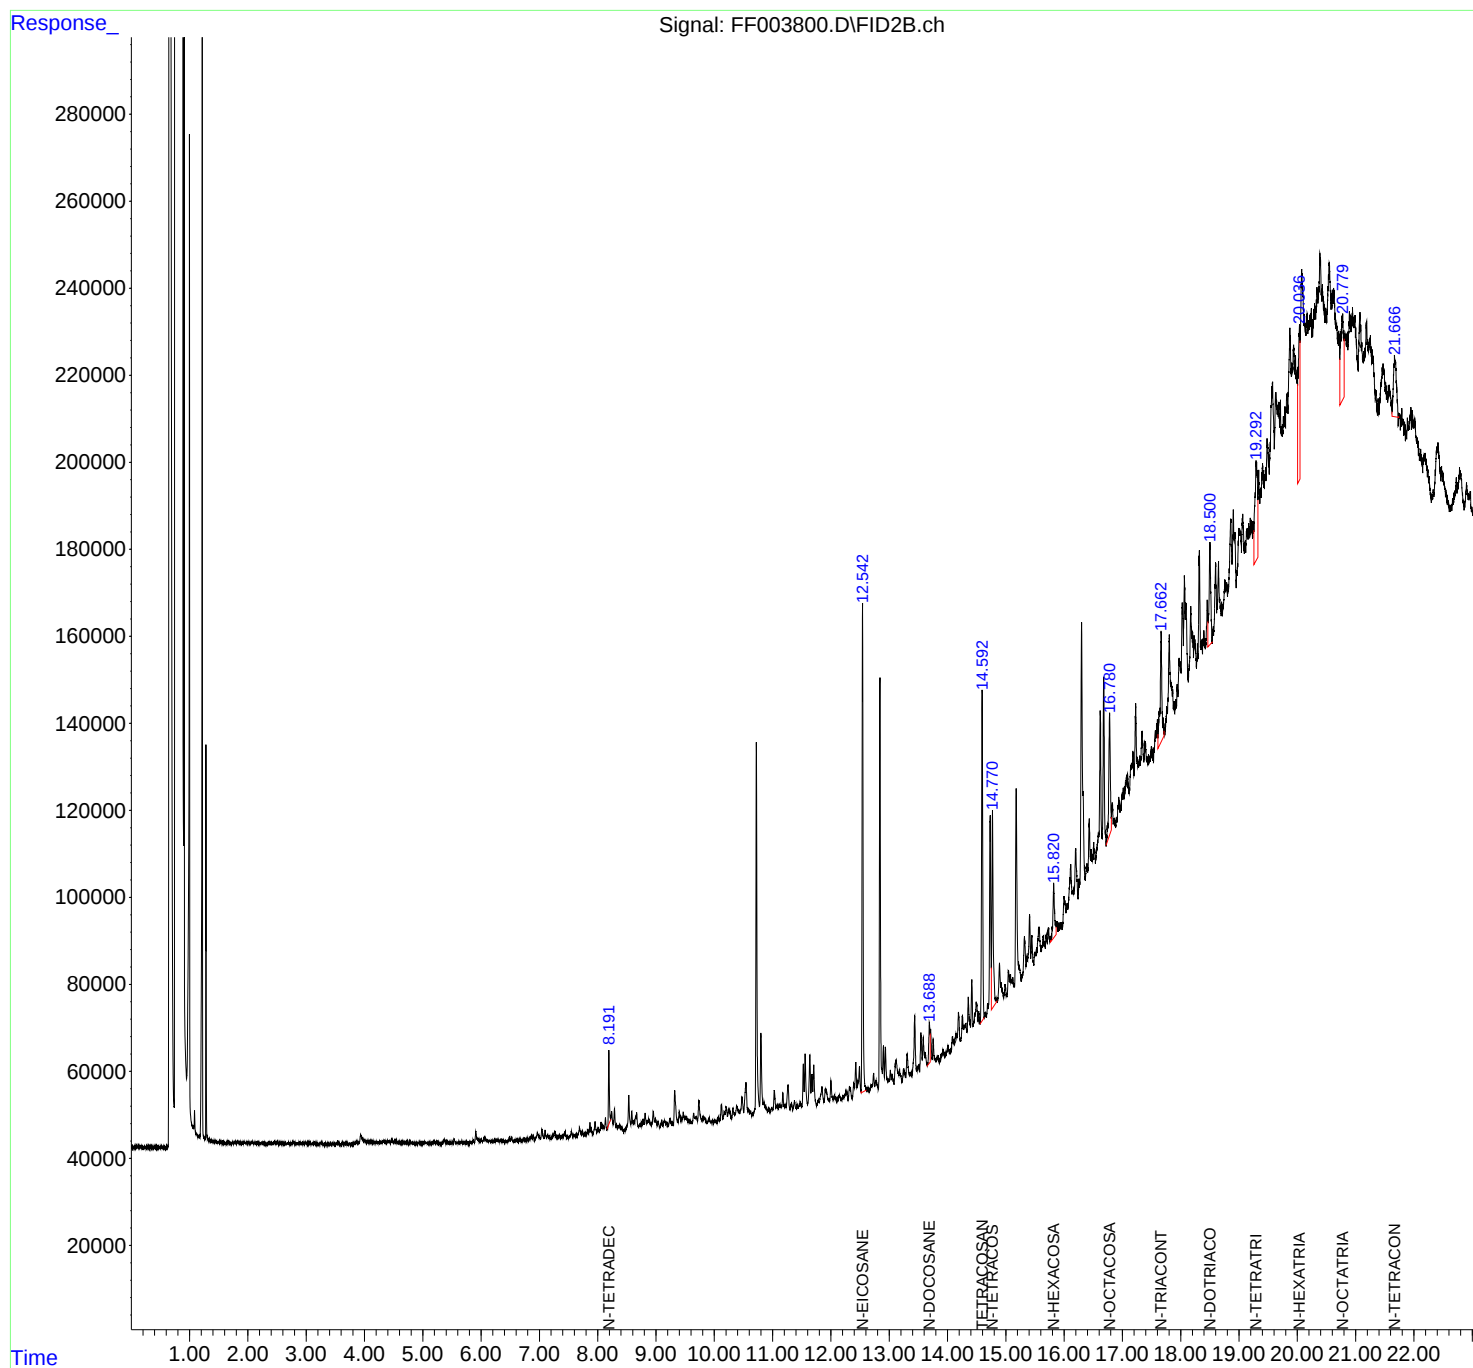


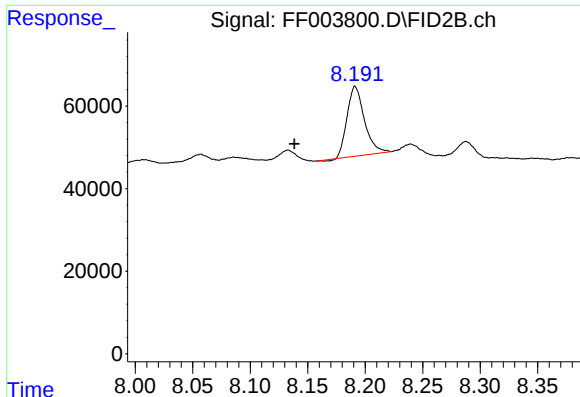

#4 N-TETRADECANE


R.T.: 8.191 min
Delta R.T.: 0.053 min
Response: 176258
Conc: 1.10 ug/ml

Instrument :
FID_F
ClientSampleId :

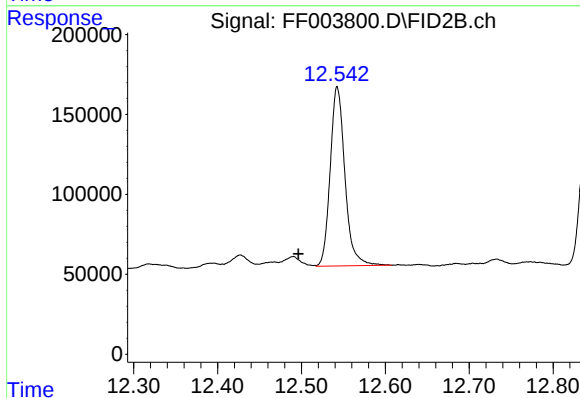


#7 N-EICOSANE

R.T.: 12.543 min
Delta R.T.: 0.046 min
Response: 1366305
Conc: 8.35 ug/ml

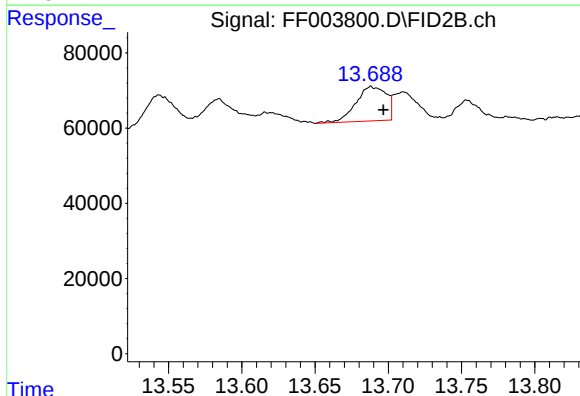


#8 N-DOCOSANE

R.T.: 13.688 min
Delta R.T.: -0.008 min
Response: 131669
Conc: 0.82 ug/ml

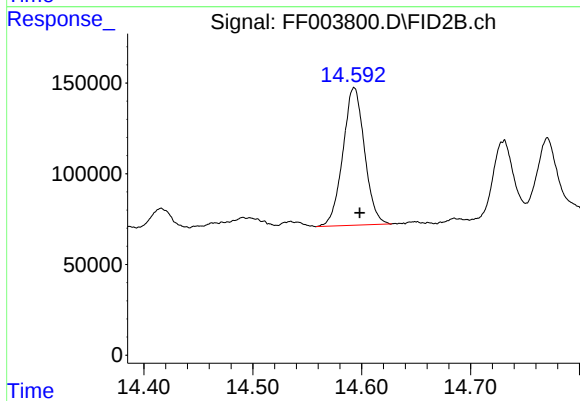

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.593 min
Delta R.T.: -0.005 min
Response: 1046203
Conc: 7.51 ug/ml

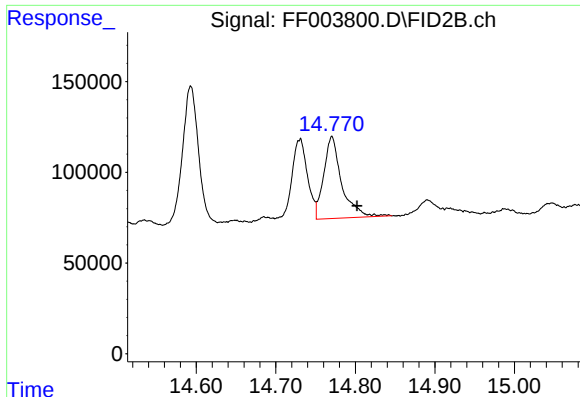

#10 N-TETRACOSANE


R.T.: 14.771 min
Delta R.T.: -0.032 min
Response: 710563
Conc: 4.49 ug/ml

Instrument :
FID_F
ClientSampleId :

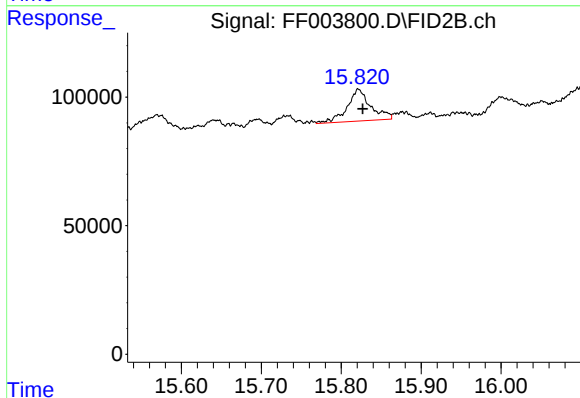


#11 N-HEXACOSANE

R.T.: 15.821 min
Delta R.T.: -0.005 min
Response: 252092
Conc: 1.63 ug/ml

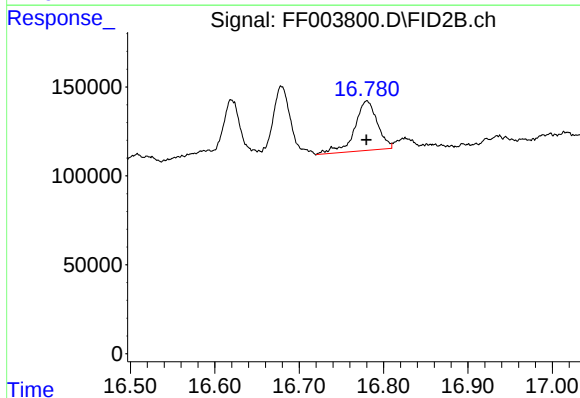


#12 N-OCTACOSANE

R.T.: 16.780 min
Delta R.T.: 0.000 min
Response: 523566
Conc: 3.46 ug/ml

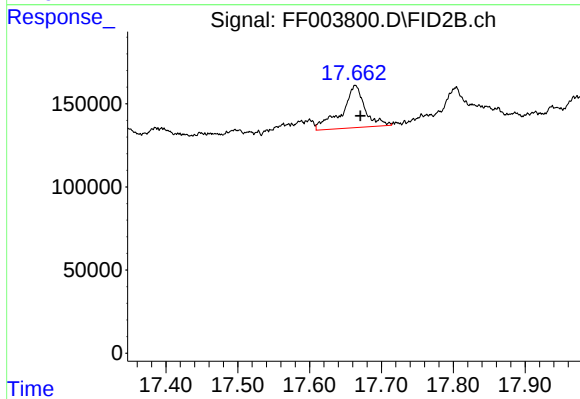

#13 N-TRIACONTANE


R.T.: 17.664 min
Delta R.T.: -0.007 min
Response: 567288
Conc: 3.86 ug/ml

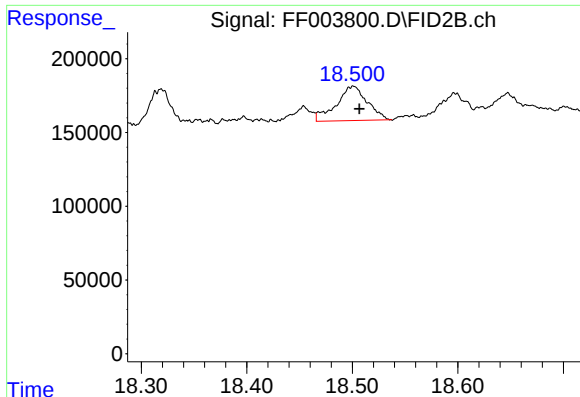

#14 N-DOTRIACONTANE


R.T.: 18.501 min
Delta R.T.: -0.005 min
Response: 474771
Conc: 3.34 ug/ml

Instrument :
FID_F
ClientSampleId :

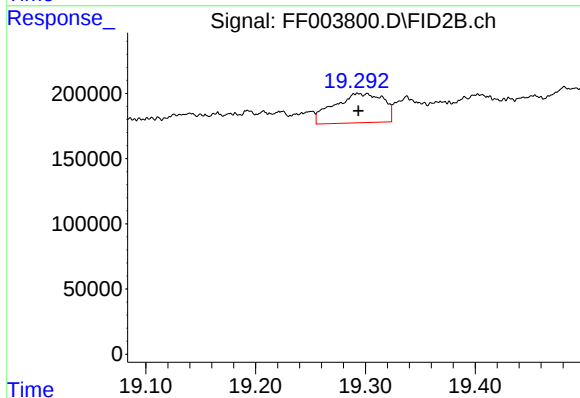


#15 N-TETRATRIACONTANE

R.T.: 19.302 min
Delta R.T.: 0.008 min
Response: 702888
Conc: 5.25 ug/ml

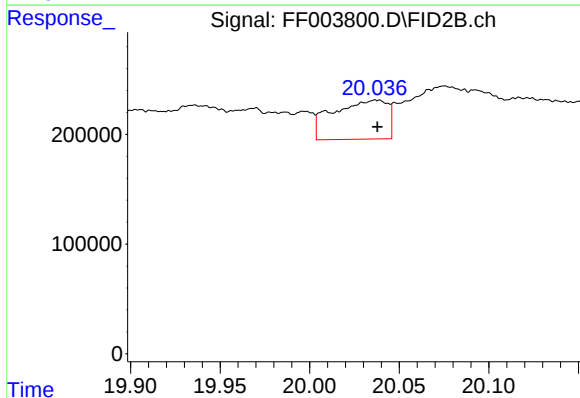


#16 N-HEXATRIACONTANE

R.T.: 20.038 min
Delta R.T.: 0.000 min
Response: 753246
Conc: 5.77 ug/ml

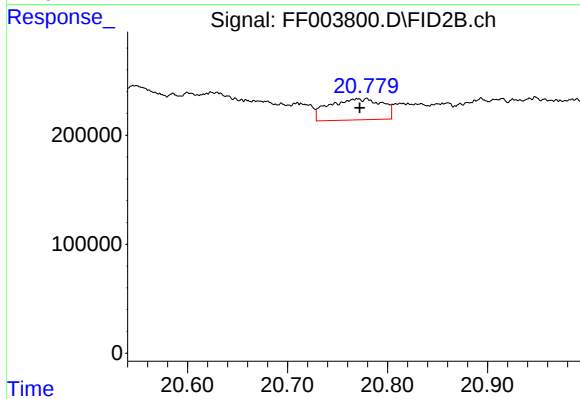

#17 N-OCTATRIACONTANE

R.T.: 20.770 min
Delta R.T.: -0.002 min
Response: 716478
Conc: 6.21 ug/ml

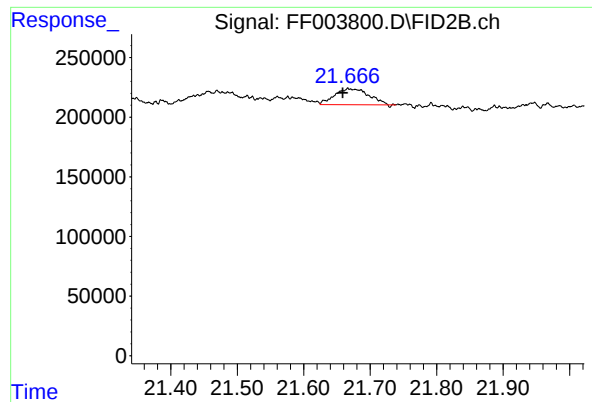

#18 N-TETRACONTANE

R.T.: 21.667 min
Delta R.T.: 0.008 min
Response: 479136
Conc: 3.85 ug/ml

Instrument :
FID_F
ClientSampleId :