

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
 Data File : FF003801.D
 Signal(s) : FID2B.ch
 Acq On : 12 Mar 2019 17:08
 Operator : AJ\SJ
 Sample : K1846-09
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 13 01:00:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.593	1356090	9.740 ug/ml
Target Compounds			
4) N-TETRADECANE	8.194f	238695	1.489 ug/ml
12) N-OCTACOSANE	16.773	174792	1.157 ug/ml
13) N-TRIACONTANE	17.663	278412	1.893 ug/ml
14) N-DOTRIACONTANE	18.497	309964	2.180 ug/ml
15) N-TETRATRIACONTANE	19.287	86165	0.644 ug/ml
16) N-HEXATRIACONTANE	20.077	634826	4.865 ug/ml
18) N-TETRACONTANE	21.689	208663	1.677 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031219\
Data File : FF003801.D
Signal(s) : FID2B.ch
Acq On : 12 Mar 2019 17:08
Operator : AJ\SJ
Sample : K1846-09
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 13 01:00:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

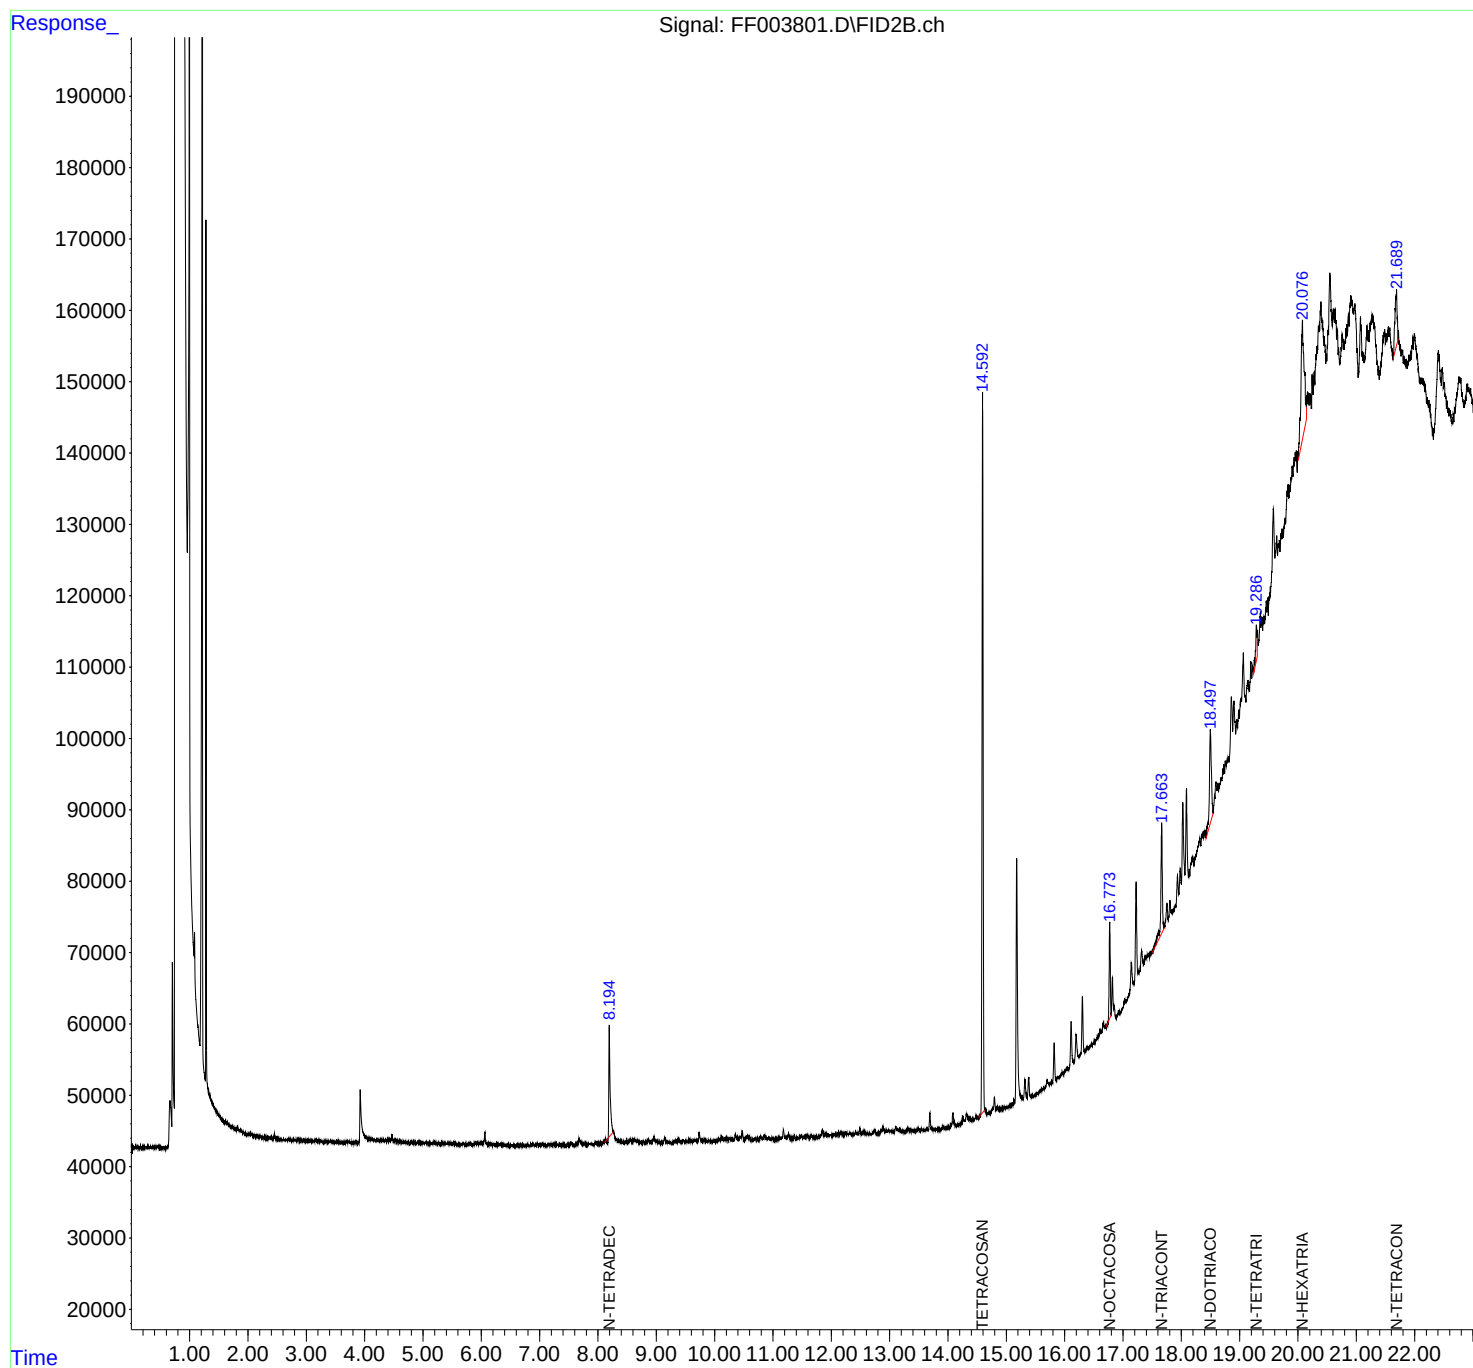


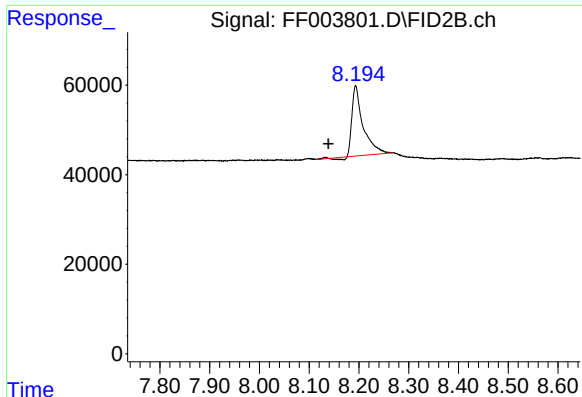

#4 N-TETRADECANE


R.T.: 8.194 min
Delta R.T.: 0.055 min
Response: 238695
Conc: 1.49 ug/ml

Instrument :
FID_F
ClientSampleId :

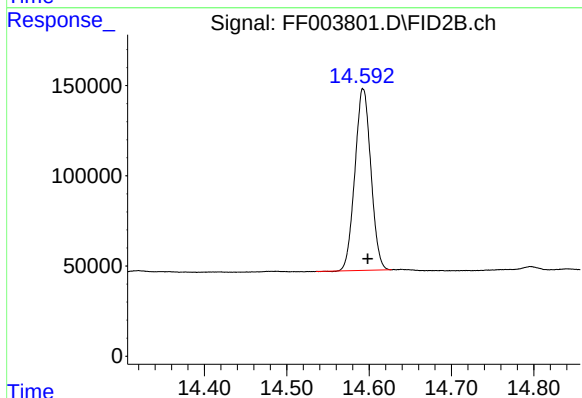


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.593 min
Delta R.T.: -0.005 min
Response: 1356090
Conc: 9.74 ug/ml

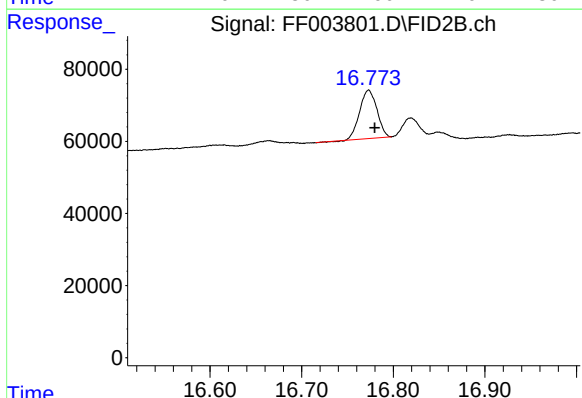


#12 N-OCTACOSANE

R.T.: 16.773 min
Delta R.T.: -0.007 min
Response: 174792
Conc: 1.16 ug/ml

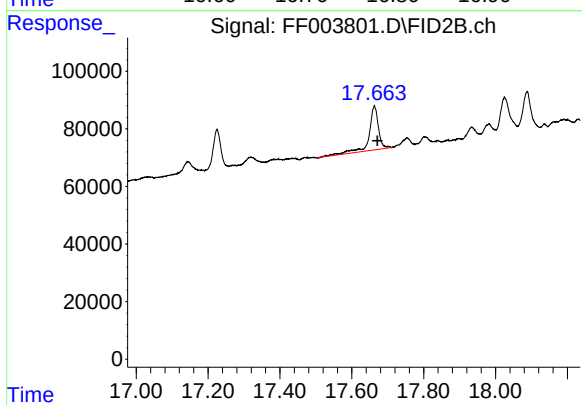

#13 N-TRIACONTANE


R.T.: 17.663 min
Delta R.T.: -0.008 min
Response: 278412
Conc: 1.89 ug/ml

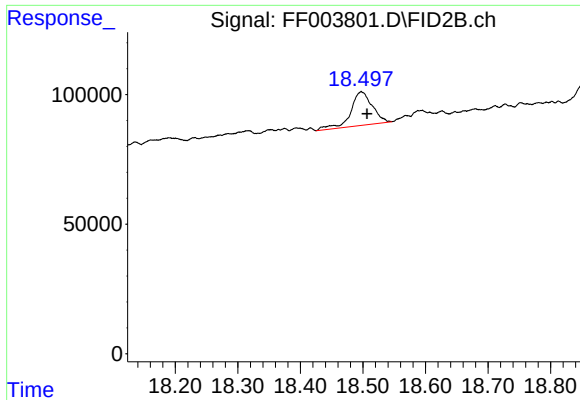

#14 N-DOTRIACONTANE


R.T.: 18.497 min
Delta R.T.: -0.009 min
Response: 309964
Conc: 2.18 ug/ml

Instrument :
FID_F
ClientSampleId :

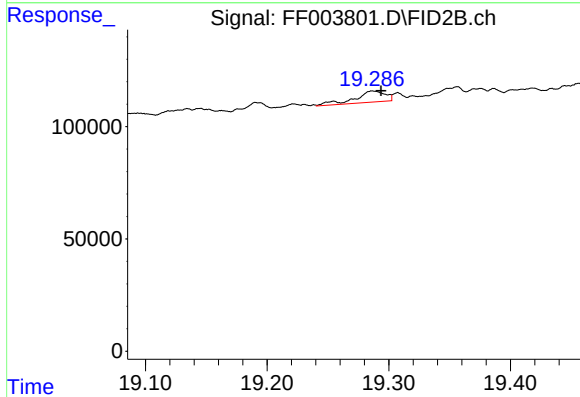


#15 N-TETRATRIACONTANE

R.T.: 19.287 min
Delta R.T.: -0.007 min
Response: 86165
Conc: 0.64 ug/ml

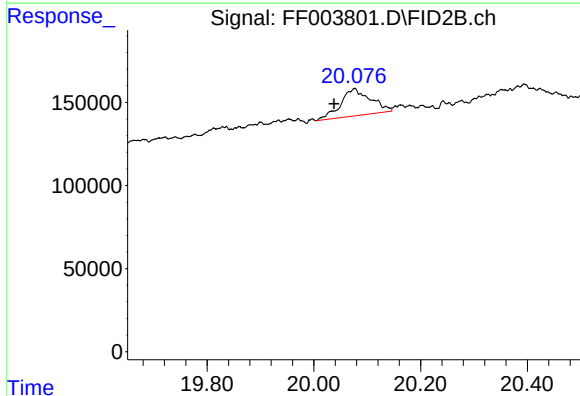

#16 N-HEXATRIACONTANE

R.T.: 20.077 min
Delta R.T.: 0.039 min
Response: 634826
Conc: 4.87 ug/ml

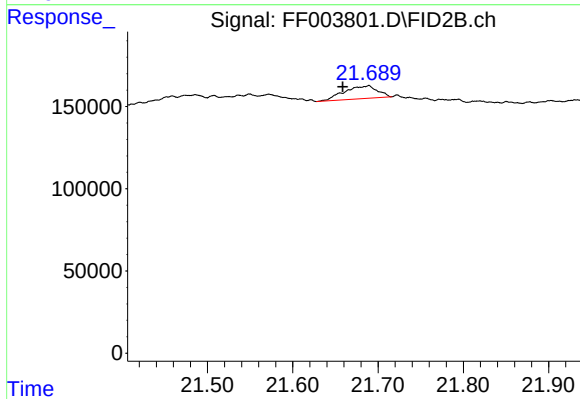

#18 N-TETRACONTANE

R.T.: 21.689 min
Delta R.T.: 0.030 min
Response: 208663
Conc: 1.68 ug/ml